

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050422\
 Data File : BF128062.D
 Acq On : 04 May 2022 10:28
 Operator : CG\JU
 Sample : PB144541BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB144541BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128062.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.551	550	555	558	rBV	3107189	3130470	75.44%	12.716%
2	6.545	718	724	727	rBV	2792522	3244273	78.19%	13.178%
3	6.916	783	787	790	rBV	808386	690791	16.65%	2.806%
4	7.481	877	883	886	rBV	2041059	2238923	53.96%	9.094%
5	8.198	1000	1005	1008	rBV	994046	910093	21.93%	3.697%
6	9.275	1182	1188	1191	rBV	3974291	3967552	95.62%	16.116%
7	9.957	1298	1304	1308	rBV	1230098	1067585	25.73%	4.336%
8	10.751	1432	1439	1443	rBV	2544844	2511280	60.52%	10.200%
9	11.451	1554	1558	1561	rBV	1353728	1098969	26.49%	4.464%
10	13.039	1823	1828	1832	rBV	3938938	4149346	100.00%	16.854%
11	14.098	2004	2008	2011	rBV	1039925	887897	21.40%	3.607%
12	15.604	2259	2264	2272	rVB	542030	722106	17.40%	2.933%




Sum of corrected areas: 24619285

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050422\
Data File : BF128062.D
Acq On : 04 May 2022 10:28
Operator : CG\JU
Sample : PB144541BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB144541BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

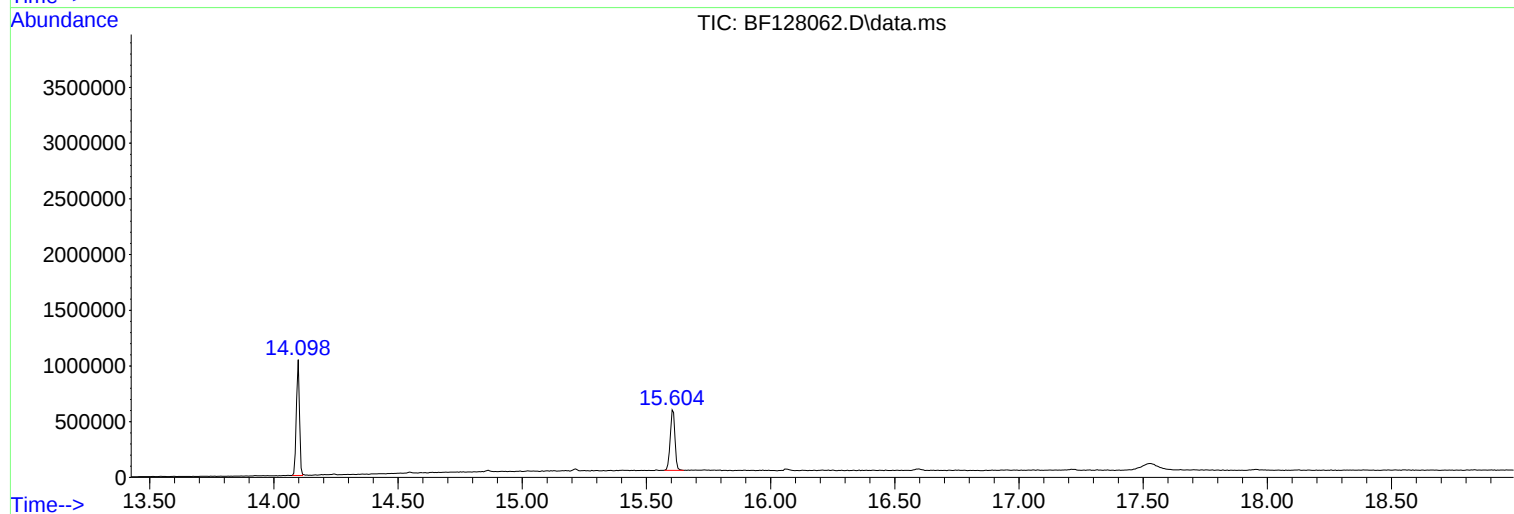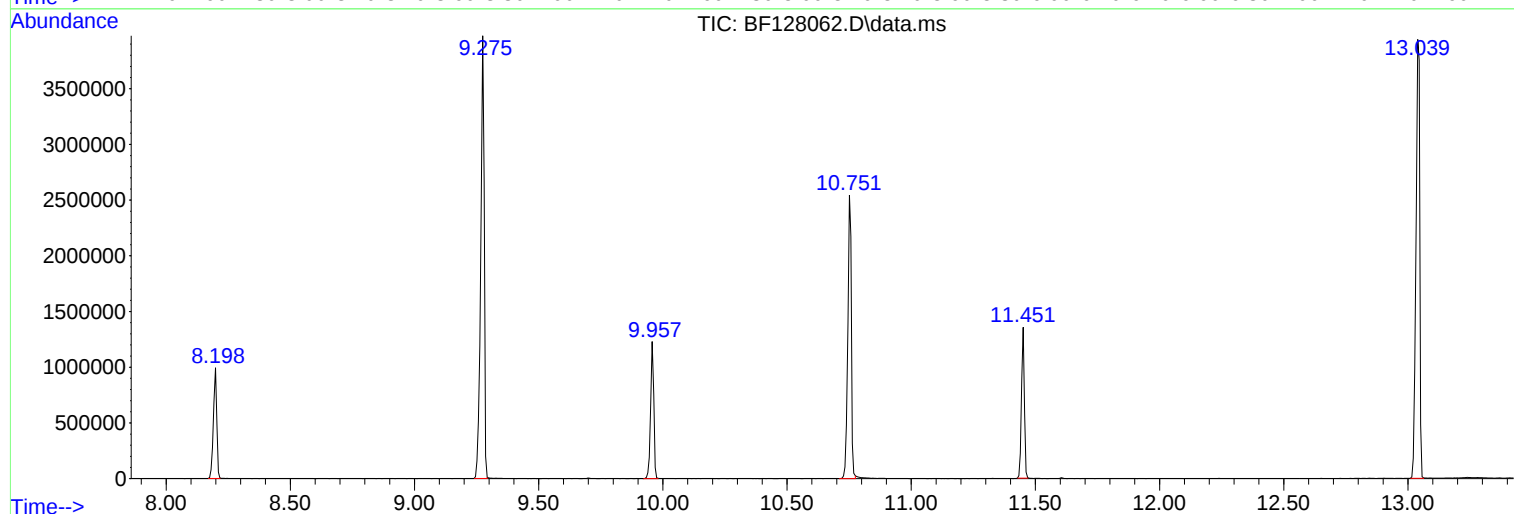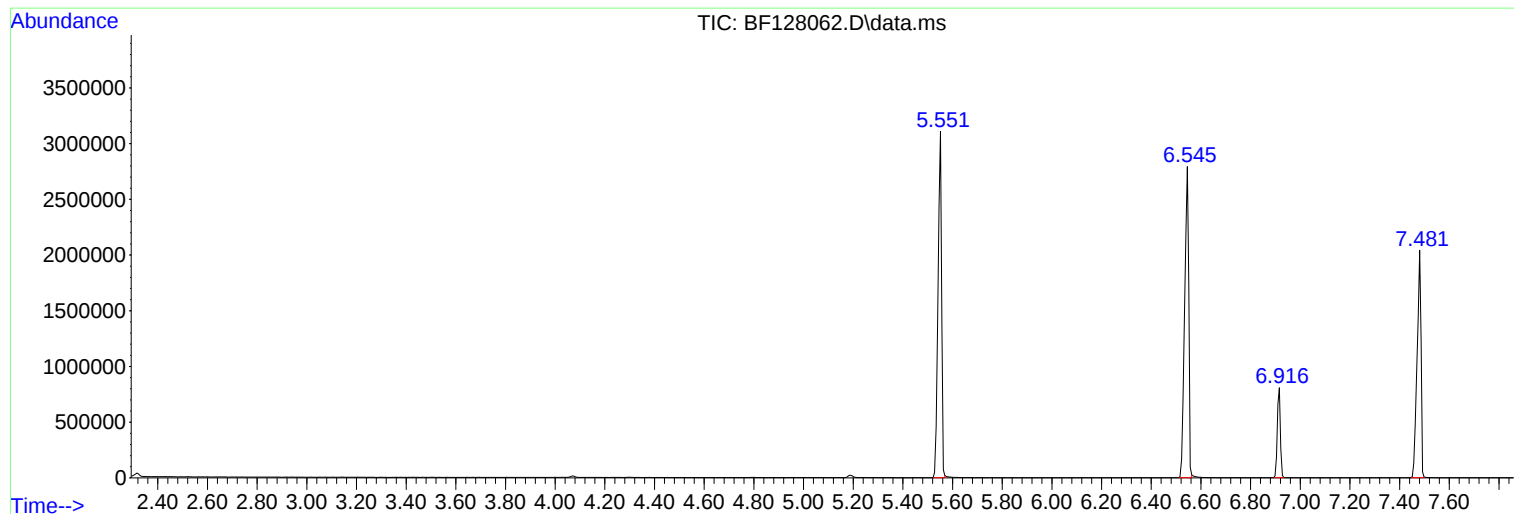

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050422\
Data File : BF128062.D
Acq On : 04 May 2022 10:28
Operator : CG\JU
Sample : PB144541BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB144541BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050422\
Data File : BF128062.D
Acq On : 04 May 2022 10:28
Operator : CG\JU
Sample : PB144541BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB144541BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------