

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050422\
 Data File : BF128072.D
 Acq On : 04 May 2022 15:28
 Operator : CG\JU
 Sample : N2665-05
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-4,6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128072.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.157	484	488	495	rVB	64224	82553	2.65%	0.452%
2	5.539	548	553	556	rBV	2550716	2513228	80.79%	13.762%
3	6.545	718	724	727	rBV	2532380	2635731	84.73%	14.433%
4	6.910	783	786	790	rBV	652161	575081	18.49%	3.149%
5	7.480	877	883	886	rBV	1944759	1803599	57.98%	9.876%
6	8.198	1001	1005	1008	rBV	880574	734721	23.62%	4.023%
7	9.274	1183	1188	1191	rBV	3726001	3110677	100.00%	17.033%
8	9.957	1300	1304	1307	rBV	1013809	816082	26.23%	4.469%
9	10.751	1434	1439	1442	rBV	1948325	1746468	56.14%	9.563%
10	11.445	1554	1557	1561	rBV	767832	710863	22.85%	3.893%
11	13.033	1823	1827	1831	rBV	2341838	2265218	72.82%	12.404%
12	13.945	1975	1982	1992	rBV3	68030	183003	5.88%	1.002%
13	14.098	2004	2008	2011	rBV	619704	570112	18.33%	3.122%
14	15.603	2259	2264	2271	rVB	410992	514853	16.55%	2.819%




Sum of corrected areas: 18262189

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050422\
Data File : BF128072.D
Acq On : 04 May 2022 15:28
Operator : CG\JU
Sample : N2665-05
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-4,6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

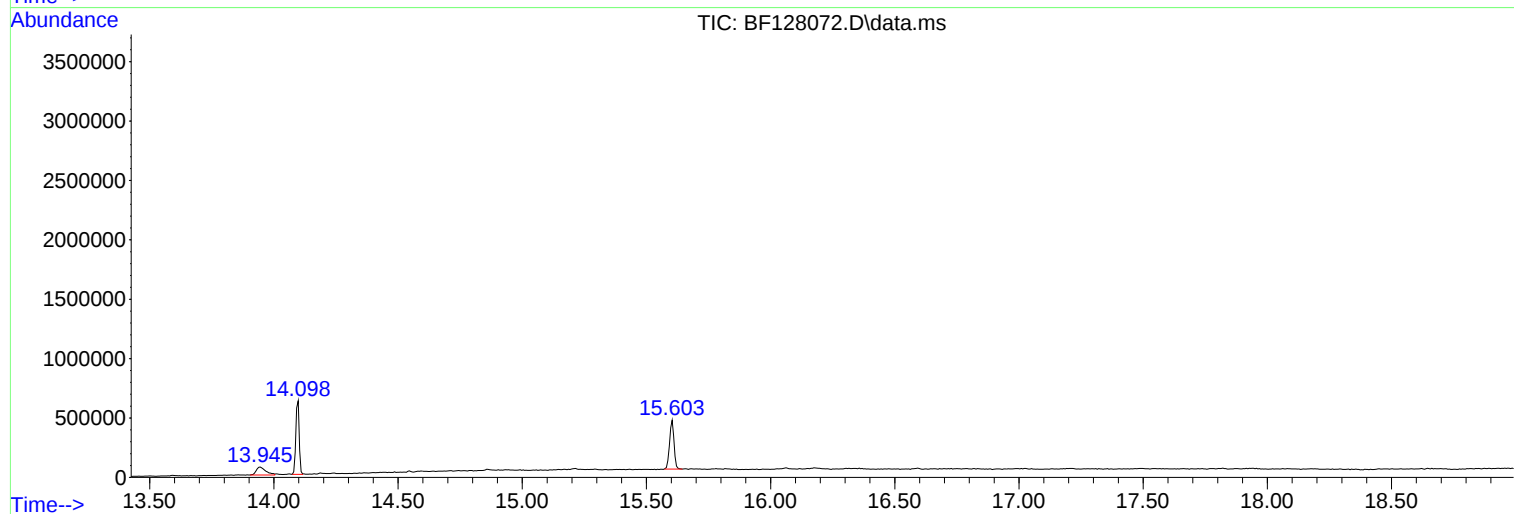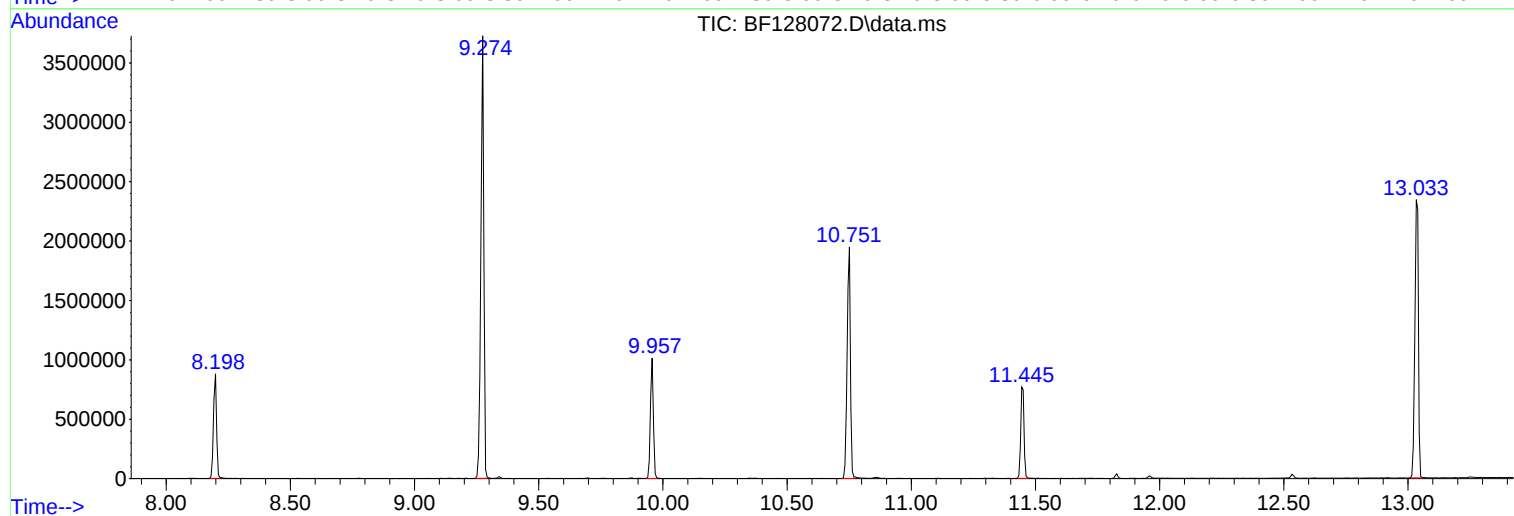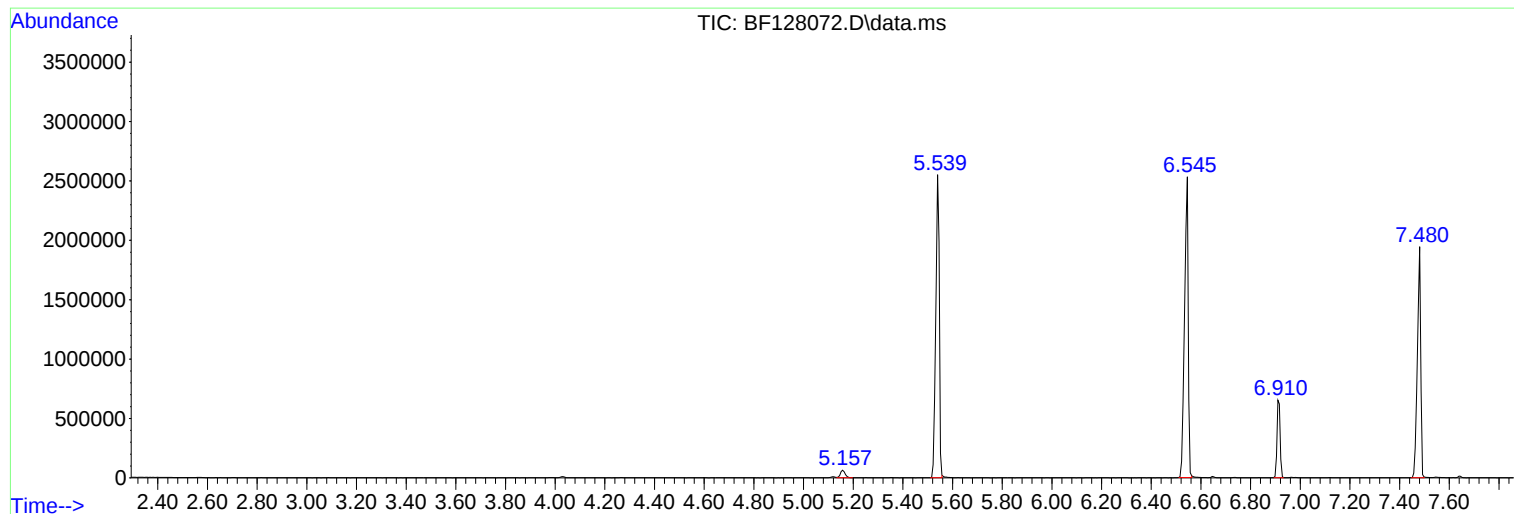

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050422\
Data File : BF128072.D
Acq On : 04 May 2022 15:28
Operator : CG\JU
Sample : N2665-05
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-4,6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050422\
Data File : BF128072.D
Acq On : 04 May 2022 15:28
Operator : CG\JU
Sample : N2665-05
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-4,6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc