

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050422\
 Data File : BF128075.D
 Acq On : 04 May 2022 16:54
 Operator : CG\JU
 Sample : N2665-11
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-10,14

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128075.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.163	486	489	496	rVB	28512	38337	1.11%	0.191%
2	5.540	548	553	556	rBV	2749401	2781324	80.31%	13.849%
3	6.545	718	724	727	rBV	2746256	2925307	84.47%	14.566%
4	6.910	783	786	790	rBV	635308	548004	15.82%	2.729%
5	7.481	877	883	886	rBV	2049200	2016585	58.23%	10.041%
6	8.198	1000	1005	1008	rBV	817370	707960	20.44%	3.525%
7	9.275	1182	1188	1191	rBV	3967452	3463203	100.00%	17.245%
8	9.957	1300	1304	1307	rBV	979546	793599	22.92%	3.952%
9	10.751	1434	1439	1442	rBV	2283010	2070360	59.78%	10.309%
10	11.445	1554	1557	1561	rBV	809214	702332	20.28%	3.497%
11	13.039	1823	1828	1831	rBV	2813326	2684690	77.52%	13.368%
12	13.939	1976	1981	1994	rBV3	100276	269887	7.79%	1.344%
13	14.092	2004	2007	2011	rBV	607652	568568	16.42%	2.831%
14	15.604	2259	2264	2271	rVB	395275	512775	14.81%	2.553%




Sum of corrected areas: 20082931

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050422\
Data File : BF128075.D
Acq On : 04 May 2022 16:54
Operator : CG\JU
Sample : N2665-11
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-10,14

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

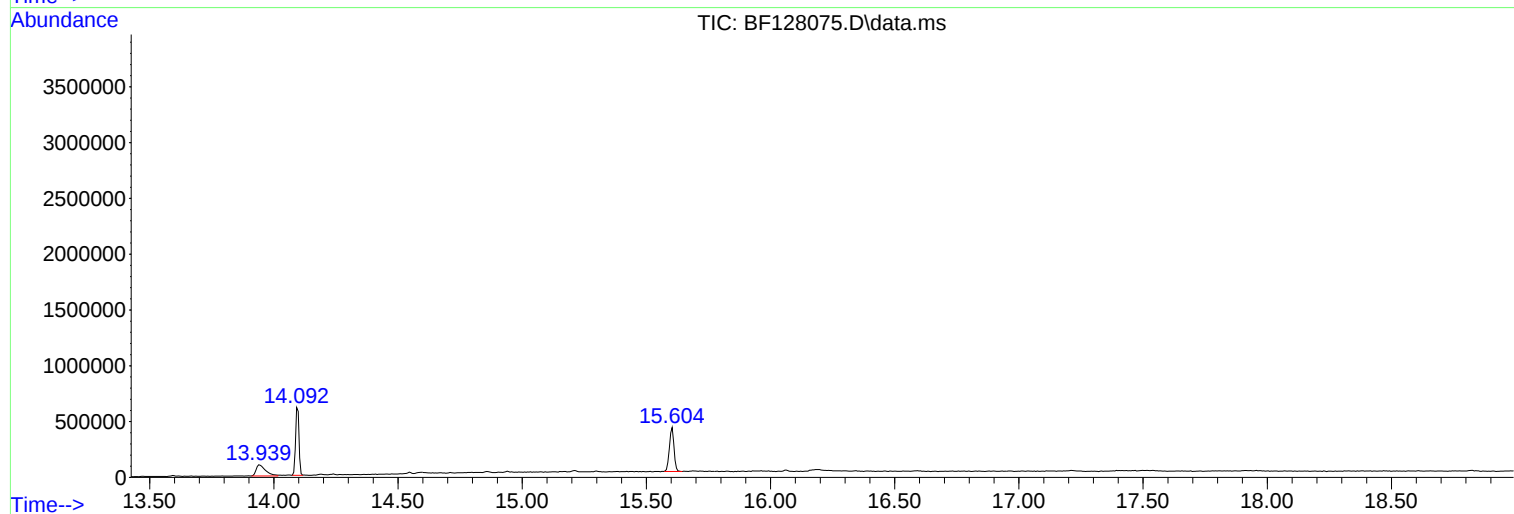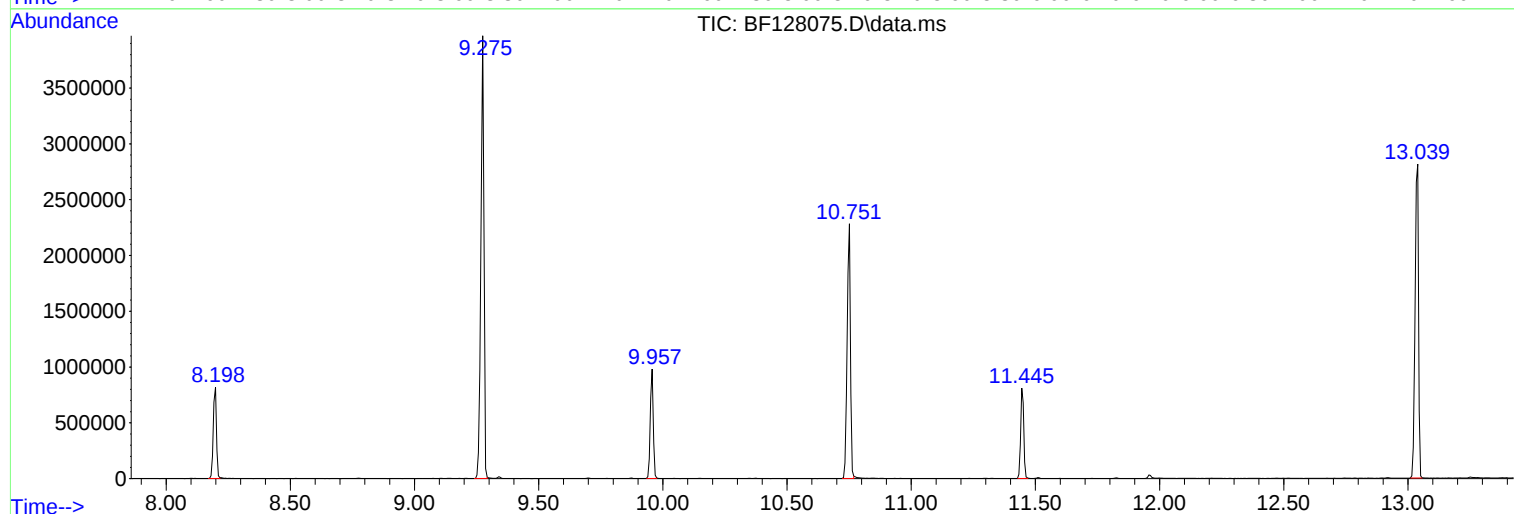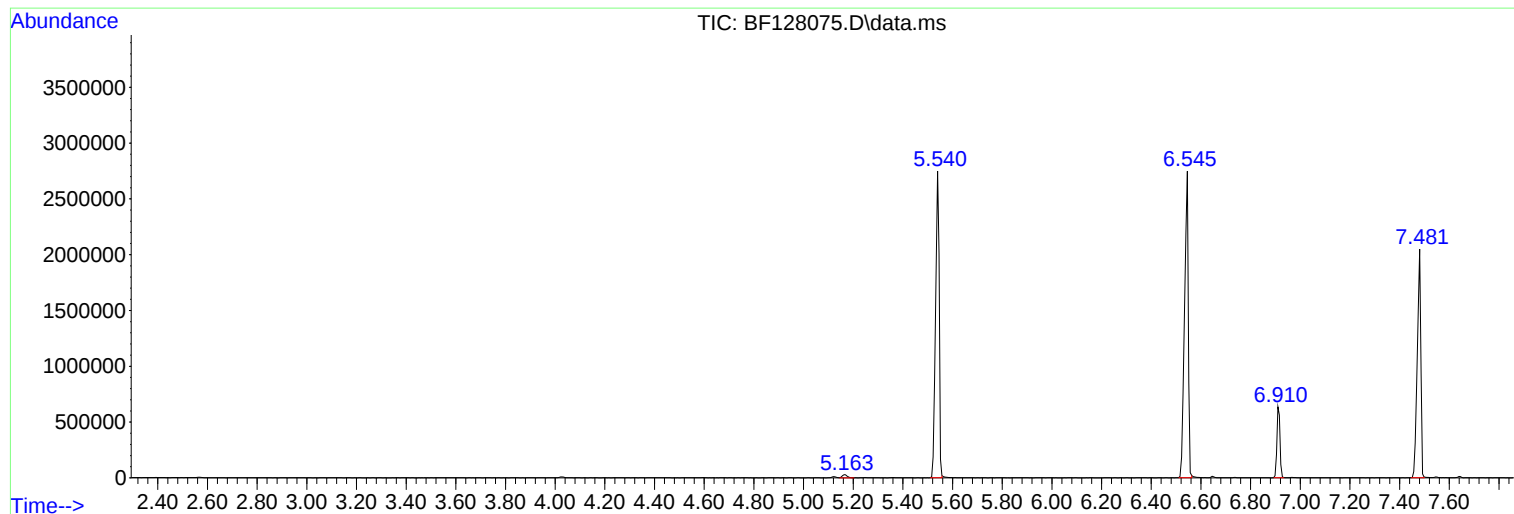

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050422\
Data File : BF128075.D
Acq On : 04 May 2022 16:54
Operator : CG\JU
Sample : N2665-11
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-10,14










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 n-Nonadecanol-1 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.939	9.49 ng	269887	Chrysene-d12	14.092

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		n-Nonadecanol-1	284	C19H40O	001454-84-8	95
2		Behenic alcohol	326	C22H46O	000661-19-8	95
3		Carbonic acid, octadecyl 2,2,2-t...	444	C21H39Cl3O3	1000314-56-3	94
4		Bromoacetic acid, hexadecyl ester	362	C18H35BrO2	005454-48-8	94
5		Heptafluorobutyric acid, pentade...	424	C19H31F7O2	959261-23-5	93

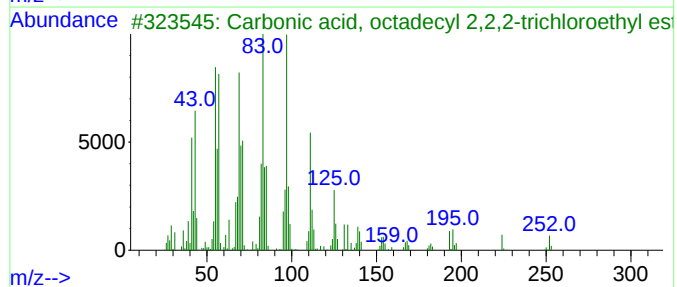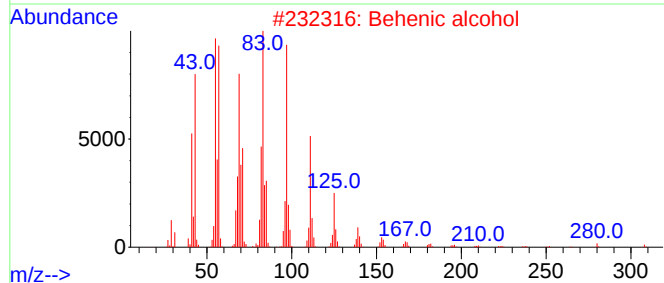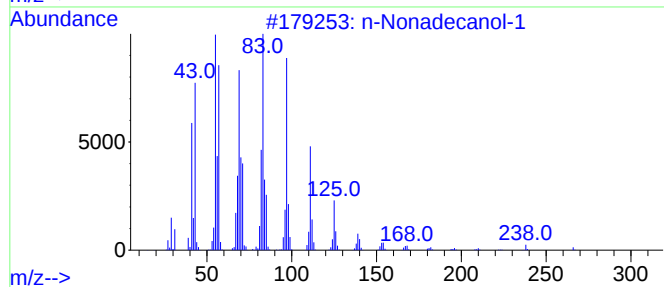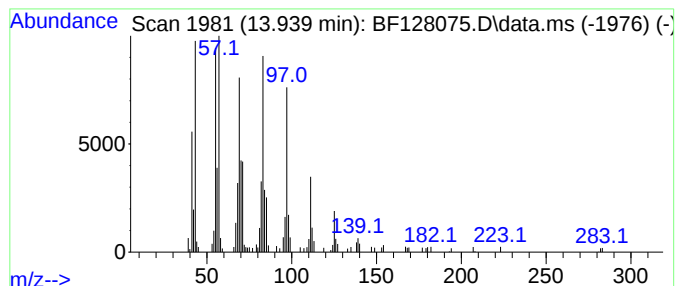

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050422\
Data File : BF128075.D
Acq On : 04 May 2022 16:54
Operator : CG\JU
Sample : N2665-11
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-10,14

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
n-Nonadecanol-1	13.939	9.5	ng	269887	5	14.092	568568	20.0