

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050422\
 Data File : BF128077.D
 Acq On : 04 May 2022 17:51
 Operator : CG\JU
 Sample : N2665-13
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-9,12

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128077.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.481	200	203	214	rBV	18456	39300	1.61%	0.265%
2	5.151	482	487	491	rVB2	20505	30598	1.25%	0.206%
3	5.540	548	553	556	rVB	1956226	1950948	79.93%	13.143%
4	5.816	595	600	603	rBV	37410	30707	1.26%	0.207%
5	6.540	718	723	726	rBV	2138510	2064773	84.60%	13.909%
6	6.910	783	786	790	rBV	650474	555565	22.76%	3.743%
7	7.475	877	882	885	rBV	1393243	1397890	57.27%	9.417%
8	8.198	1001	1005	1008	rBV	800548	717002	29.38%	4.830%
9	9.275	1183	1188	1191	rBV	2811317	2440763	100.00%	16.442%
10	9.957	1300	1304	1307	rBV	902026	769127	31.51%	5.181%
11	10.745	1434	1438	1452	rBV	1486446	1318227	54.01%	8.880%
12	11.445	1554	1557	1561	rBV	762856	652689	26.74%	4.397%
13	13.033	1823	1827	1830	rBV	2088873	1723528	70.61%	11.611%
14	13.945	1975	1982	1992	rBV5	47909	130687	5.35%	0.880%
15	14.092	2003	2007	2011	rBV	599803	530377	21.73%	3.573%
16	15.604	2259	2264	2269	rVB	379284	492329	20.17%	3.317%




Sum of corrected areas: 14844510

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050422\
Data File : BF128077.D
Acq On : 04 May 2022 17:51
Operator : CG\JU
Sample : N2665-13
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-9,12

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

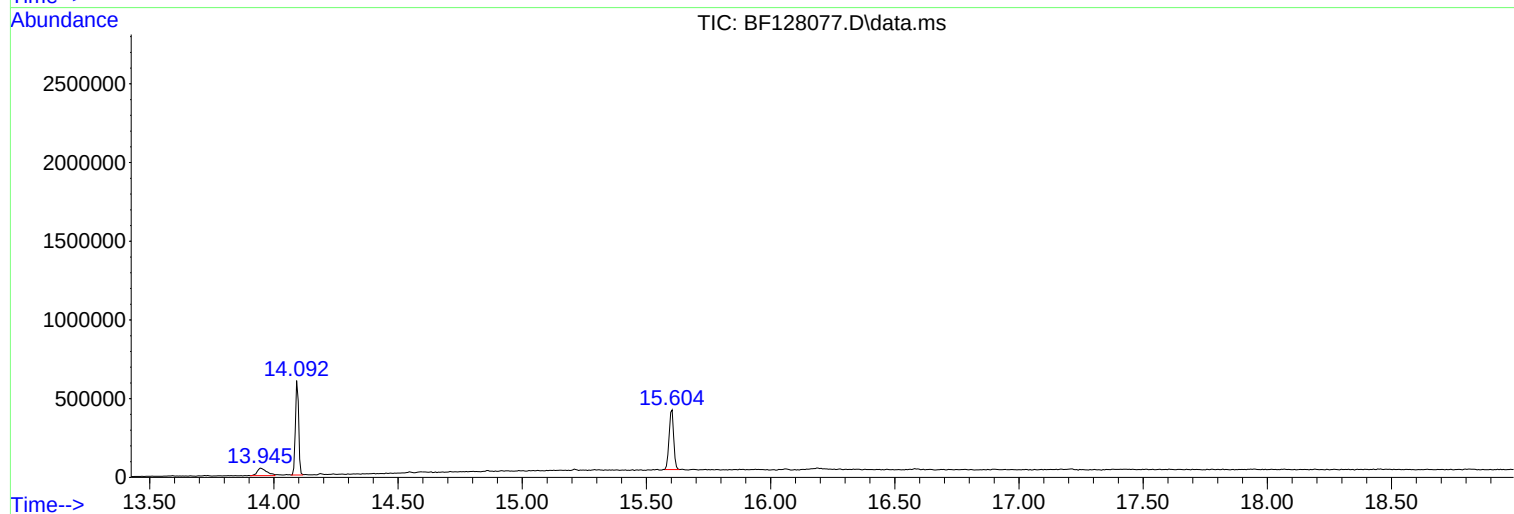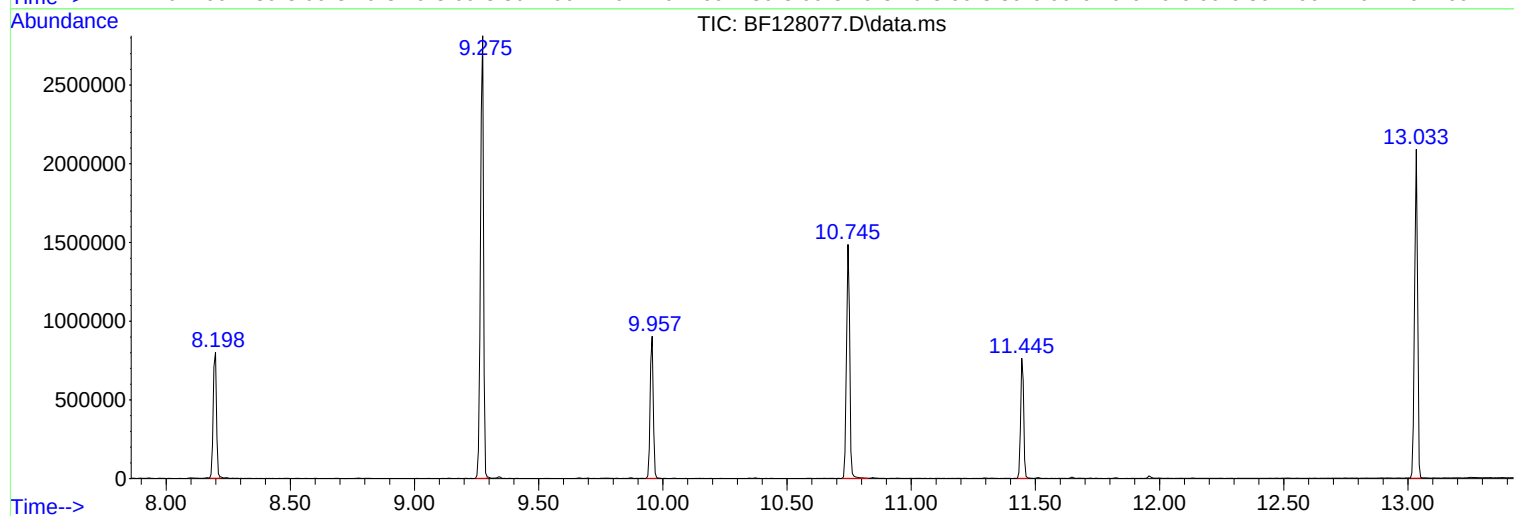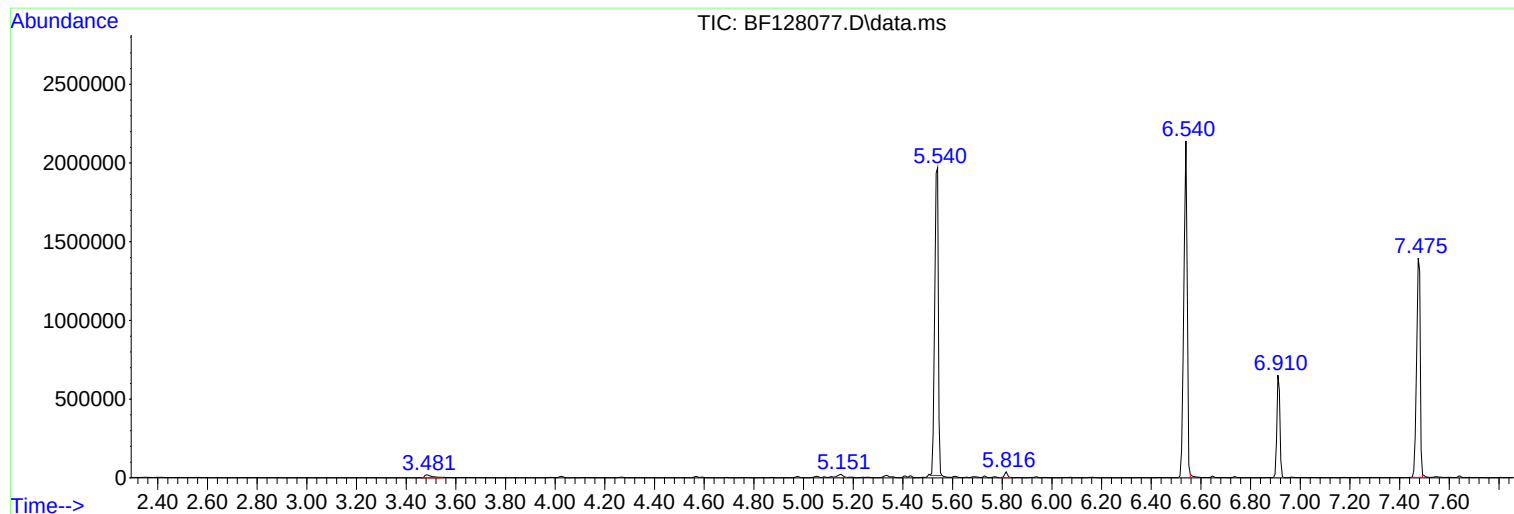

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050422\
Data File : BF128077.D
Acq On : 04 May 2022 17:51
Operator : CG\JU
Sample : N2665-13
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-9,12










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Cyclopentadecane Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.945	4.93 ng	130687	Chrysene-d12	14.092

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclopentadecane	210	C15H30	000295-48-7	97
2			Bromoacetic acid, pentadecyl ester	348	C17H33BrO2	131143-01-6	93
3			1-Docosene	308	C22H44	001599-67-3	91
4			1-Nonadecene	266	C19H38	018435-45-5	91
5			Behenic alcohol	326	C22H46O	000661-19-8	90

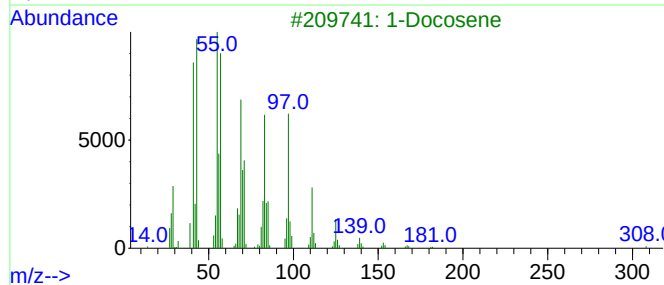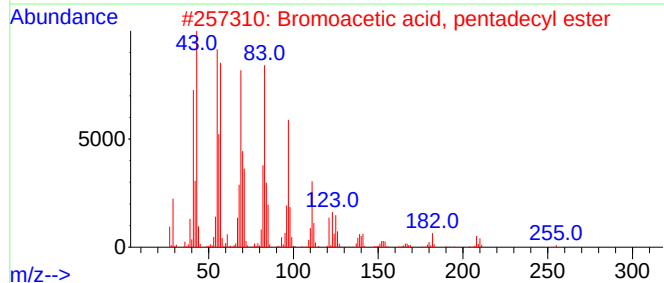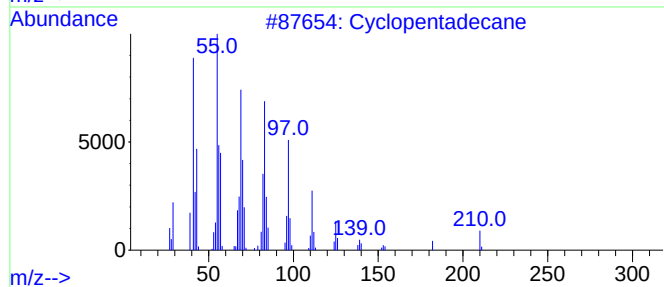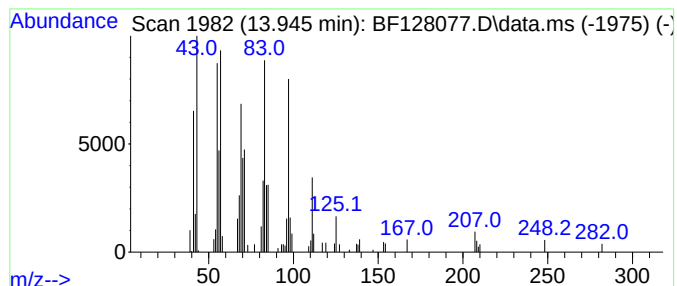

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050422\
Data File : BF128077.D
Acq On : 04 May 2022 17:51
Operator : CG\JU
Sample : N2665-13
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-9,12

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Cyclopentadecane	13.945	4.9	ng	130687	5	14.092	530377	20.0