

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050422\
 Data File : BF128082.D
 Acq On : 04 May 2022 20:16
 Operator : CG\JU
 Sample : N2675-01 2X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 BU-1-050322

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128082.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.010	288	293	297	rVB2	9291	11293	1.33%	0.143%
2	5.528	547	551	567	rBV	905051	795386	93.43%	10.039%
3	6.534	718	722	737	rBV	922818	806452	94.73%	10.179%
4	6.910	783	786	790	rBV	650828	585046	68.72%	7.384%
5	7.475	878	882	885	rBV	655413	520008	61.08%	6.564%
6	8.198	1001	1005	1008	rBV	871565	702339	82.50%	8.865%
7	9.269	1183	1187	1195	rBV	1066896	851319	100.00%	10.745%
8	9.957	1300	1304	1307	rBV	840619	677864	79.63%	8.556%
9	10.745	1434	1438	1450	rBV	523180	437511	51.39%	5.522%
10	11.451	1554	1558	1561	rBV	688035	626983	73.65%	7.914%
11	11.957	1641	1644	1652	rBV6	29438	41555	4.88%	0.525%
12	12.516	1737	1739	1741	rBV2	15515	13796	1.62%	0.174%
13	12.663	1761	1764	1768	rBV	51490	47598	5.59%	0.601%
14	12.898	1798	1804	1806	rBV	63160	78191	9.18%	0.987%
15	13.033	1823	1827	1830	rBV	911284	739240	86.83%	9.331%
16	14.098	2004	2008	2011	rBV	633750	577583	67.85%	7.290%
17	15.604	2260	2264	2272	rVB	311900	410470	48.22%	5.181%


Sum of corrected areas: 7922634

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050422\
Data File : BF128082.D
Acq On : 04 May 2022 20:16
Operator : CG\JU
Sample : N2675-01 2X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
BU-1-050322

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

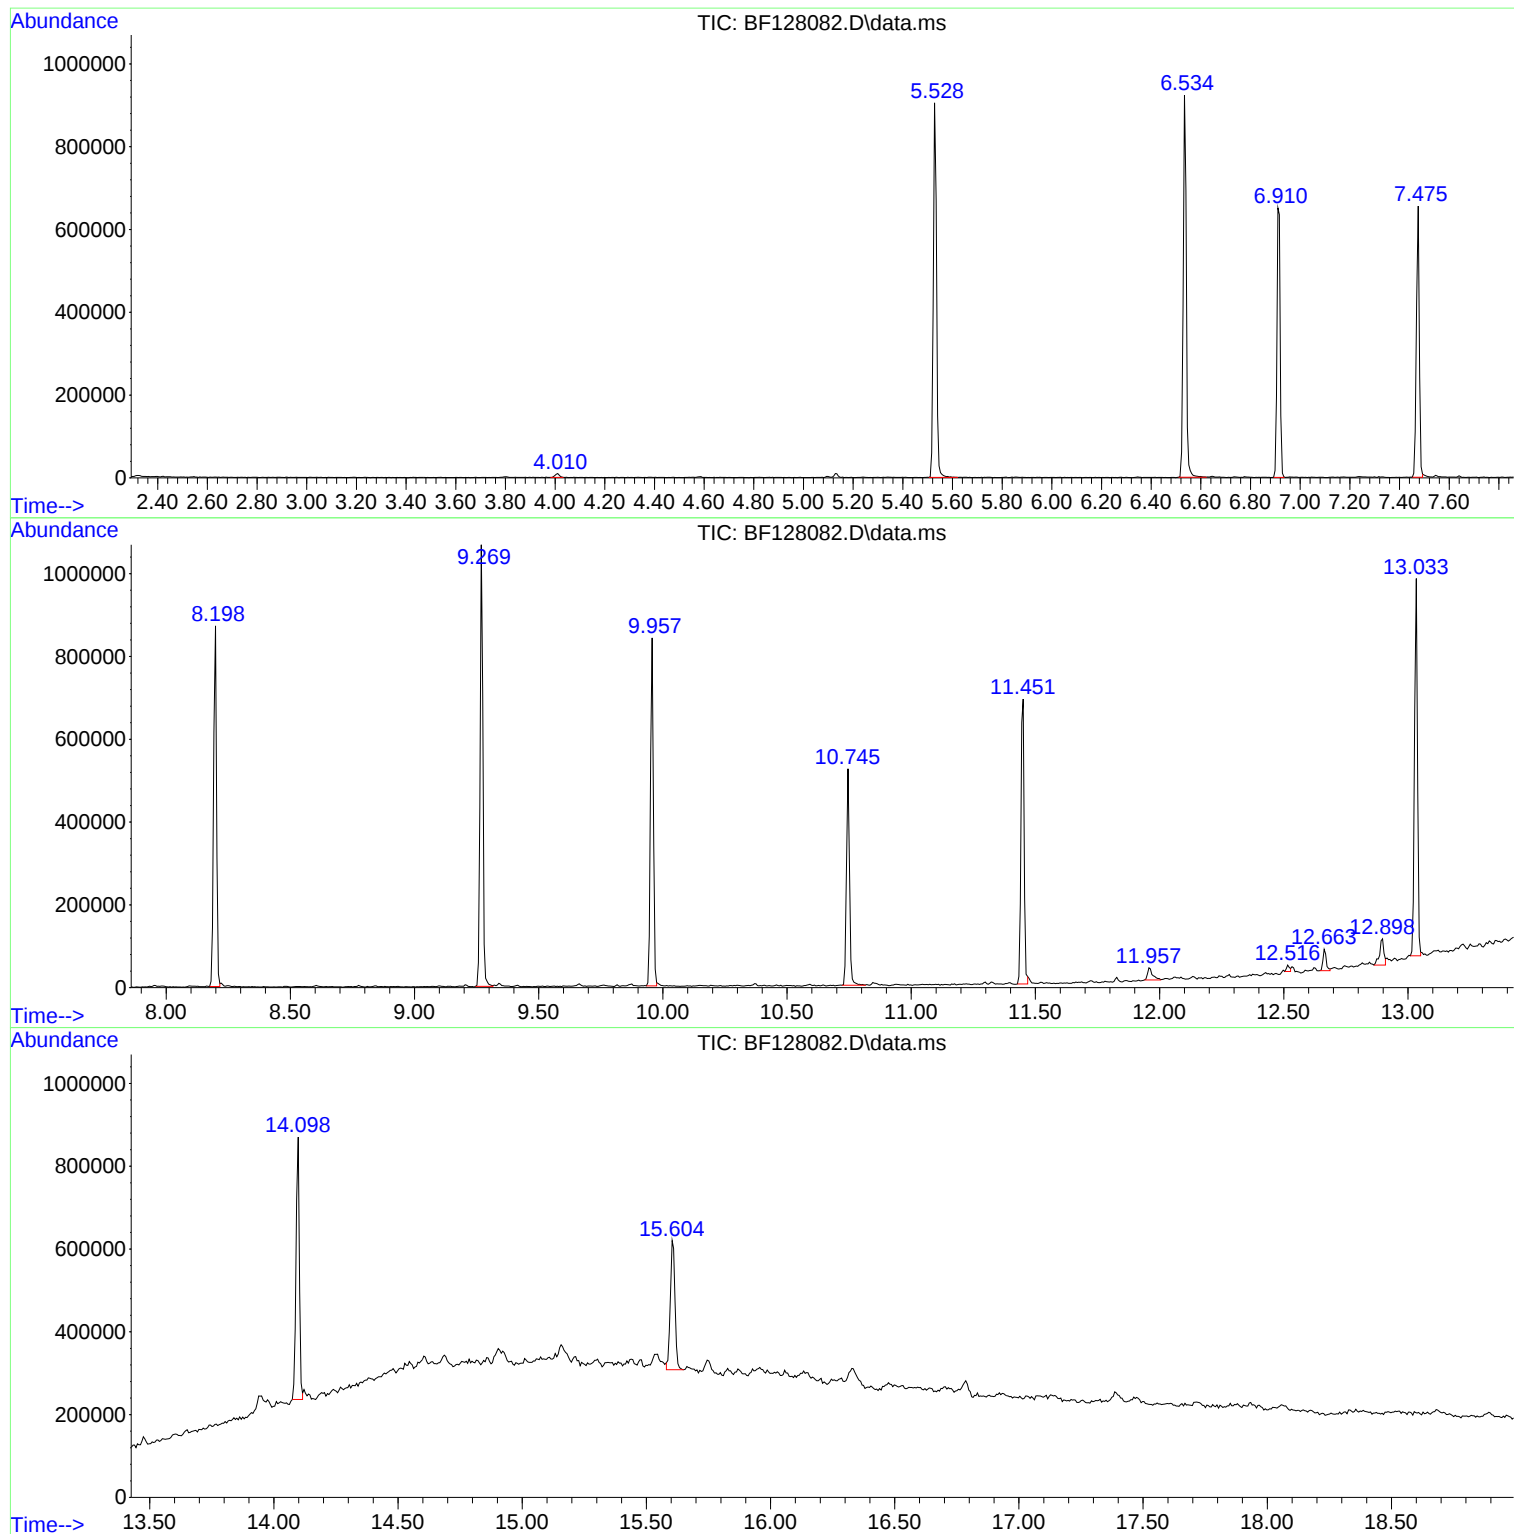

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050422\
Data File : BF128082.D
Acq On : 04 May 2022 20:16
Operator : CG\JU
Sample : N2675-01 2X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
BU-1-050322

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050422\
Data File : BF128082.D
Acq On : 04 May 2022 20:16
Operator : CG\JU
Sample : N2675-01 2X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
BU-1-050322

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------