
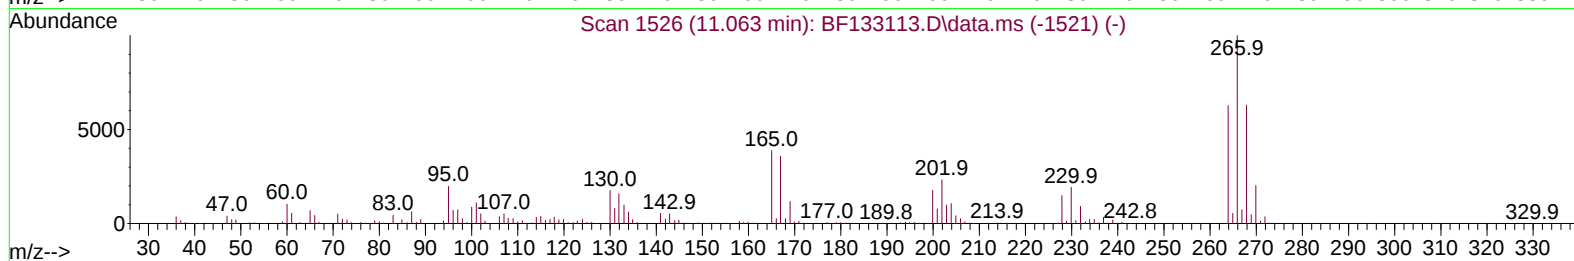
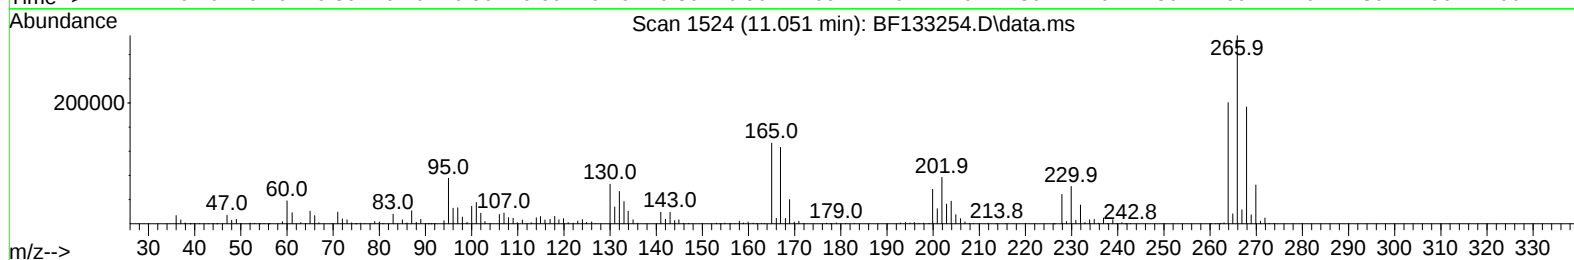


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050523\
 Data File : BF133254.D
 Acq On : 05 May 2023 09:20
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 08 05:22:47 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 05 10:49:34 2023
 Response via : Initial Calibration

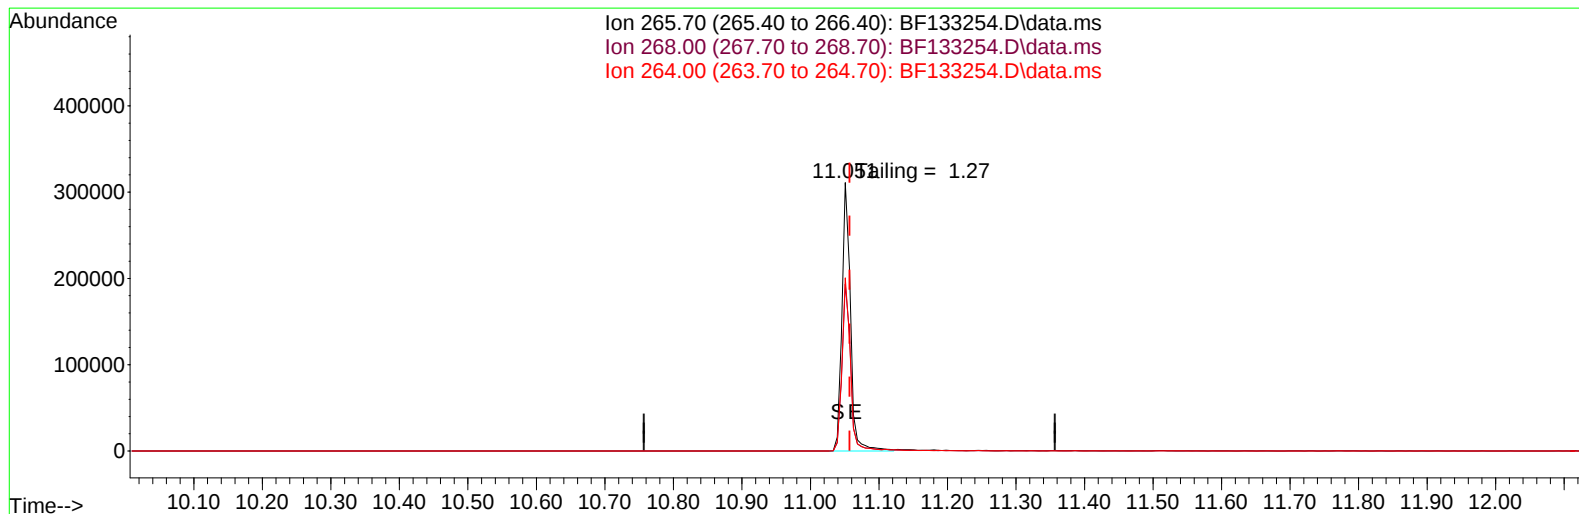

TIC: BF133254.D\data.ms

(70) Pentachlorophenol (C)




11.051min (-0.006) 151645.50 ng

response 267656

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.00	62.12
264.00	63.30	64.49
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050523\
Data File : BF133254.D
Acq On : 05 May 2023 09:20
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 08 05:22:47 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 05 10:49:34 2023
Response via : Initial Calibration

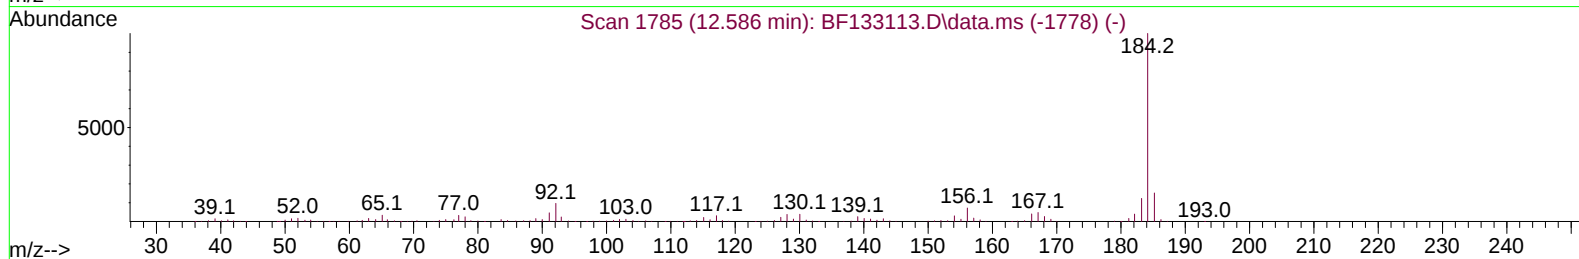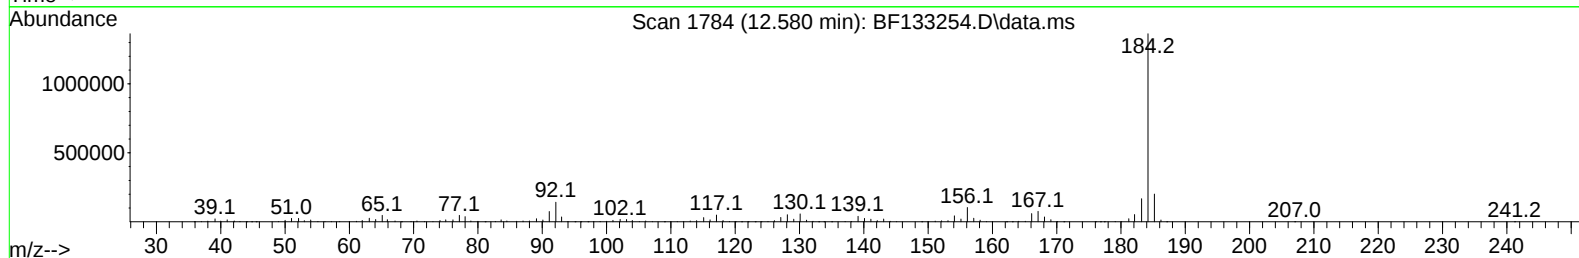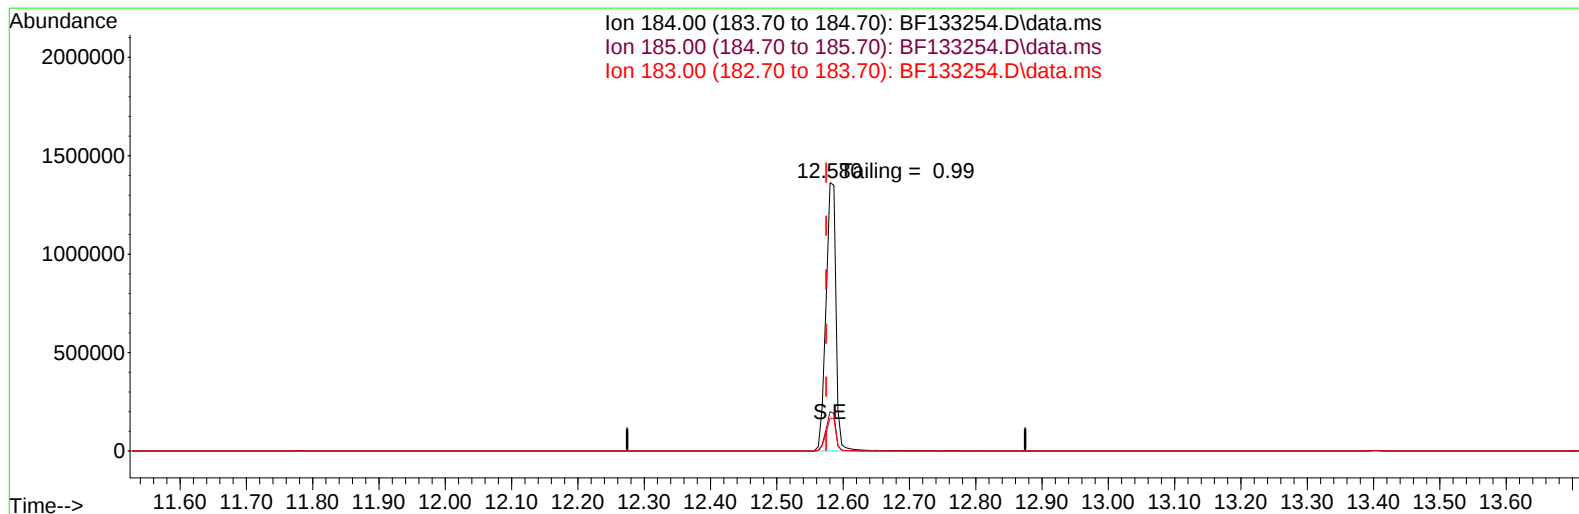

TIC: BF133254.D\data.ms

(77) Benzidine

12.580min (+ 0.006) 239898.49 ng

response 1427997

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	19.30	14.70#
183.00	11.70	12.27
0.00	0.00	0.00