
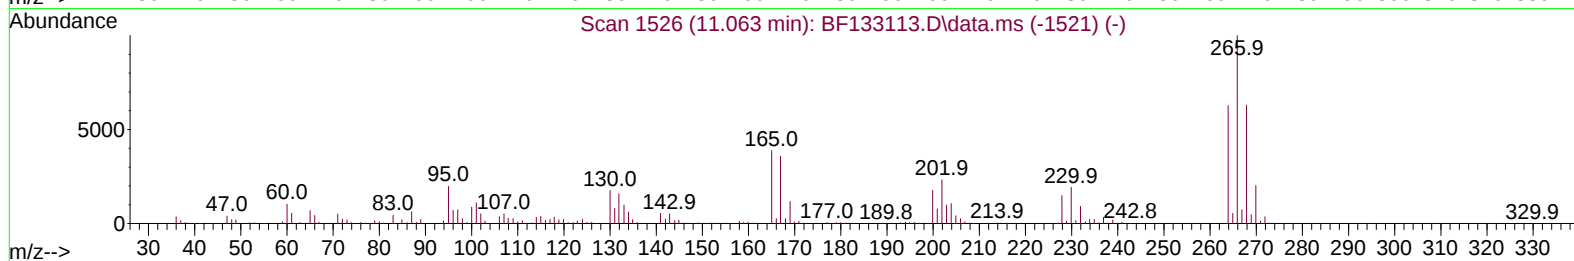
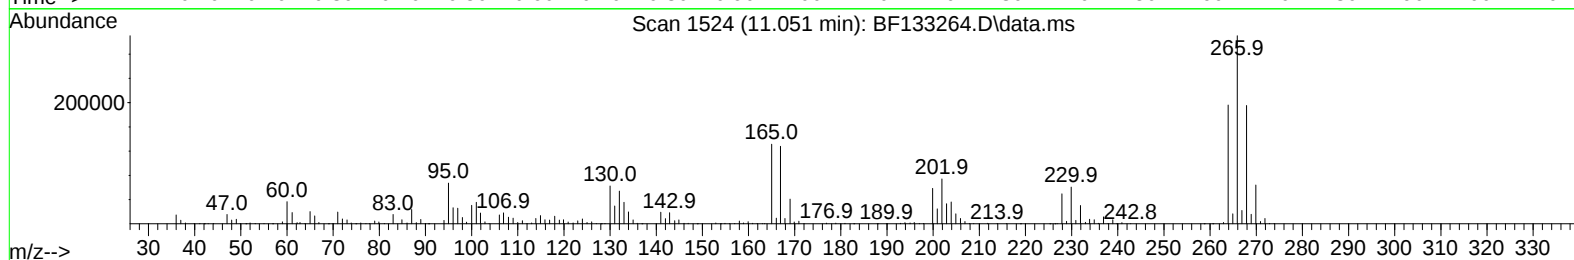


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050523\
Data File : BF133264.D
Acq On : 05 May 2023 15:04
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 08 05:24:05 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 05 10:49:34 2023
Response via : Initial Calibration

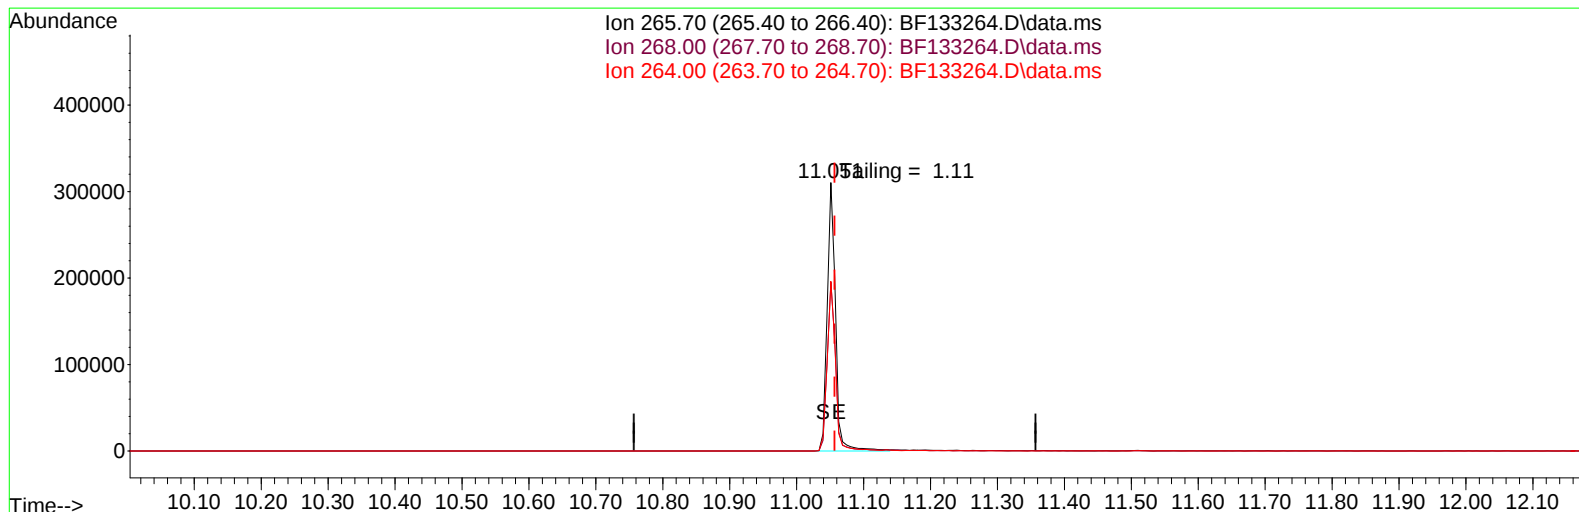

TIC: BF133264.D\data.ms

(70) Pentachlorophenol (C)




11.051min (-0.006) 95326.46 ng

response 271618

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.00	62.90
264.00	63.30	63.19
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050523\
Data File : BF133264.D
Acq On : 05 May 2023 15:04
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 08 05:24:05 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 05 10:49:34 2023
Response via : Initial Calibration

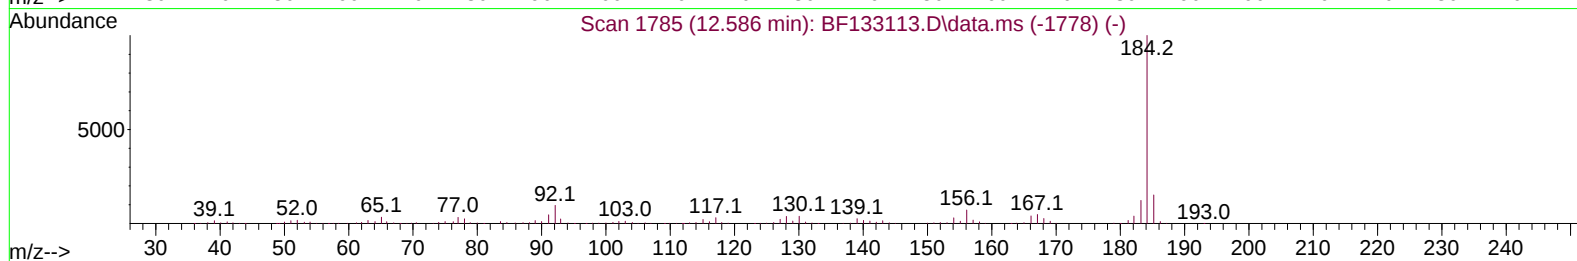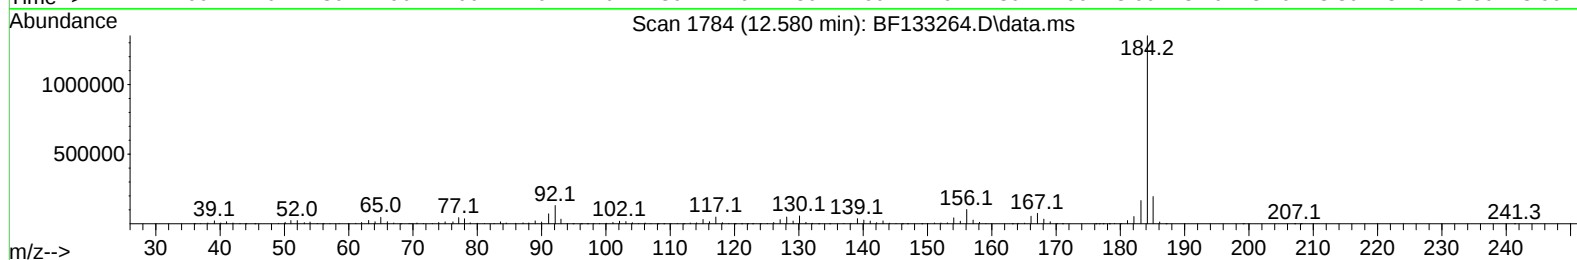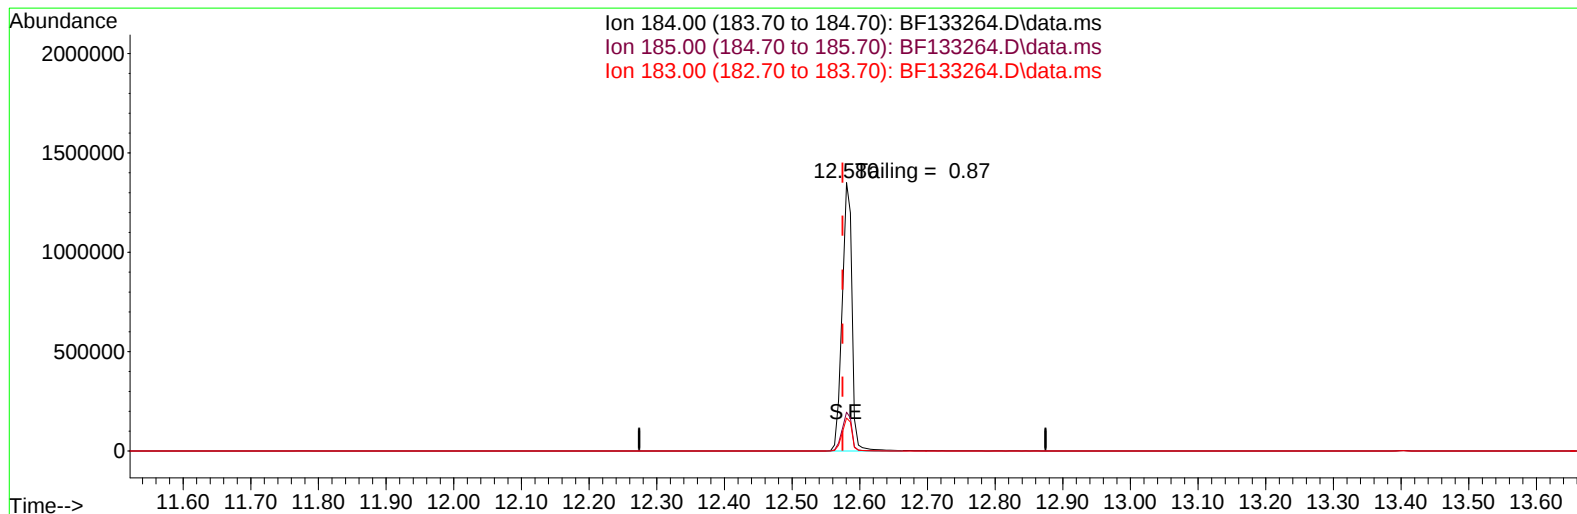

TIC: BF133264.D\data.ms

(77) Benzidine

12.580min (+ 0.006) 168381.59 ng

response 1372457

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	19.30	14.52#
183.00	11.70	12.32
0.00	0.00	0.00