

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050523\
 Data File : BF133269.D
 Acq On : 05 May 2023 18:15
 Operator : CG\JU
 Sample : 02597-08
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 EB-20230503

Quant Time: May 06 05:50:30 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 05 10:49:34 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.722	152	201572	20.000	ng	0.00
21) Naphthalene-d8	8.010	136	807706	20.000	ng	0.00
39) Acenaphthene-d10	9.763	164	430414	20.000	ng	0.00
64) Phenanthrene-d10	11.239	188	783794	20.000	ng	0.00
76) Chrysene-d12	13.874	240	597563	20.000	ng	0.00
86) Perylene-d12	15.292	264	590304	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.334	112	644593	48.307	ng	0.00
7) Phenol-d6	6.357	99	465509	28.106	ng	-0.01
23) Nitrobenzene-d5	7.292	82	1216691	81.308	ng	0.00
42) 2,4,6-Tribromophenol	10.551	330	494487	114.236	ng	0.00
45) 2-Fluorobiphenyl	9.086	172	1986776	77.225	ng	0.00
79) Terphenyl-d14	12.833	244	2361338	68.152	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050523\
Data File : BF133269.D
Acq On : 05 May 2023 18:15
Operator : CG\JU
Sample : 02597-08
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
EB-20230503

Quant Time: May 06 05:50:30 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 05 10:49:34 2023
Response via : Initial Calibration




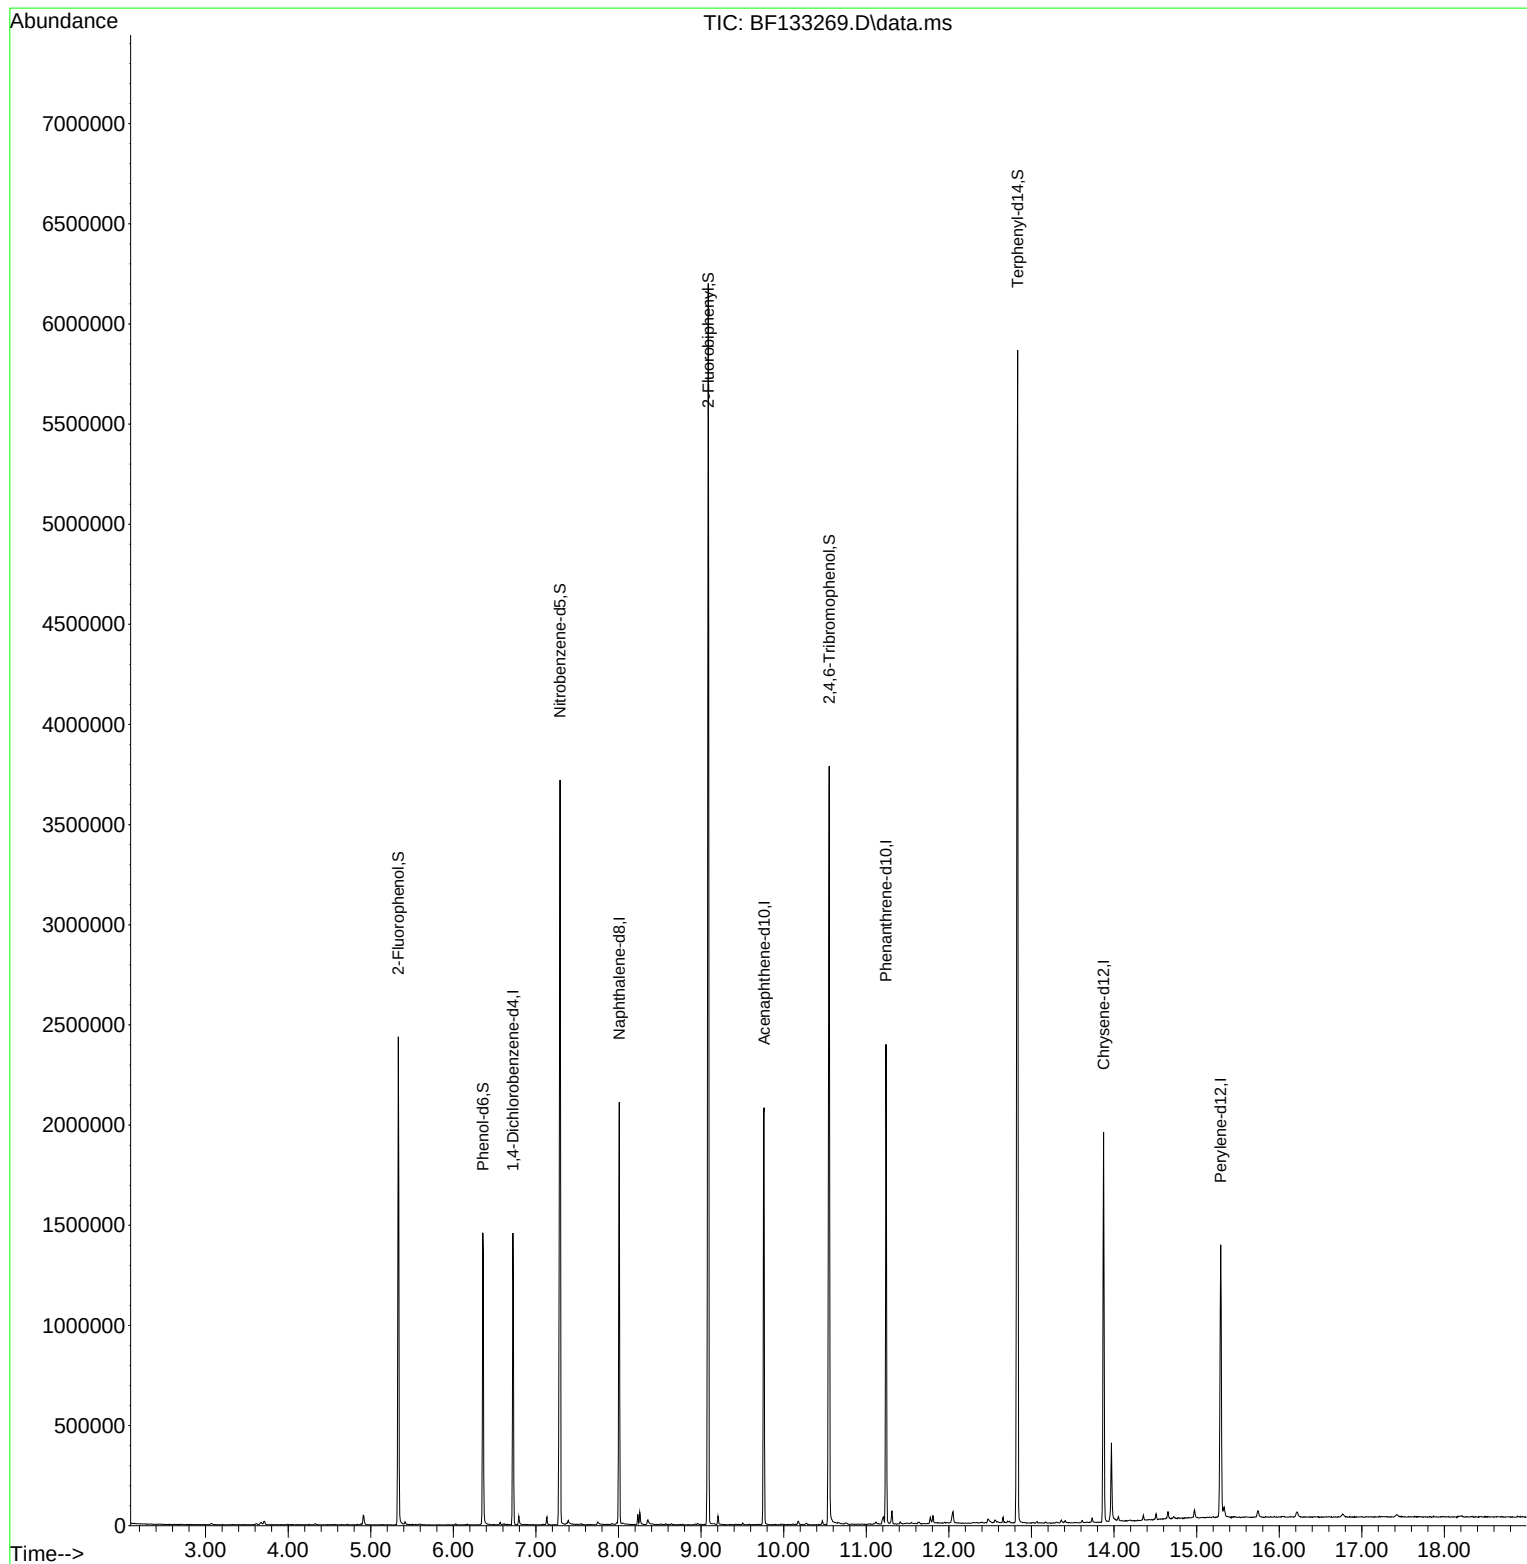




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.722 min Scan# 71
Delta R.T. -0.006 min
Lab File: BF133269.D
Acq: 05 May 2023 18:15




Instrument :
BNA_F
ClientSampleId :
EB-20230503


Tgt Ion:152 Resp: 201572
Ion Ratio Lower Upper
152 100
150 157.8 124.8 187.2
115 62.9 49.9 74.9

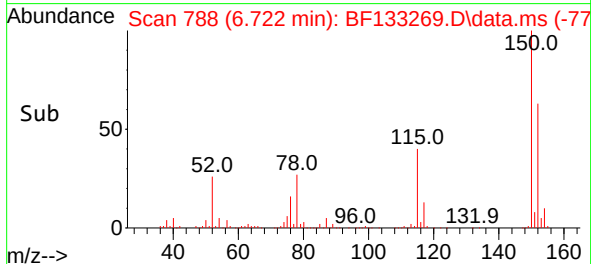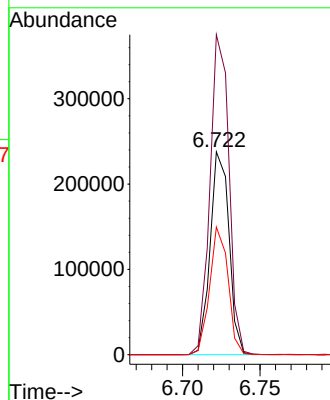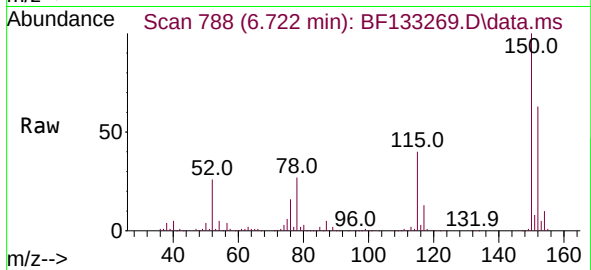

#5
2-Fluorophenol
Concen: 48.307 ng
RT: 5.334 min Scan# 552
Delta R.T. -0.000 min
Lab File: BF133269.D
Acq: 05 May 2023 18:15

Tgt Ion:112 Resp: 644593
Ion Ratio Lower Upper
112 100
64 57.5 46.8 70.2
63 30.1 23.8 35.8


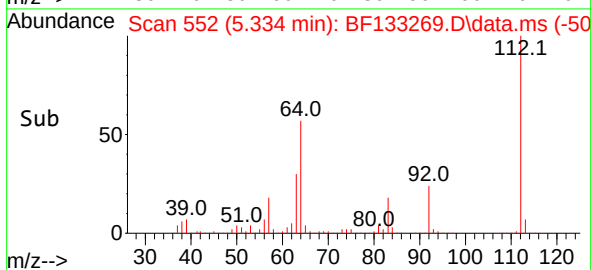
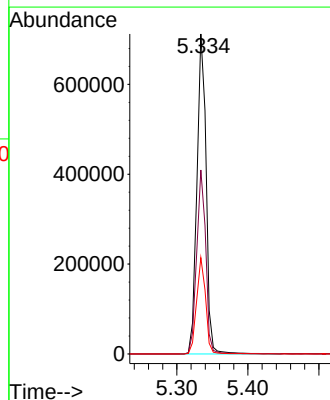
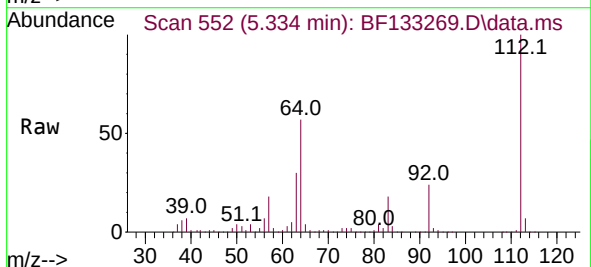


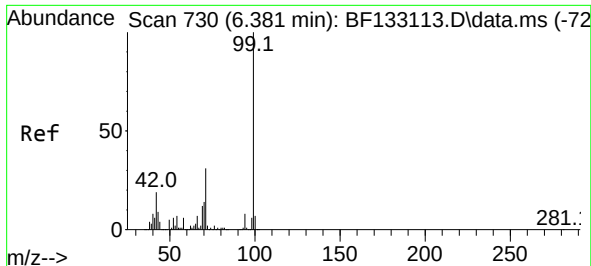

#7
Phenol-d6
Concen: 28.106 ng
RT: 6.357 min Scan# 71
Delta R.T. -0.012 min
Lab File: BF133269.D
Acq: 05 May 2023 18:15




Instrument :
BNA_F
ClientSampleId :
EB-20230503


Tgt Ion: 99 Resp: 465509
Ion Ratio Lower Upper
99 100
42 20.2 16.3 24.5
71 32.3 25.6 38.4

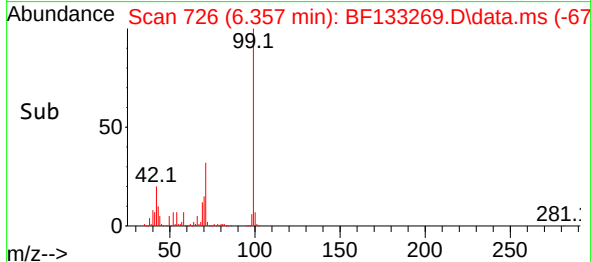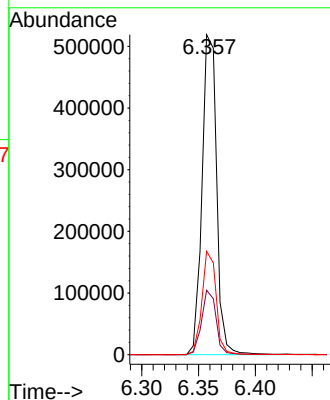

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.010 min Scan# 1007
Delta R.T. -0.006 min
Lab File: BF133269.D
Acq: 05 May 2023 18:15

Tgt Ion: 136 Resp: 807706
Ion Ratio Lower Upper
136 100
137 10.9 8.6 13.0
54 8.5 7.0 10.4
68 6.5 5.4 8.2

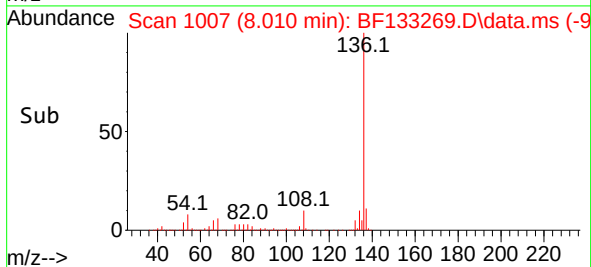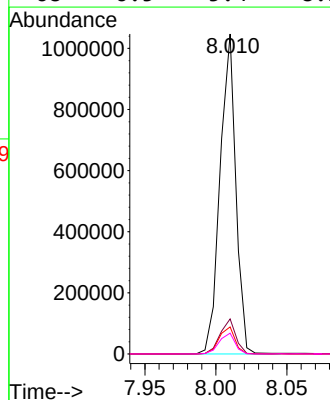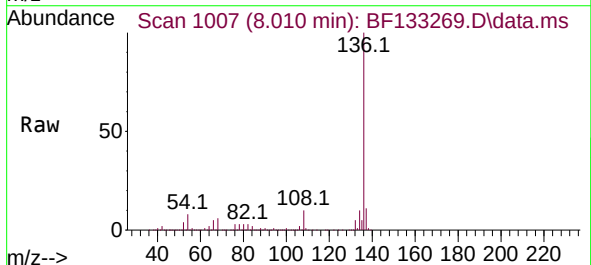

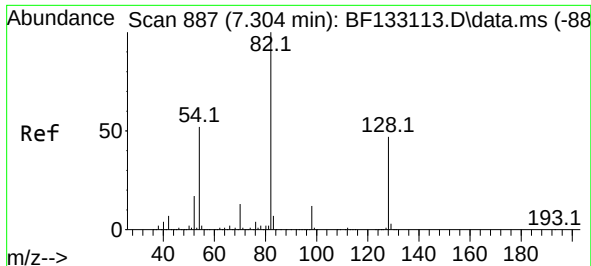

#23

Nitrobenzene-d5

Concen: 81.308 ng

RT: 7.292 min Scan# 81

Delta R.T. -0.006 min

Lab File: BF133269.D

Acq: 05 May 2023 18:15

Instrument :





BNA_F

ClientSampleId :

EB-20230503

Tgt Ion: 82 Resp: 1216691

Ion	Ratio	Lower	Upper
82	100		
128	47.1	37.7	56.5
54	52.3	43.0	64.4

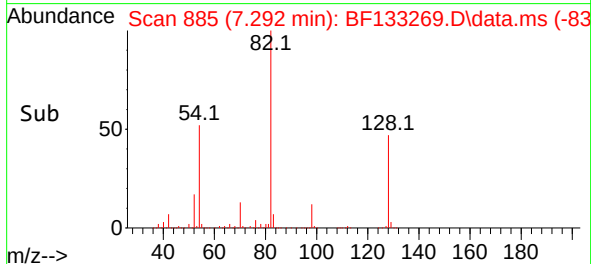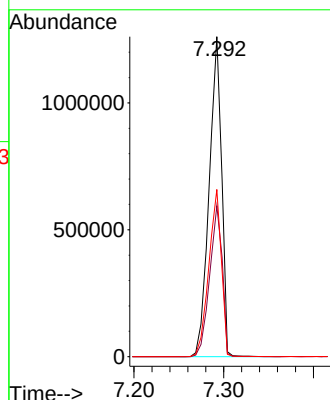

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.763 min Scan# 1305




Delta R.T. -0.000 min


Lab File: BF133269.D

Acq: 05 May 2023 18:15

Tgt Ion: 164 Resp: 430414

Ion	Ratio	Lower	Upper
164	100		
162	101.9	78.7	118.1
160	45.2	35.8	53.6



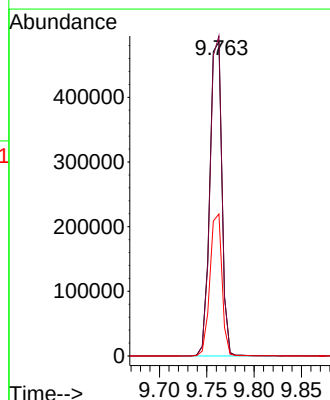
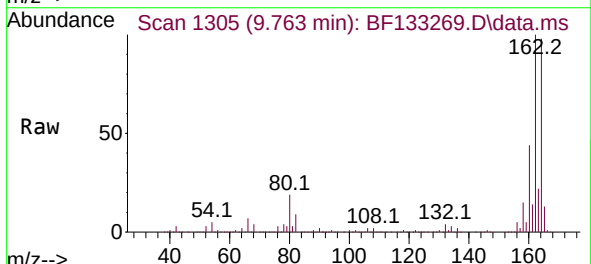


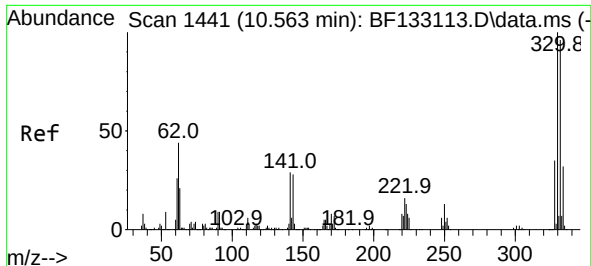

#42
2,4,6-Tribromophenol
Concen: 114.236 ng
RT: 10.551 min Scan# 1441
Delta R.T. -0.006 min
Lab File: BF133269.D
Acq: 05 May 2023 18:15




Instrument :
BNA_F
ClientSampleId :
EB-20230503


Tgt Ion: 330 Resp: 494487
Ion Ratio Lower Upper
330 100
332 97.8 77.1 115.7
141 31.4 25.8 38.8

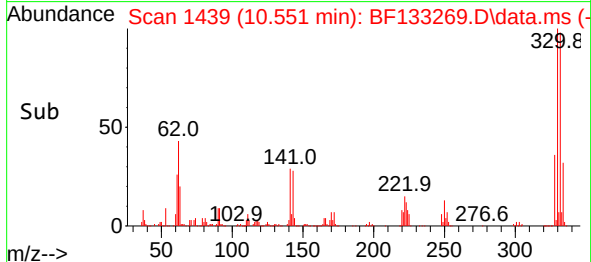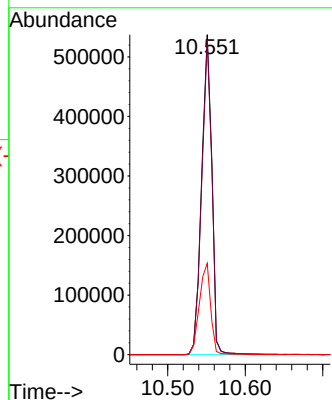

#45
2-Fluorobiphenyl
Concen: 77.225 ng
RT: 9.086 min Scan# 1190
Delta R.T. -0.006 min
Lab File: BF133269.D
Acq: 05 May 2023 18:15

Tgt Ion: 172 Resp: 1986776
Ion Ratio Lower Upper
172 100
171 36.4 28.8 43.2
170 24.3 19.4 29.2


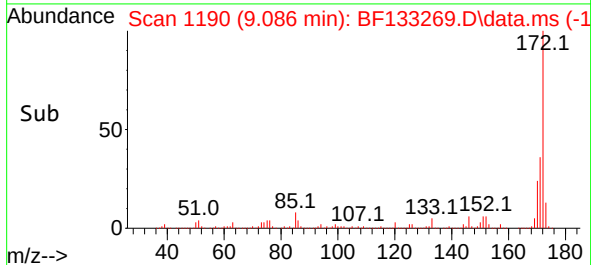
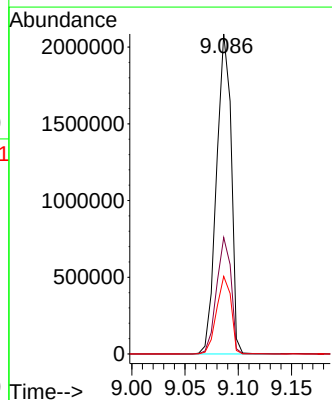
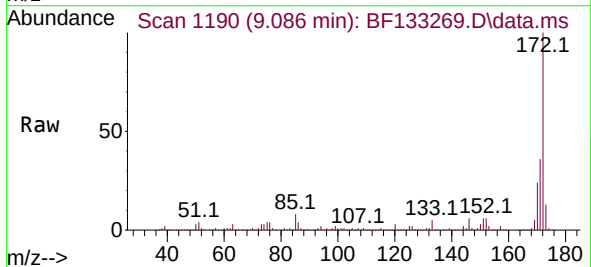


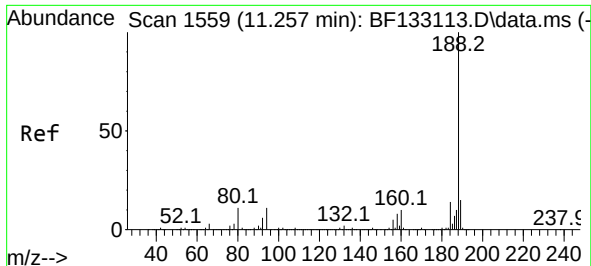

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.239 min Scan# 1
Delta R.T. -0.006 min
Lab File: BF133269.D
Acq: 05 May 2023 18:15




Instrument :
BNA_F
ClientSampleId :
EB-20230503


Tgt Ion:188 Resp: 783794
Ion Ratio Lower Upper
188 100
94 11.5 9.7 14.5
80 11.6 10.4 15.6

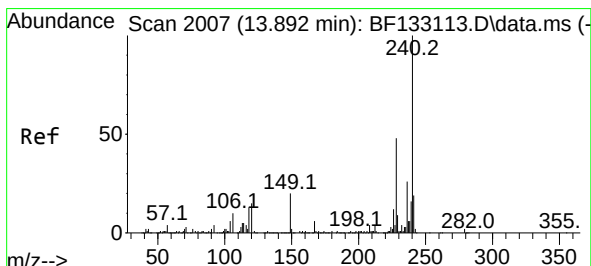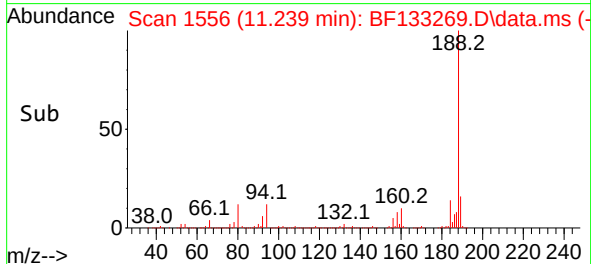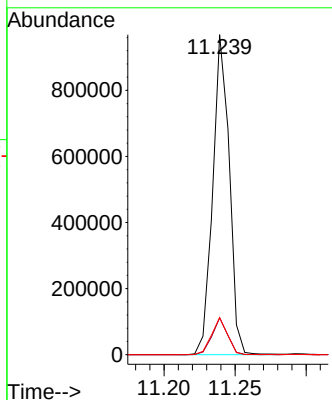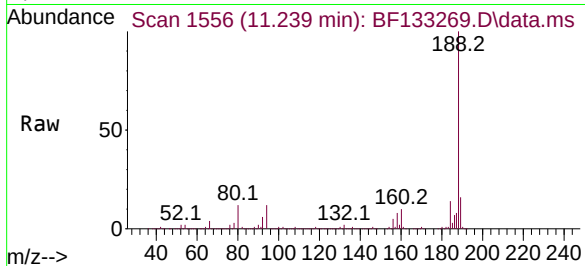

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.874 min Scan# 2004
Delta R.T. -0.006 min
Lab File: BF133269.D
Acq: 05 May 2023 18:15


Tgt Ion:240 Resp: 597563
Ion Ratio Lower Upper
240 100
120 12.9 10.5 15.7
236 27.1 21.5 32.3

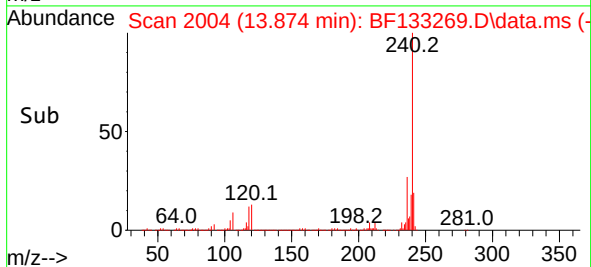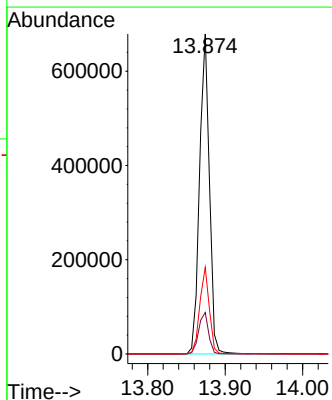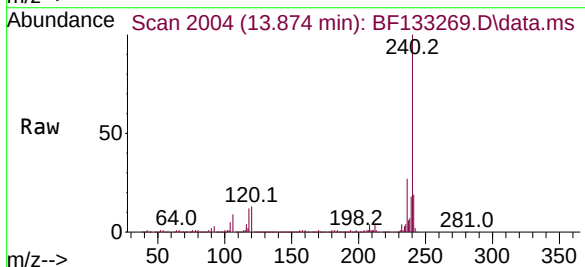



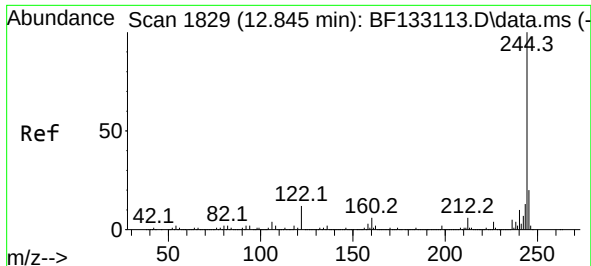


#79
 Terphenyl-d14
 Concen: 68.152 ng
 RT: 12.833 min Scan# 1827
 Delta R.T. -0.000 min
 Lab File: BF133269.D
 Acq: 05 May 2023 18:15

Instrument :
 BNA_F
 ClientSampleId :
 EB-20230503

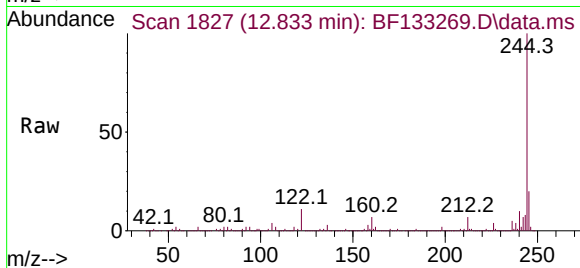

Tgt Ion:244 Resp: 2361338
 Ion Ratio Lower Upper
 244 100
 212 6.6 5.1 7.7
 122 11.4 8.6 13.0

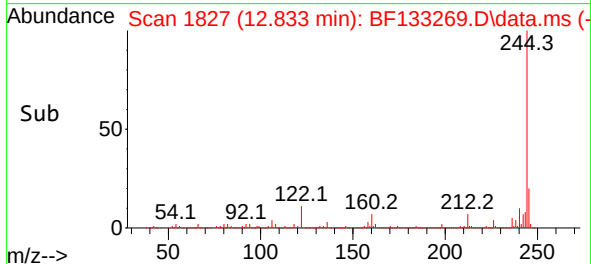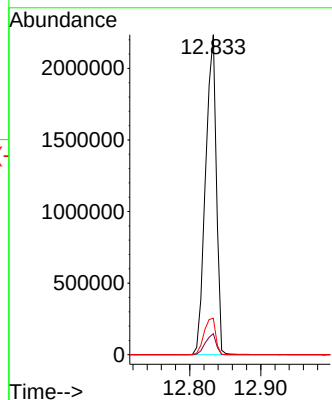

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.292 min Scan# 2245
 Delta R.T. -0.000 min
 Lab File: BF133269.D
 Acq: 05 May 2023 18:15

Tgt Ion:264 Resp: 590304
 Ion Ratio Lower Upper
 264 100
 260 24.9 18.8 28.2
 265 21.9 17.0 25.4

