

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050523\
 Data File : BF133269.D
 Acq On : 05 May 2023 18:15
 Operator : CG\JU
 Sample : 02597-08
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 EB-20230503

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF133269.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.334	548	552	556	rBV	2435486	2160991	34.61%	6.500%
2	6.357	723	726	736	rVB	1455545	1305210	20.90%	3.926%
3	6.722	785	788	792	rBV	1455253	1214858	19.46%	3.654%
4	7.292	879	885	888	rBV	3717346	3611482	57.84%	10.862%
5	8.010	1003	1007	1010	rBV	2101816	1621742	25.97%	4.878%
6	9.086	1185	1190	1193	rBV	6195722	5815736	93.14%	17.492%
7	9.763	1301	1305	1308	rVB	2075624	1859280	29.78%	5.592%
8	10.551	1434	1439	1442	rBV	3786417	3667522	58.74%	11.031%
9	11.239	1553	1556	1560	rVV	2385264	1904182	30.50%	5.727%
10	12.051	1686	1694	1702	rVB2	56908	84347	1.35%	0.254%
11	12.833	1821	1827	1830	rBV	5853025	6244156	100.00%	18.781%
12	13.874	1999	2004	2007	rBV	1948450	1714492	27.46%	5.157%
13	13.968	2014	2020	2031	rBV	392267	412409	6.60%	1.240%
14	15.292	2239	2245	2250	rBV	1357119	1631322	26.13%	4.907%




Sum of corrected areas: 33247729

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050523\
Data File : BF133269.D
Acq On : 05 May 2023 18:15
Operator : CG\JU
Sample : 02597-08
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
EB-20230503

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

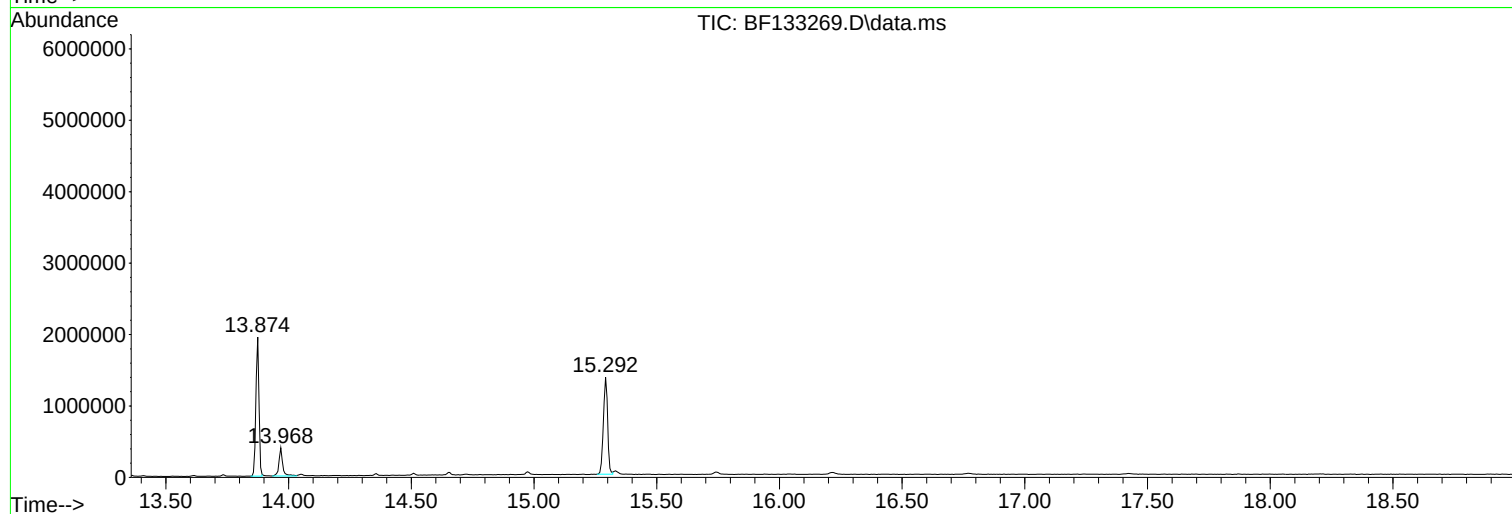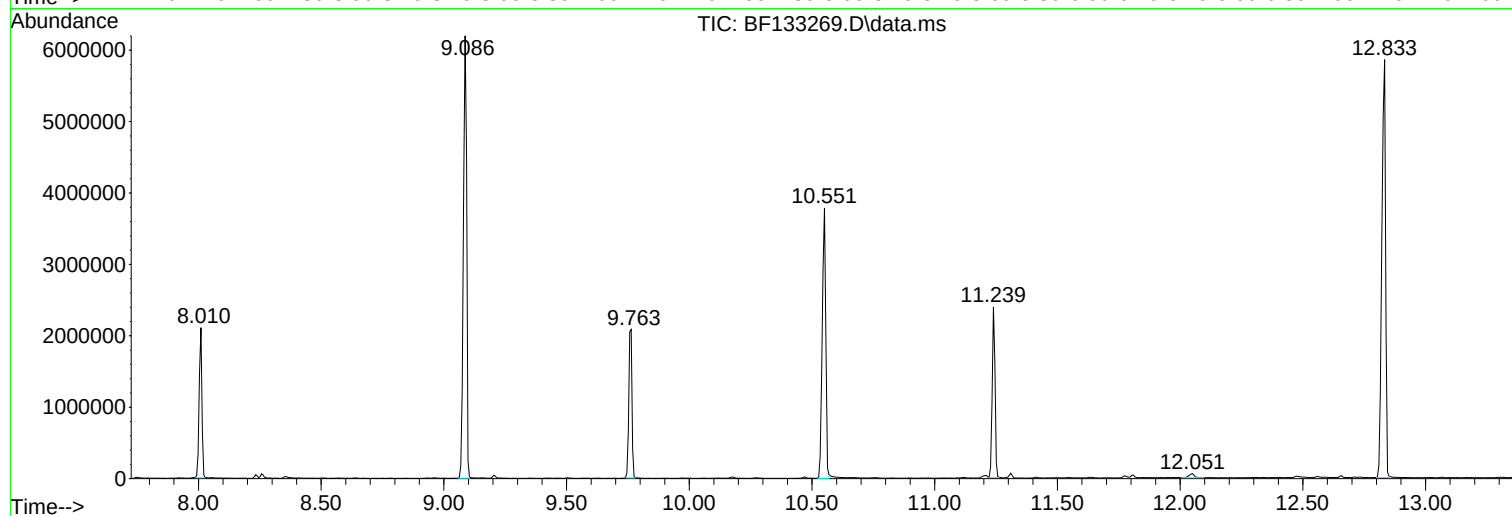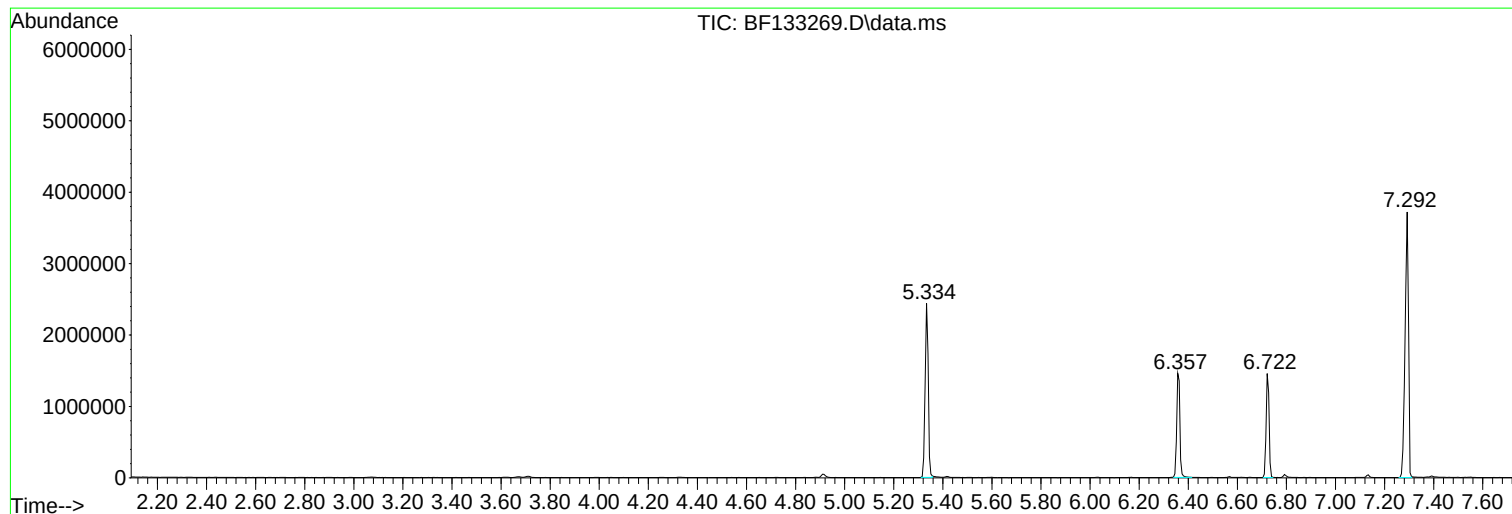

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050523\
Data File : BF133269.D
Acq On : 05 May 2023 18:15
Operator : CG\JU
Sample : 02597-08
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
EB-20230503










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.968	4.81 ng	412409	Chrysene-d12	13.874

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	92
2			(E)-7-Benzylidene-1-azabicyclo[3...]	293	C15H19NO3S	1000483-83-4	91
3			Formaldehyde, (triphenylphosphor...]	304	C19H17N2P	015990-54-2	50
4			Vanadium, cycloheptatrienyl-(pen...]	277	C17H22V	1000155-20-5	23
5			Thiophene-3-carbonitrile, 4-(4-m...]	277	C13H11NO2S2	1000268-75-0	9

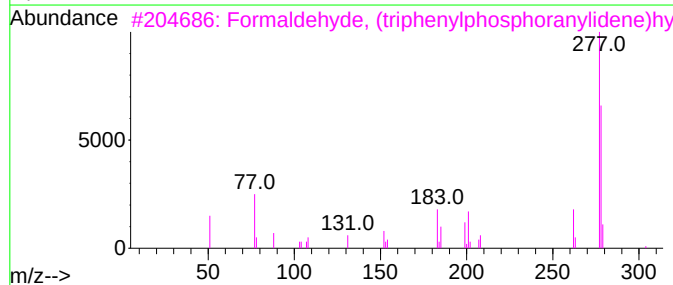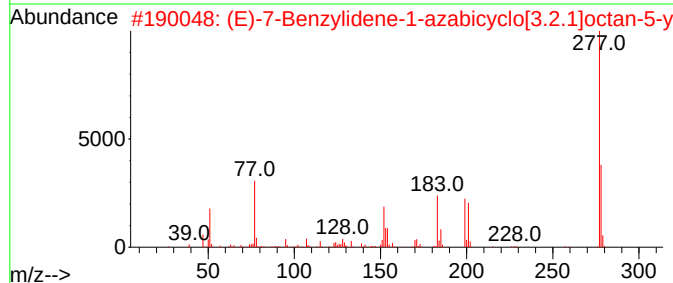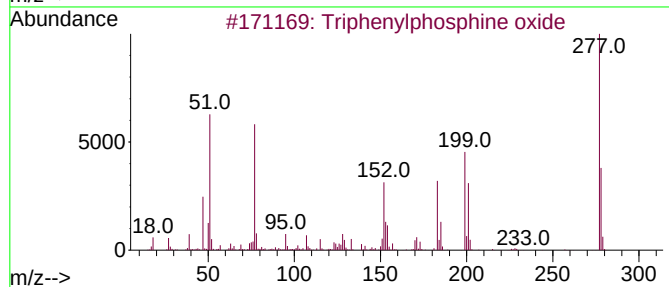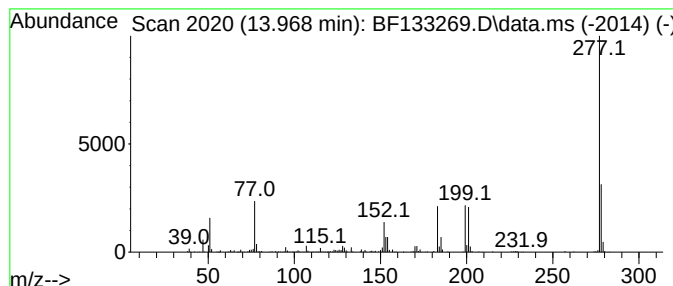

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050523\
Data File : BF133269.D
Acq On : 05 May 2023 18:15
Operator : CG\JU
Sample : 02597-08
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
EB-20230503

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triphenylphosph...	13.968	4.8	ng	412409	5	13.874	1714490	20.0