
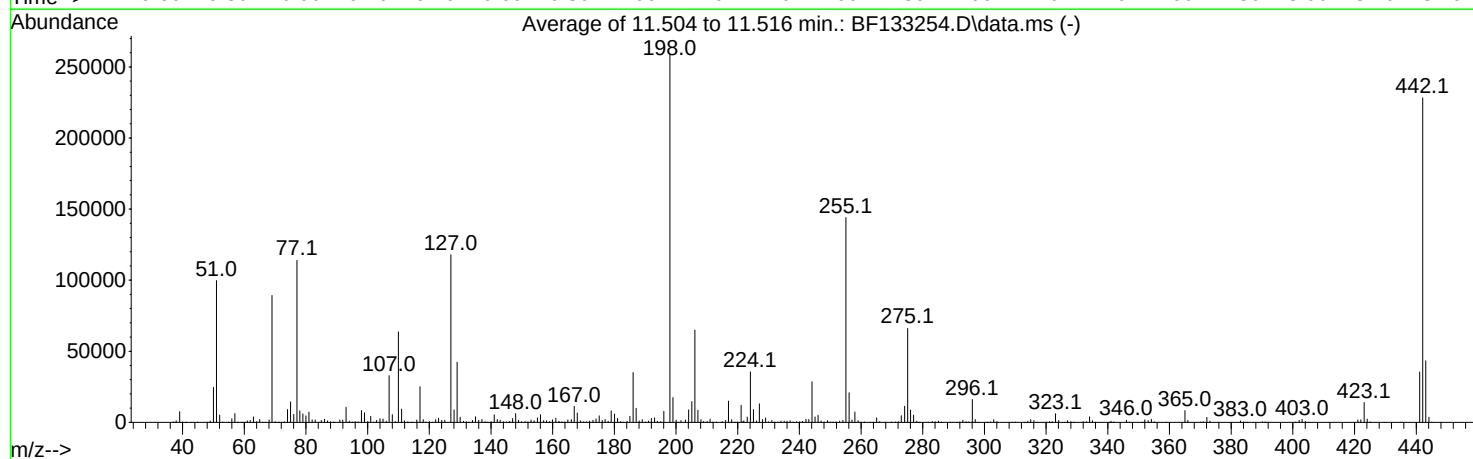


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050523\
Data File : BF133254.D
Acq On : 05 May 2023 09:20
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon May 08 11:30:53 2023

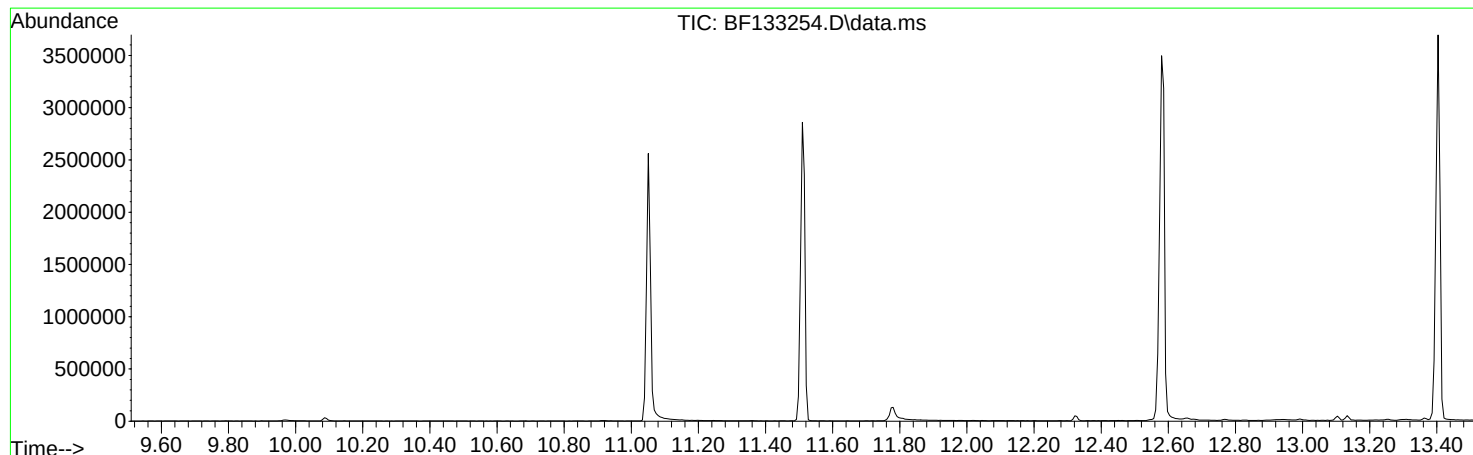

AutoFind: Scans 1601, 1602, 1603; Background Corrected with Scan 1596

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.5	99720	PASS
68	69	0.00	2	1.9	1725	PASS
69	198	0.00	100	34.5	89285	PASS
70	69	0.00	2	0.5	425	PASS
127	198	10	80	45.6	117949	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	258731	PASS
199	198	5	9	6.7	17458	PASS
275	198	10	60	25.5	66080	PASS
365	198	1	100	3.2	8335	PASS
441	198	0.01	100	13.7	35428	PASS
442	442	50	100	100.0	228176	PASS
443	442	15	24	19.0	43317	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/5/2023	BNA_F	<u>BF133254.D</u>
Compound Name	Response	Retention Time
DDT	623657	13.404
DDD	12407	13.104
DDE	1614	12.768
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14021	637678	2.20

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050523\
Data File : BF133254.D
Acq On : 05 May 2023 09:20
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 08 05:22:47 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 05 10:49:34 2023
Response via : Initial Calibration

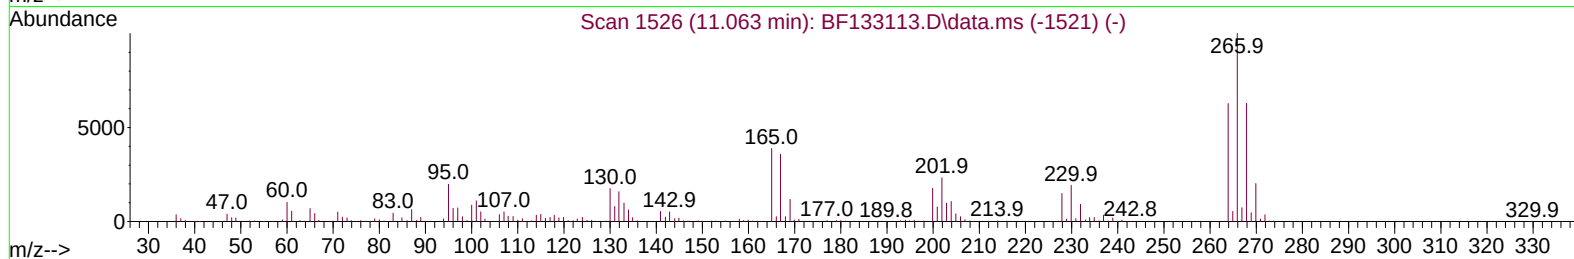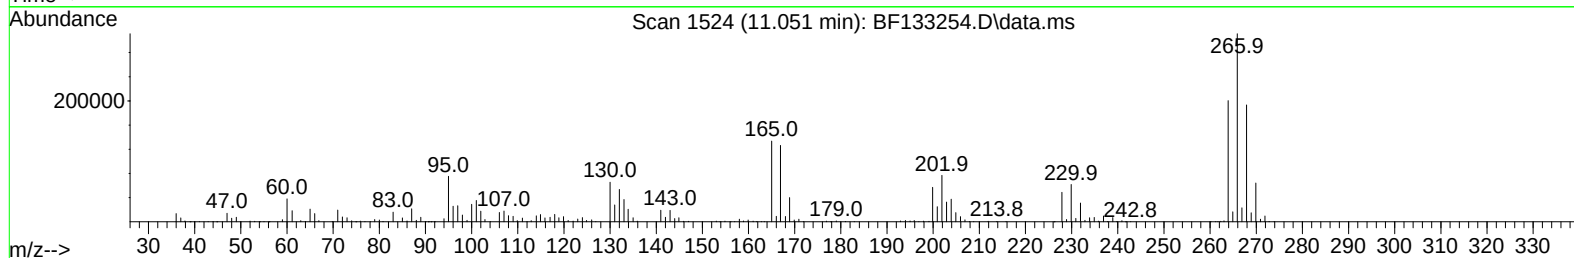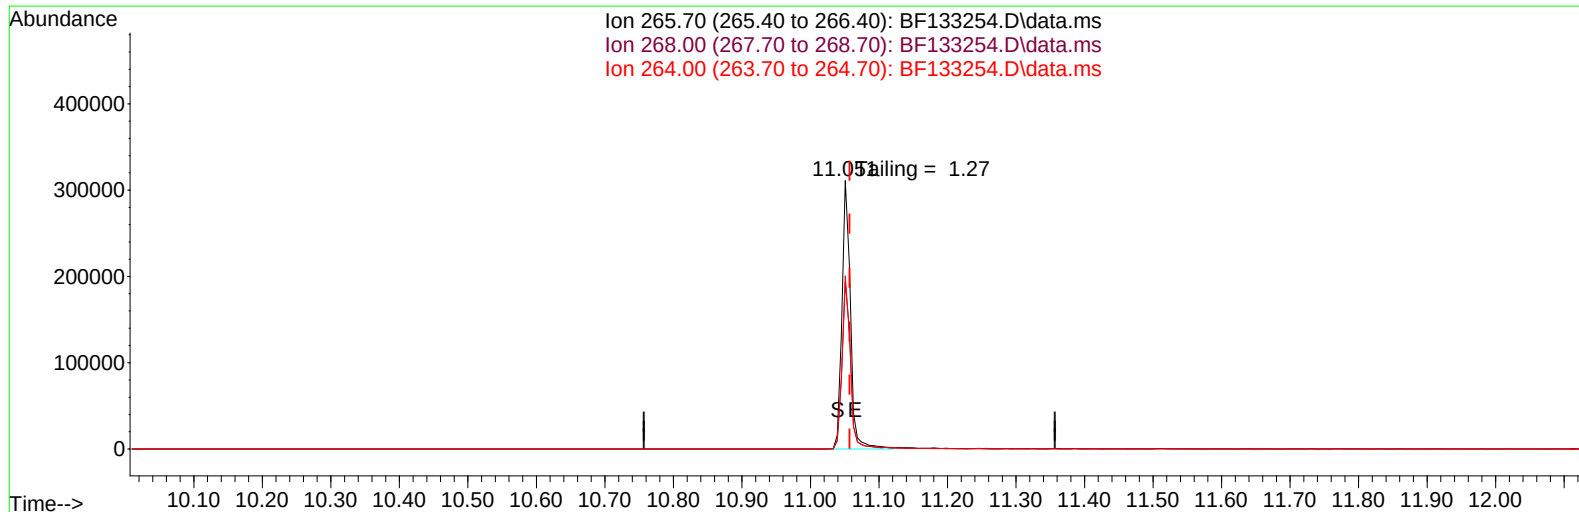

TIC: BF133254.D\data.ms

(70) Pentachlorophenol (C)

11.051min (-0.006) 151645.50 ng




response 267656

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.00	62.12
264.00	63.30	64.49
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050523\
Data File : BF133254.D
Acq On : 05 May 2023 09:20
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 08 05:22:47 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 05 10:49:34 2023
Response via : Initial Calibration

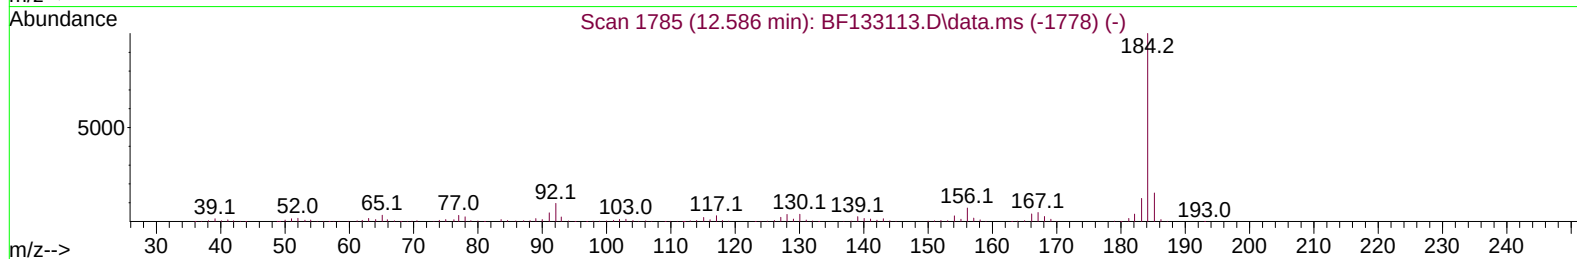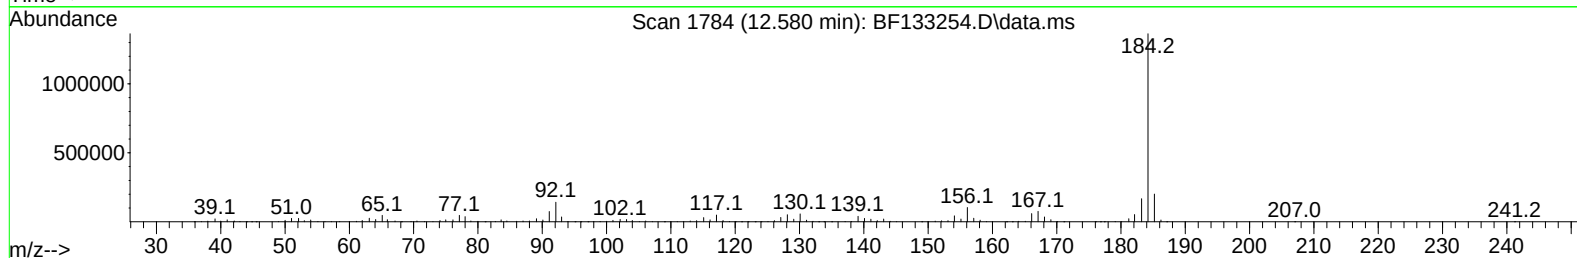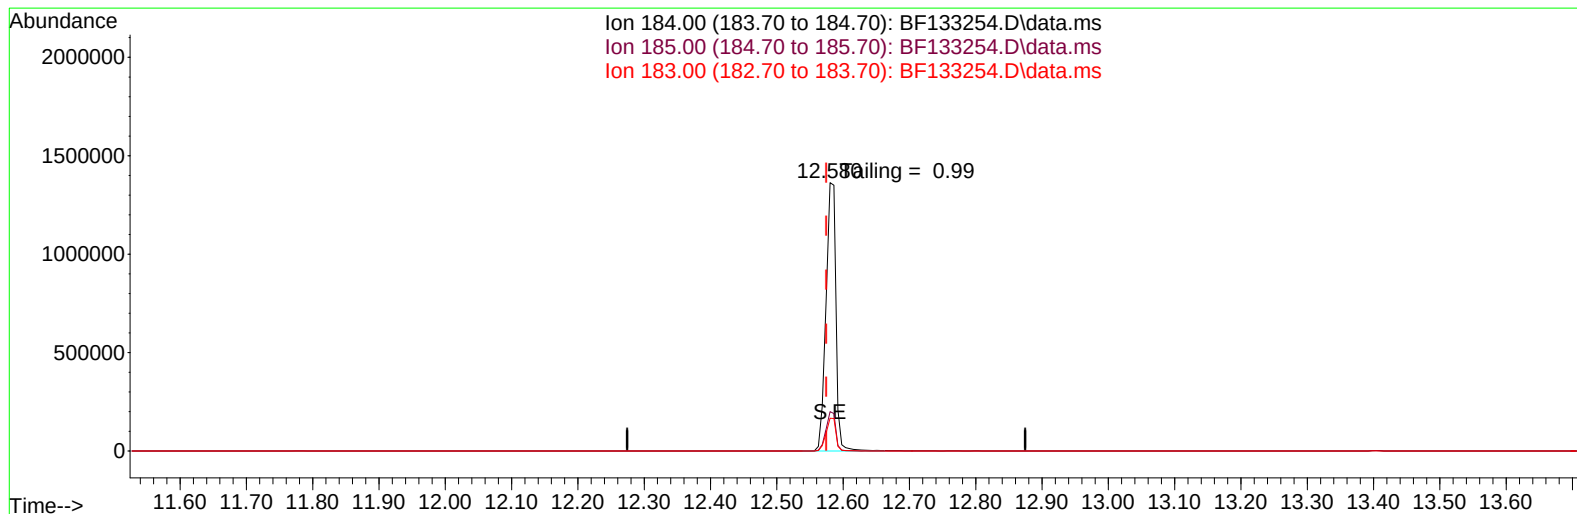

TIC: BF133254.D\data.ms

(77) Benzidine

12.580min (+ 0.006) 239898.49 ng

response 1427997

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	19.30	14.70#
183.00	11.70	12.27
0.00	0.00	0.00