
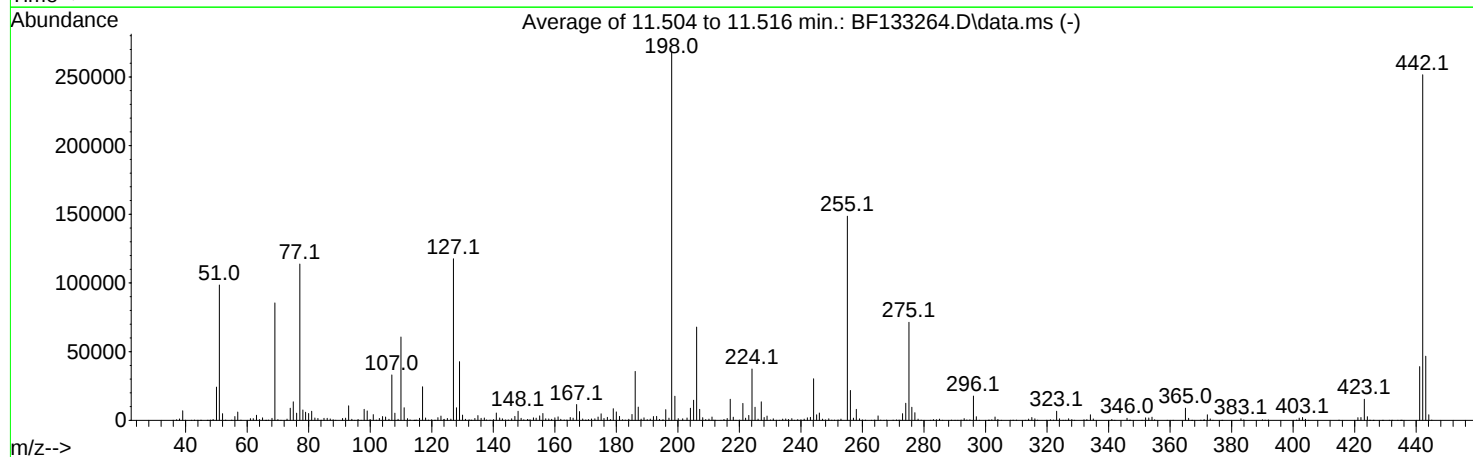


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050523\
Data File : BF133264.D
Acq On : 05 May 2023 15:04
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon May 08 11:30:53 2023

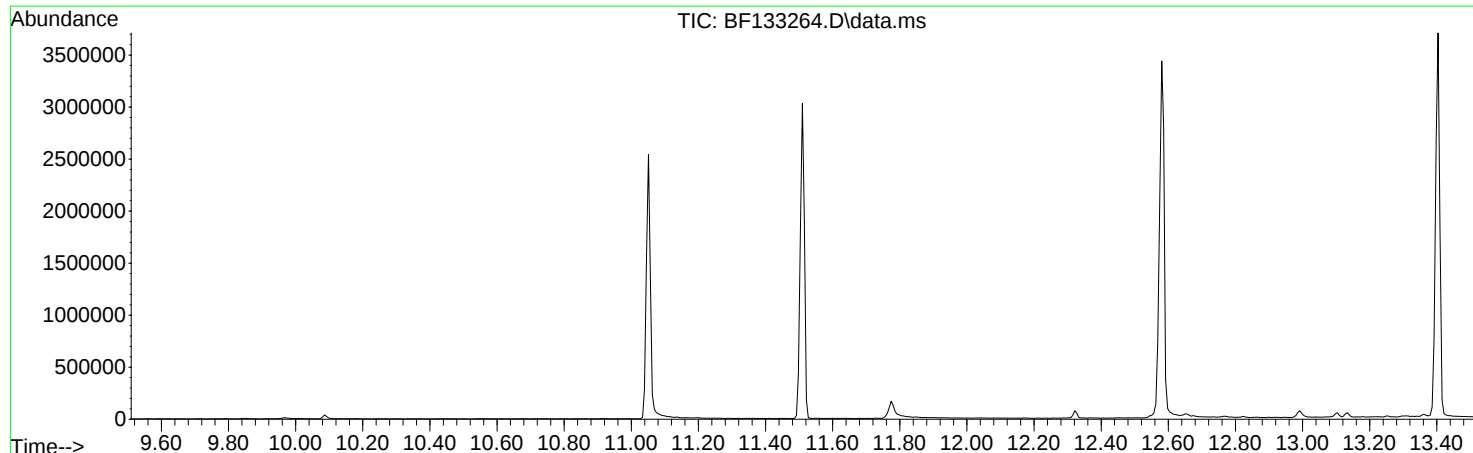

AutoFind: Scans 1601, 1602, 1603; Background Corrected with Scan 1596

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.8	98558	PASS
68	69	0.00	2	1.8	1545	PASS
69	198	0.00	100	31.9	85495	PASS
70	69	0.00	2	0.7	606	PASS
127	198	10	80	43.9	117675	PASS
197	198	0.00	2	0.6	1651	PASS
198	198	100	100	100.0	267776	PASS
199	198	5	9	6.6	17639	PASS
275	198	10	60	26.7	71429	PASS
365	198	1	100	3.3	8859	PASS
441	198	0.01	100	14.6	39157	PASS
442	442	50	100	100.0	251541	PASS
443	442	15	24	18.6	46715	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/5/2023	BNA_F	<u>BF133264.D</u>
Compound Name	Response	Retention Time
DDT	628059	13.404
DDD	12137	13.104
DDE	1610	12.769
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13747	641806	2.14

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050523\
Data File : BF133264.D
Acq On : 05 May 2023 15:04
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 08 05:24:05 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 05 10:49:34 2023
Response via : Initial Calibration

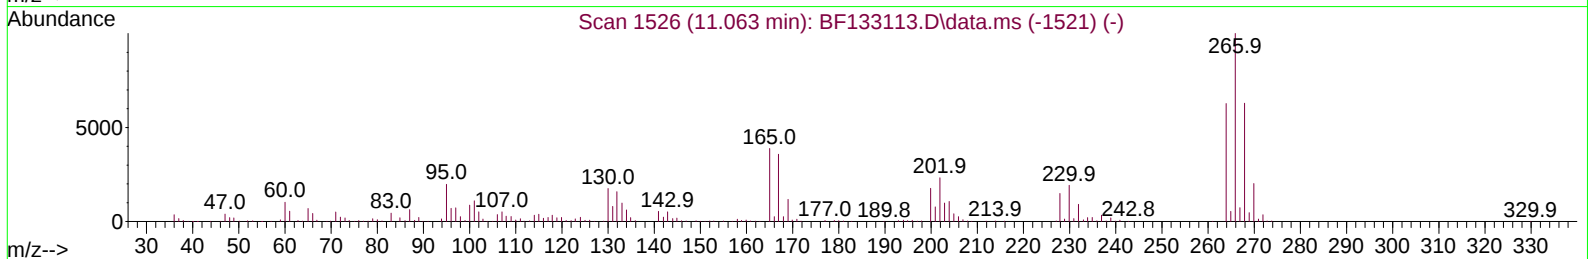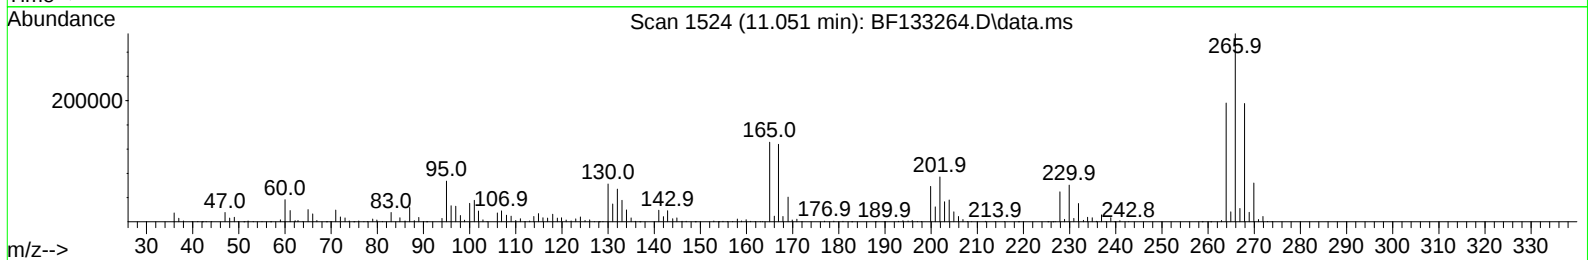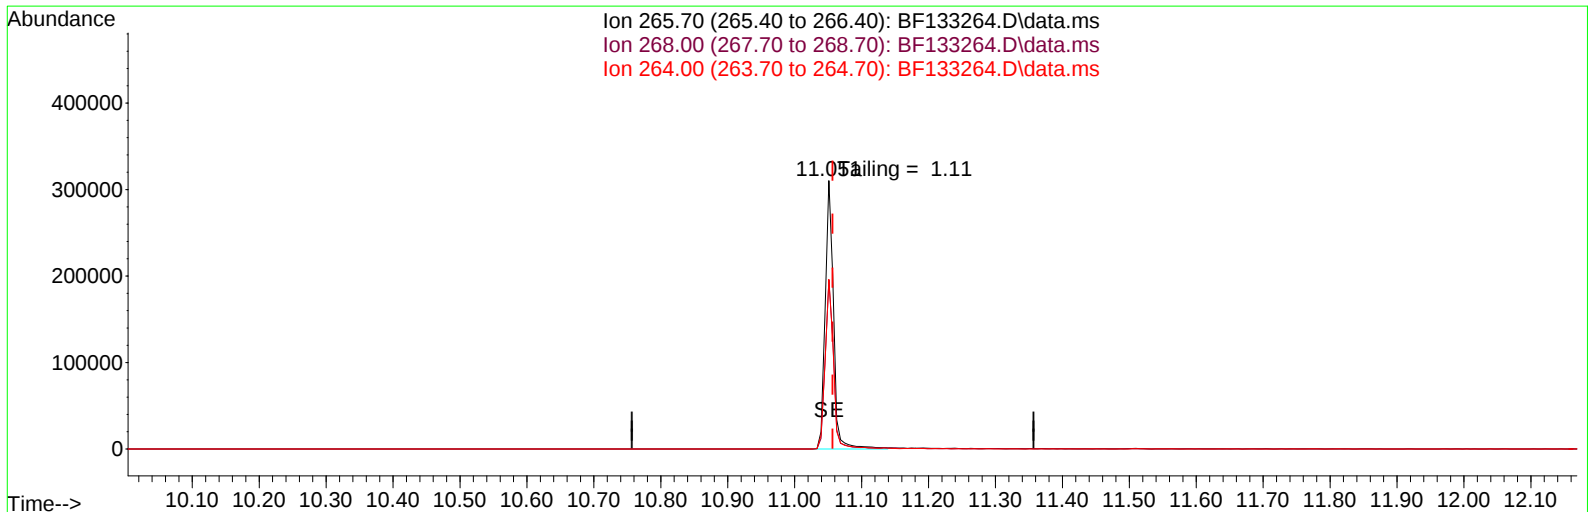

TIC: BF133264.D\data.ms

(70) Pentachlorophenol (C)

11.051min (-0.006) 95326.46 ng




response 271618

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.00	62.90
264.00	63.30	63.19
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050523\
Data File : BF133264.D
Acq On : 05 May 2023 15:04
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 08 05:24:05 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 05 10:49:34 2023
Response via : Initial Calibration

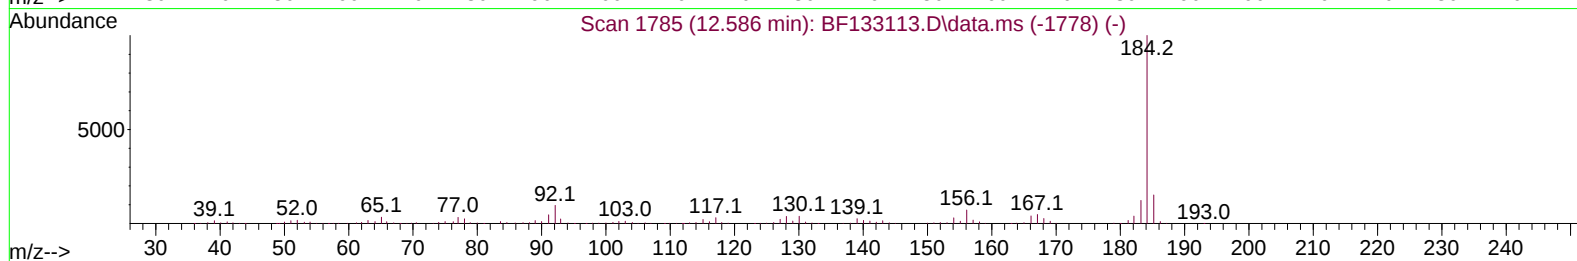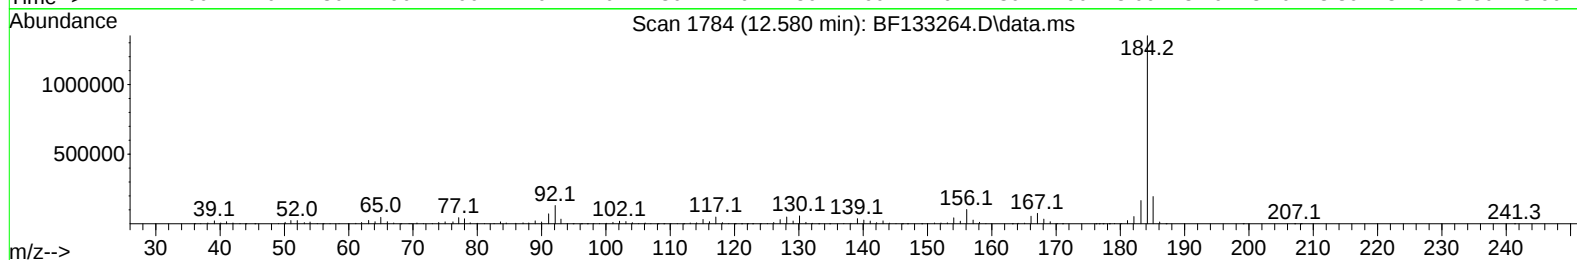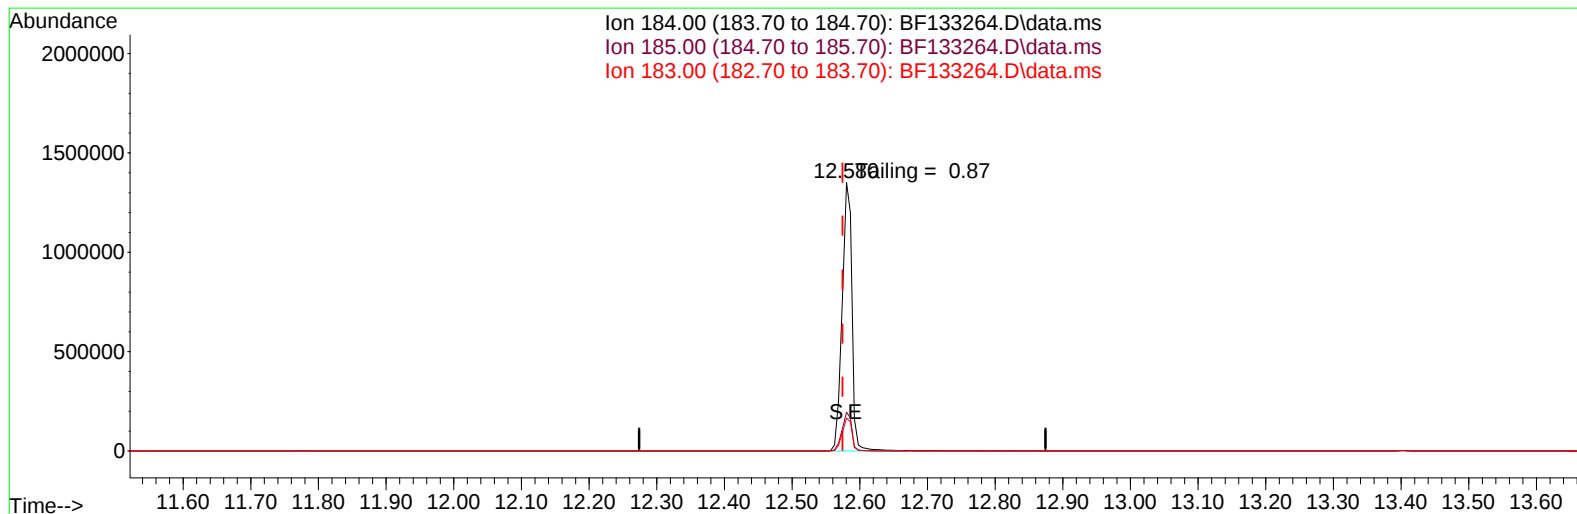

TIC: BF133264.D\data.ms

(77) Benzidine

12.580min (+ 0.006) 168381.59 ng

response 1372457

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	19.30	14.52#
183.00	11.70	12.32
0.00	0.00	0.00