

Data Path : Z:\HPCHEM1\BNA F\DATA\BF050818\
 Data File : BF105150.D
 Acq On : 8 May 2018 18:06
 Operator : JU/SJ
 Sample : J2683-11
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: May 08 19:00:03 2018
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 08 16:33:54 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.79	152	241883	20.00	ng	0.00
21) Naphthalene-d8	8.07	136	959145	20.00	ng	0.00
38) Acenaphthene-d10	9.83	164	472725	20.00	ng	0.00
63) Phenanthrene-d10	11.32	188	932522	20.00	ng	0.00
75) Chrysene-d12	14.00	240	816944	20.00	ng	-0.01
86) Perylene-d12	15.56	264	644378	20.00	ng	0.00

System Monitoring Compounds

5) 2-Fluorophenol	5.40	112	686368	46.75	ng	0.00
7) Phenol-d6	6.41	99	536362	30.68	ng	-0.01
23) Nitrobenzene-d5	7.36	82	1507047	106.49	ng	0.00
41) 2,4,6-Tribromophenol	10.62	330	536122	102.79	ng	0.00
44) 2-Fluorobiphenyl	9.16	172	2636668	86.57	ng	0.00
78) Terphenyl-d14	12.92	244	2950037	83.88	ng	0.00

Target Compounds

						Qvalue
2) 1,4-Dioxane	2.48	88	107	0.014	ng	# 1
4) n-Nitrosodimethylamine	3.05	42	124	0.012	ng	# 29
6) Aniline	6.42	93	463	0.018	ng	# 1
8) 2-Chlorophenol	6.57	128	279	0.018	ng	# 47
9) Benzaldehyde	6.41	77	1245	0.093	ng	# 1
10) Phenol	6.42	94	22495	1.156	ng	# 97
11) bis(2-Chloroethyl)ether	6.56	93	1693	0.106	ng	# 1
12) 1,3-Dichlorobenzene	6.95	146	504	0.027	ng	# 1
13) 1,4-Dichlorobenzene	6.95	146	504	0.027	ng	# 1
14) 1,2-Dichlorobenzene	6.95	146	504	0.029	ng	# 1
15) Benzyl Alcohol	6.95	79	24422	1.825	ng	# 31
16) 2,2'-oxybis(1-Chloropropan	7.10	45	130	0.004	ng	# 70
17) 2-Methylphenol	6.95	107	122	0.009	ng	# 1
19) n-Nitroso-di-n-propylamine	7.36	70	209297	18.082	ng	# 81
20) 3+4-Methylphenols	6.95	107	122	0.008	ng	# 1
22) Acetophenone	7.19	105	325	0.015	ng	# 16
24) Nitrobenzene	7.36	77	5018	0.313	ng	# 31
25) Isophorone	7.36	82	1505905	47.580	ng	# 64
27) 2,4-Dimethylphenol	7.74	122	196	0.014	ng	# 4
28) bis(2-Chloroethoxy)methane	8.07	93	256	0.013	ng	# 1
31) Naphthalene	8.09	128	888	0.019	ng	# 68
32) Benzoic acid	7.74	122	196	9.165	ng	# 69
36) 4-Chloro-3-methylphenol	8.35	107	283	0.021	ng	# 20
37) 2-Methylnaphthalene	8.79	142	339	0.011	ng	# 15
45) 1,1'-Biphenyl	9.25	154	9877	0.256	ng	# 99
46) 2-Chloronaphthalene	9.54	162	1072	0.037	ng	# 1
47) 2-Nitroaniline	9.54	65	1200	5.926	ng	# 1
49) Dimethylphthalate	9.54	163	103481	3.234	ng	# 99
50) 2,6-Dinitrotoluene	9.83	165	60569	8.722	ng	# 26
51) Acenaphthene	9.86	154	110	0.004	ng	# 4
52) 3-Nitroaniline	9.93	138	732	0.100	ng	# 2
54) Dibenzofuran	10.03	168	340	0.008	ng	# 45
56) 2,4-Dinitrotoluene	9.83	165	60569	9.675	ng	# 23
57) Fluorene	10.62	166	19474	0.634	ng	# 92

Data Path : Z:\HPCHEM1\BNA F\DATA\BF050818\
 Data File : BF105150.D
 Acq On : 8 May 2018 18:06
 Operator : JU/SJ
 Sample : J2683-11
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: May 08 19:00:03 2018
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 08 16:33:54 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
59) Diethylphthalate	10.25	149	10518	0.334	nq	# 88
61) 4-Nitroaniline	10.51	138	137	0.019	nq	# 19
62) Azobenzene	10.54	77	1085	0.033	nq	# 1
64) 4,6-Dinitro-2-methylphenol	10.62	198	1150	9.111	nq	# 1
65) n-Nitrosodiphenylamine	10.62	169	14047	0.483	nq	# 41
66) 4-Bromophenyl-phenylether	10.62	248	30684	3.085	nq	# 1
70) Phenanthrene	11.33	178	1605	0.033	nq	# 92
71) Anthracene	11.39	178	376	0.008	nq	# 60
73) Di-n-butylphthalate	11.88	149	9304	0.193	nq	# 92
74) Fluoranthene	12.52	202	639	0.012	nq	# 62
76) Benzidine	12.91	184	37790	1.239	nq	# 96
77) Pyrene	12.74	202	514	0.009	nq	# 57
79) Butylbenzylphthalate	13.39	149	480	6.919	nq	# 63
80) Benzo(a)anthracene	14.00	228	2284	0.046	nq	# 56
82) Chrysene	14.03	228	107	0.002	nq	# 48
83) Bis(2-ethylhexyl)phthalate	13.99	149	2886	0.117	nq	# 90
84) Di-n-octyl phthalate	14.64	149	109	6.937	nq	# 75
87) Benzo(b)fluoranthene	15.12	252	122	0.003	nq	# 60
88) Benzo(k)fluoranthene	15.12	252	122	0.003	nq	# 59
89) Benzo(a)pyrene	15.55	252	2140	0.060	nq	# 75


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF050818\
Data File : BF105150.D
Acq On : 8 May 2018 18:06
Operator : JU/SJ
Sample : J2683-11
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: May 08 19:00:03 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 08 16:33:54 2018
Response via : Initial Calibration

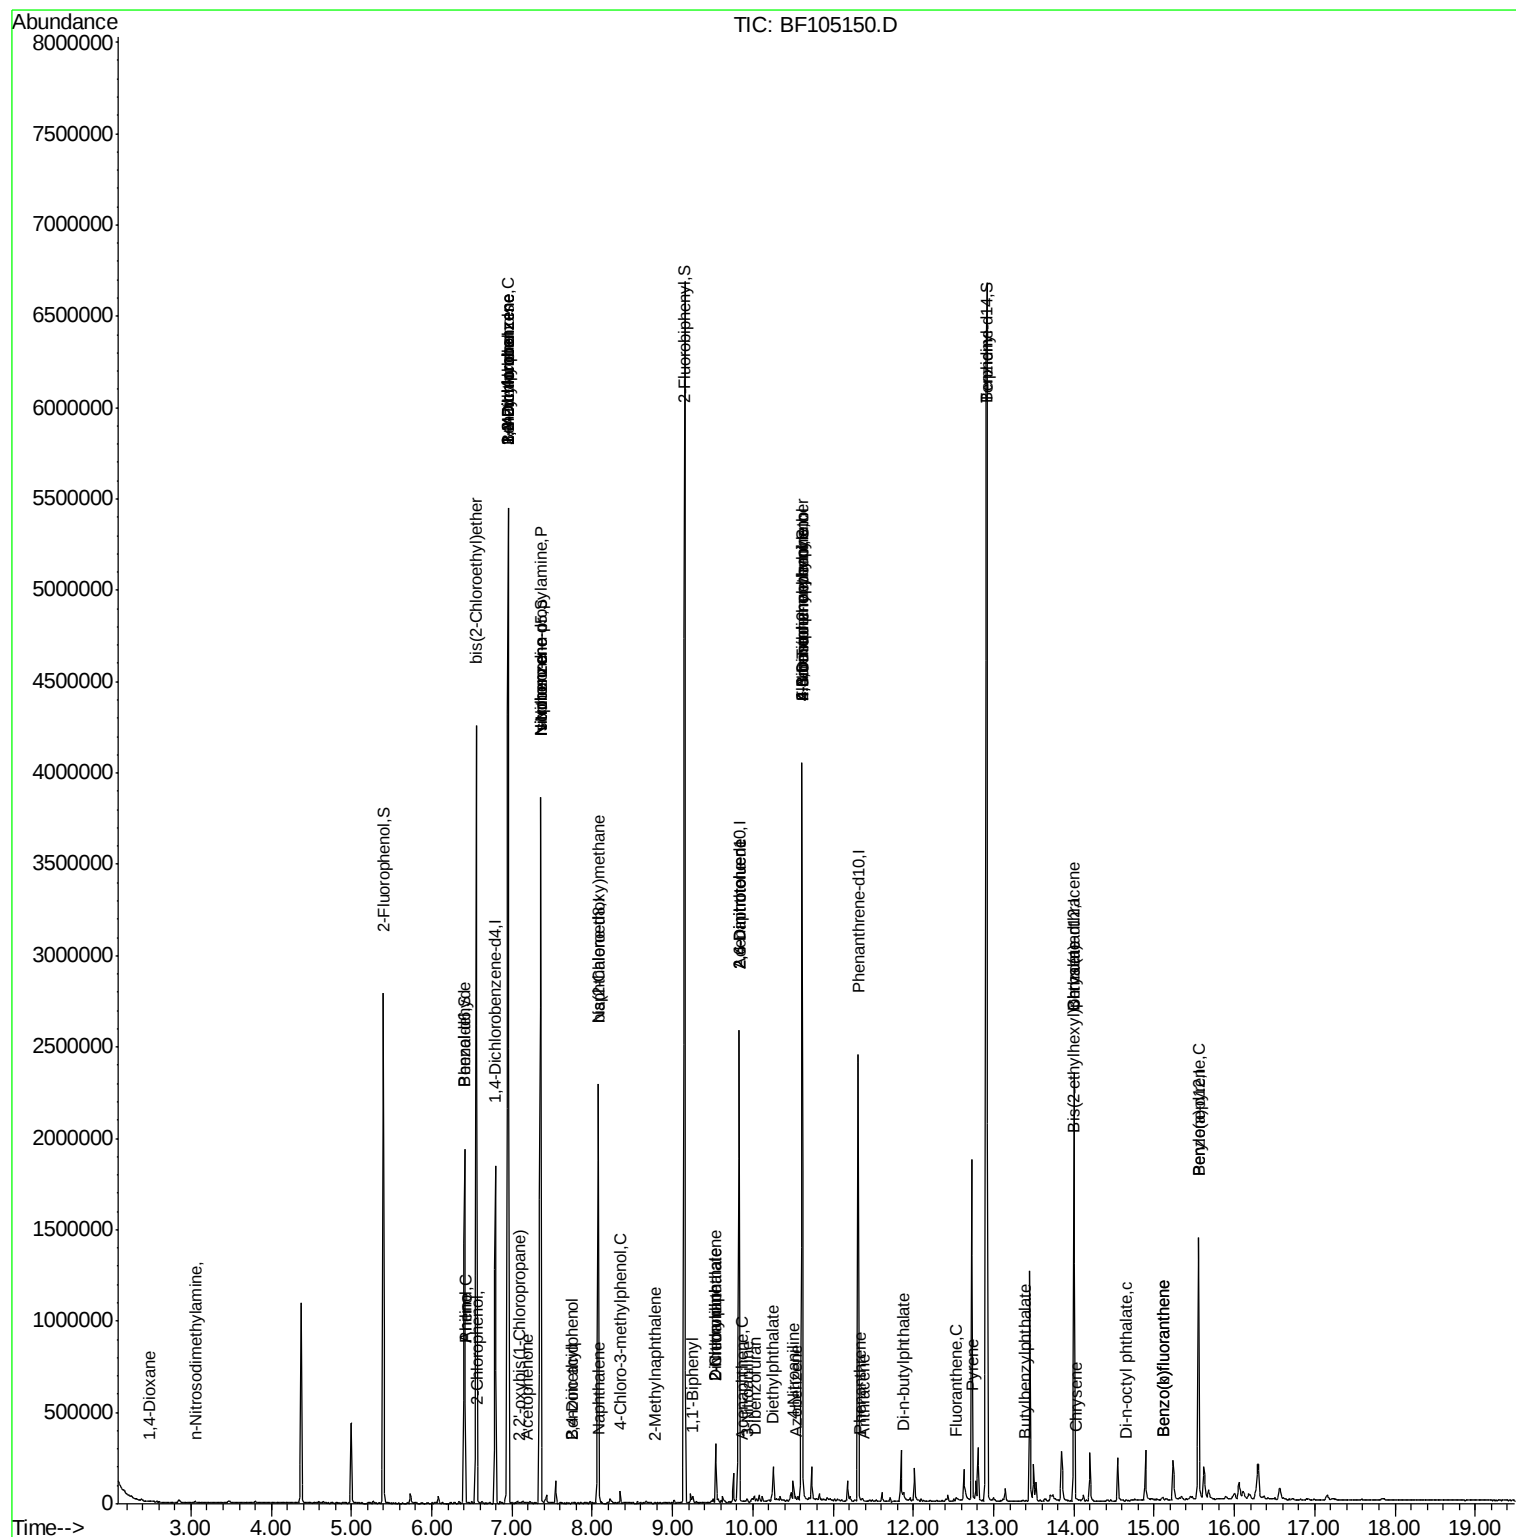







#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.79 min Scan# 800
Delta R.T. -0.00 min
Lab File: BF105150.D
Acq: 8 May 2018 18:06

Instrument :
BNA_F
ClientSampleId :




Tot Ion:152 Resp: 241883
Ion Ratio Lower Upper
152 100
150 156.0 124.6 186.8
115 58.8 50.1 75.1

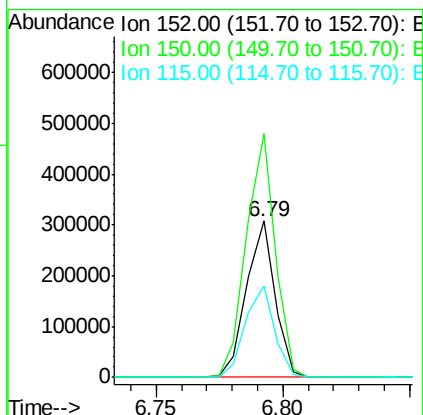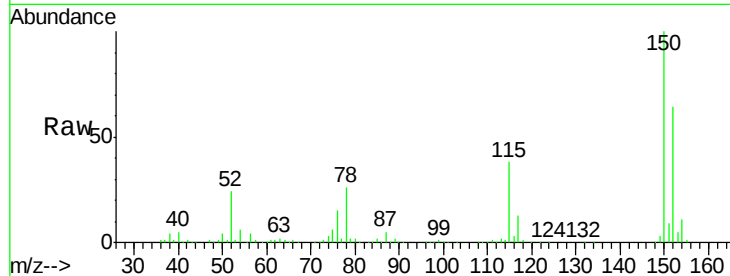


#2

1,4-Dioxane
Concen: 0.014 ng
RT: 2.48 min Scan# 67
Delta R.T. -0.04 min
Lab File: BF105150.D
Acq: 8 May 2018 18:06

Tgt Ion: 88 Resp: 107
Ion Ratio Lower Upper
88 100
58 0.0 62.6 93.8#
43 406.5 24.6 37.0#

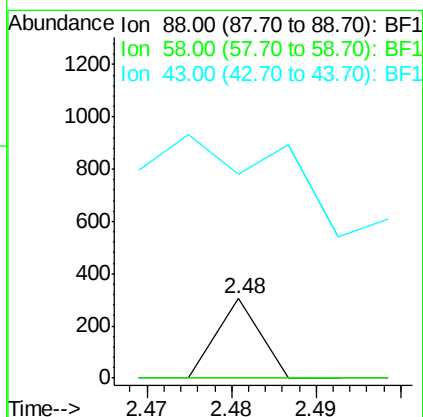




#4




n-Nitrosodimethylamine
Concen: 0.012 ng
RT: 3.05 min Scan# 164
Delta R.T. -0.15 min
Lab File: BF105150.D
Acq: 8 May 2018 18:06

Instrument :
BNA_F
ClientSampleId :

Tot Ion: 42 Resp: 124
Ion Ratio Lower Upper
42 100
74 117.1 104.9 157.3
44 355.3 6.9 10.3#




Abundance Ion 42.00 (41.70 to 42.70): BF1
Ion 74.00 (73.70 to 74.70): BF1
Ion 44.00 (43.70 to 44.70): BF1

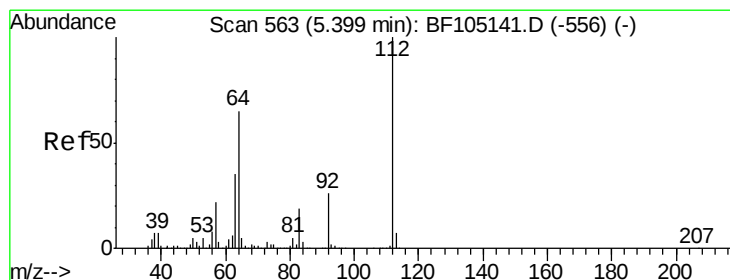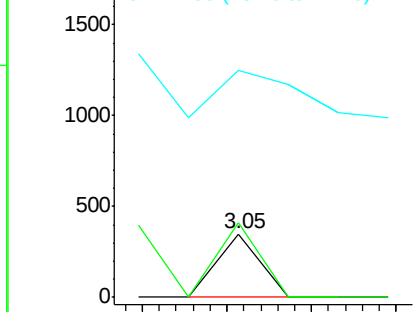



#5


2-Fluorophenol
Concen: 46.748 ng
RT: 5.40 min Scan# 563
Delta R.T. -0.00 min
Lab File: BF105150.D
Acq: 8 May 2018 18:06

Tgt Ion: 112 Resp: 686368
Ion Ratio Lower Upper
112 100
64 62.8 47.9 71.9
63 32.1 23.7 35.5



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

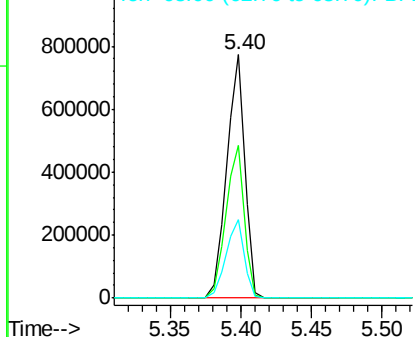



#6

Aniline

Concen: 0.018 ng

RT: 6.42 min Scan# 737

Delta R.T. -0.04 min

Lab File: BF105150.D

Acq: 8 May 2018 18:06

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 93 Resp: 463

Ion Ratio Lower Upper

93 100

66 1844.7 32.2 48.2#




65 1305.4 16.4 24.6#



Abundance Ion 93.00 (92.70 to 93.70): BF1

Ion 66.00 (65.70 to 66.70): BF1

Ion 65.00 (64.70 to 65.70): BF1

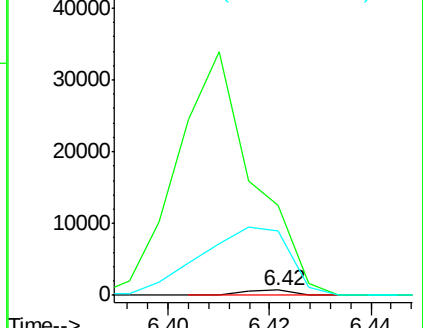

#7

Phenol-d6

Concen: 30.680 ng

RT: 6.41 min Scan# 735

Delta R.T. -0.01 min

Lab File: BF105150.D

Acq: 8 May 2018 18:06


Tgt Ion: 99 Resp: 536362

Ion Ratio Lower Upper

99 100

42 21.1 14.5 21.7



71 33.4 25.4 38.0




Abundance Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

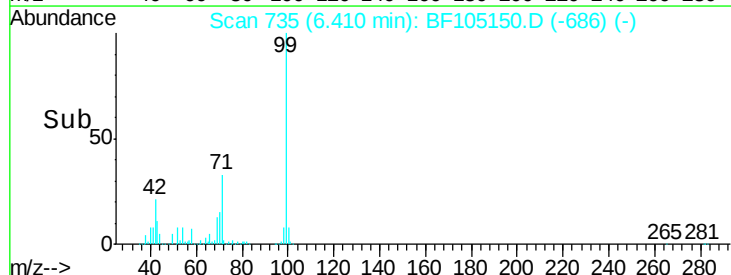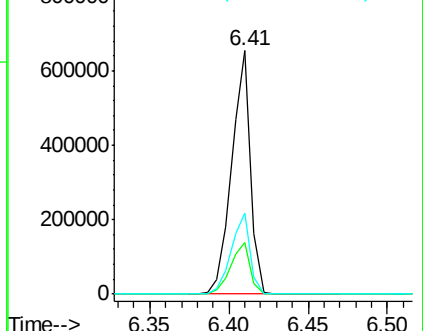

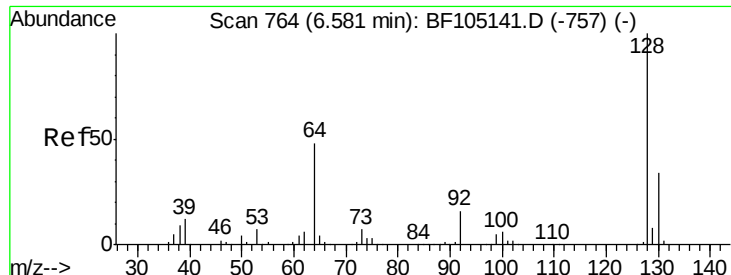

#8

2-Chlorophenol

Concen: 0.018 ng

RT: 6.57 min Scan# 763

Delta R.T. -0.01 min

Lab File: BF105150.D

Acq: 8 May 2018 18:06

Instrument :

BNA_F

ClientSampleId :


Tot Ion:128 Resp: 279

Ion Ratio Lower Upper

128 100

130 0.0 13.0 53.0#




64 83.6 29.4 69.4#



Abundance Ion 128.00 (127.70 to 128.70): E

Ion 130.00 (129.70 to 130.70): E

Ion 64.00 (63.70 to 64.70): BF1

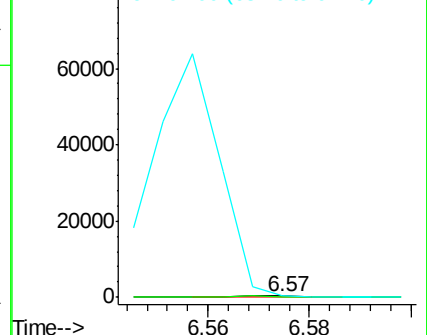

#9

Benzaldehyde

Concen: 0.093 ng

RT: 6.41 min Scan# 735

Delta R.T. 0.06 min

Lab File: BF105150.D

Acq: 8 May 2018 18:06


Tgt Ion: 77 Resp: 1245

Ion Ratio Lower Upper

77 100

105 0.0 81.1 121.1#



106 0.0 74.5 114.5#






Abundance Ion 77.00 (76.70 to 77.70): BF1

Ion 105.00 (104.70 to 105.70): E

Ion 106.00 (105.70 to 106.70): E

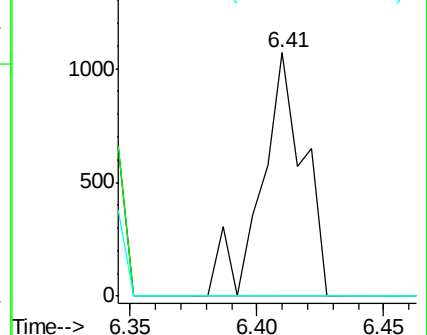



#10

Phenol

Concen: 1.156 ng

RT: 6.42 min Scan# 737

Delta R.T. -0.01 min

Lab File: BF105150.D

Acq: 8 May 2018 18:06

Instrument :

BNA_F

ClientSampleId :





Tot Ion: 94 Resp: 22495

Ion Ratio Lower Upper

94 100

65 27.9 7.9 47.9

66 39.4 16.2 56.2

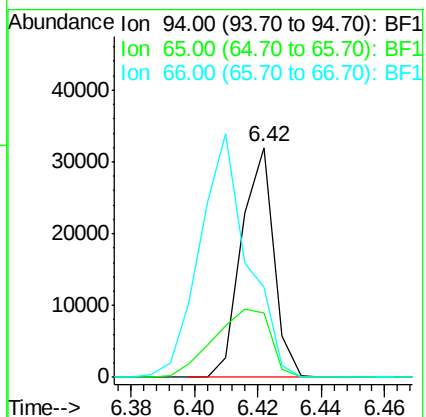

#11

bis(2-Chloroethyl)ether

Concen: 0.106 ng

RT: 6.56 min Scan# 760

Delta R.T. 0.02 min

Lab File: BF105150.D

Acq: 8 May 2018 18:06


Tgt Ion: 93 Resp: 1693


Ion Ratio Lower Upper

93 100

63 699.4 58.6 98.6#

95 211.5 11.8 51.8#

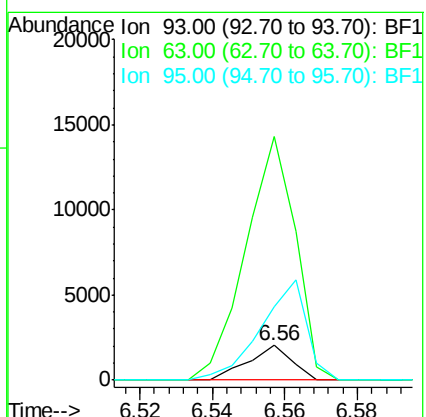

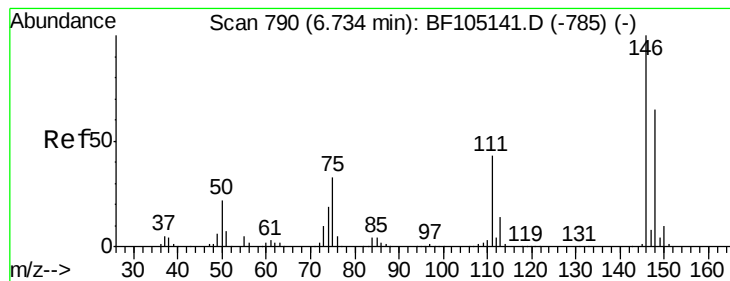

#12

1,3-Dichlorobenzene

Concen: 0.027 ng

RT: 6.95 min Scan# 826

Delta R.T. 0.21 min

Lab File: BF105150.D

Acq: 8 May 2018 18:06

Instrument :

BNA_F

ClientSampleId :


Tot Ion:146 Resp: 504

Ion Ratio Lower Upper

146 100

148 339.4 51.8 77.8#




75 9408.3 24.2 36.4#



Abundance Ion 146.00 (145.70 to 146.70): E

Ion 148.00 (147.70 to 148.70): E

Ion 75.00 (74.70 to 75.70): BF1

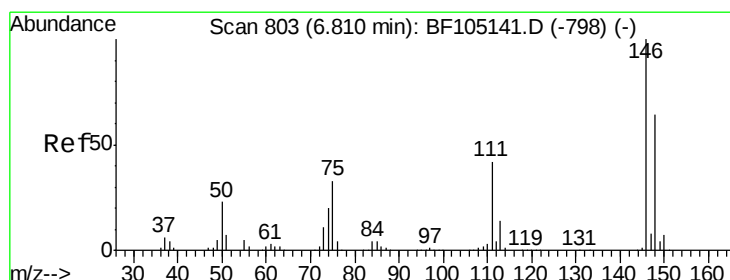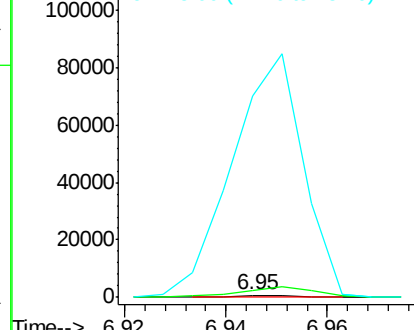

#13

1,4-Dichlorobenzene

Concen: 0.027 ng

RT: 6.95 min Scan# 826

Delta R.T. 0.13 min

Lab File: BF105150.D

Acq: 8 May 2018 18:06


Tgt Ion:146 Resp: 504

Ion Ratio Lower Upper

146 100

148 339.4 50.8 76.2#



111 1328.1 34.2 51.2#

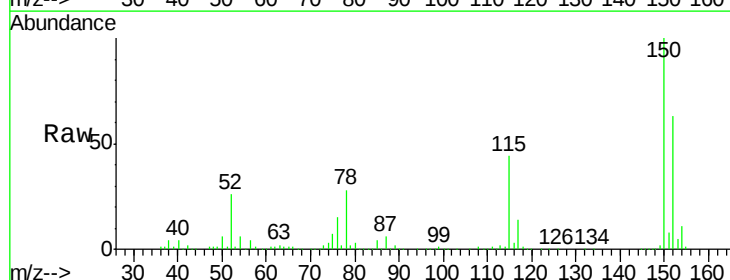


Abundance Ion 146.00 (145.70 to 146.70): E

Ion 148.00 (147.70 to 148.70): E

Ion 111.00 (110.70 to 111.70): E

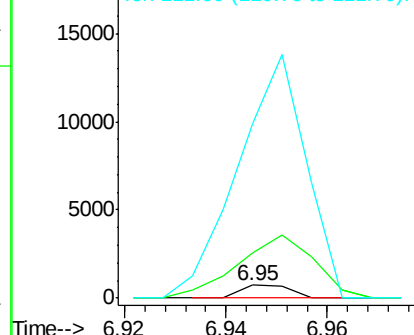







#14
 1,2-Dichlorobenzene
 Concen: 0.029 ng
 RT: 6.95 min Scan# 826
 Delta R.T. -0.02 min
 Lab File: BF105150.D
 Acq: 8 May 2018 18:06

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:146 Resp: 504
 Ion Ratio Lower Upper
 146 100
 148 339.4 50.6 75.8#
 111 1328.1 36.0 54.0#




Abundance Ion 146.00 (145.70 to 146.70): E
 Ion 148.00 (147.70 to 148.70): E
 Ion 111.00 (110.70 to 111.70): E

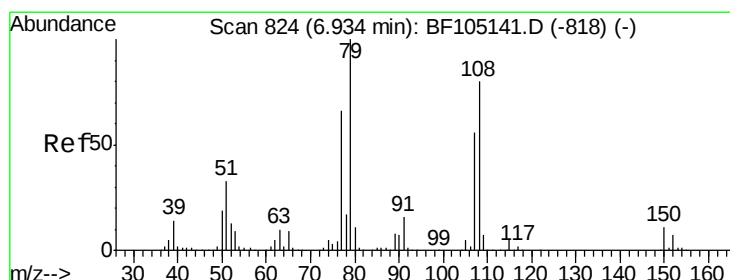
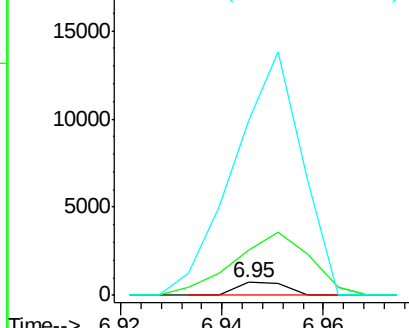



#15
 Benzyl Alcohol
 Concen: 1.825 ng
 RT: 6.95 min Scan# 827
 Delta R.T. 0.02 min
 Lab File: BF105150.D
 Acq: 8 May 2018 18:06

Tgt Ion: 79 Resp: 24422
 Ion Ratio Lower Upper
 79 100
 108 35.2 65.1 97.7#
 77 134.3 50.6 75.8#



Abundance Ion 79.00 (78.70 to 79.70): BF1
 Ion 108.00 (107.70 to 108.70): E
 Ion 77.00 (76.70 to 77.70): BF1

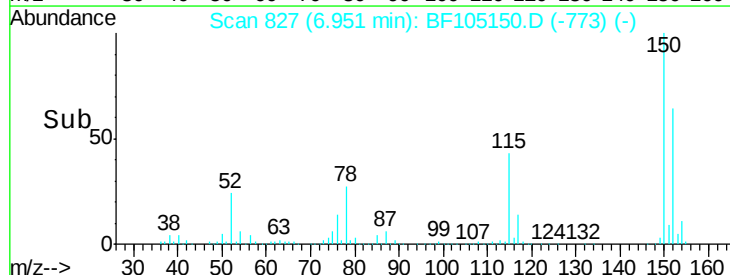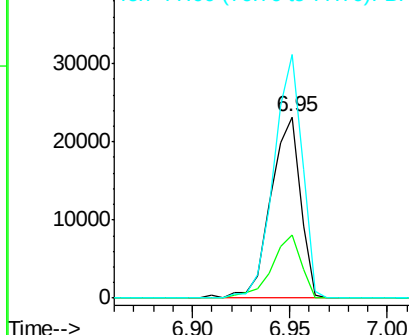







#16
2,2'-oxvbis(1-Chloropropane)
Concen: 0.004 ng
RT: 7.10 min Scan# 852
Delta R.T. 0.03 min
Lab File: BF105150.D
Acq: 8 May 2018 18:06

Instrument :
BNA_F
ClientSampleId :

Tot Ion: 45 Resp: 130
Ion Ratio Lower Upper
45 100
77 0.0 0.0 32.9
79 0.0 0.0 29.6




Abundance Ion 45.00 (44.70 to 45.70): BF1
Ion 77.00 (76.70 to 77.70): BF1
Ion 79.00 (78.70 to 79.70): BF1

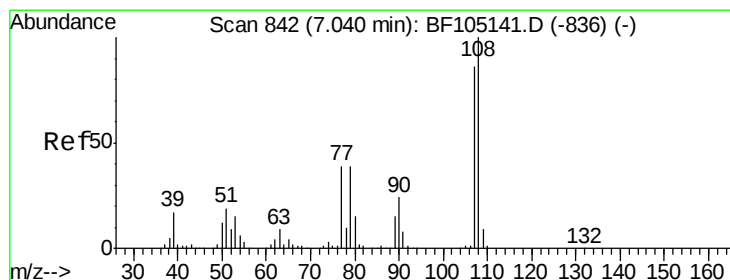
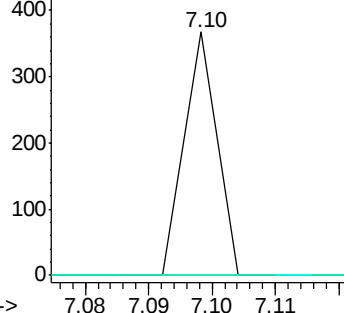





#17
2-Methylphenol
Concen: 0.009 ng
RT: 6.95 min Scan# 827
Delta R.T. -0.09 min
Lab File: BF105150.D
Acq: 8 May 2018 18:06

Tgt Ion:107 Resp: 122
Ion Ratio Lower Upper
107 100
108 2359.2 91.7 137.5#
77 9008.1 33.8 50.8#
79 6707.5 33.8 50.8#

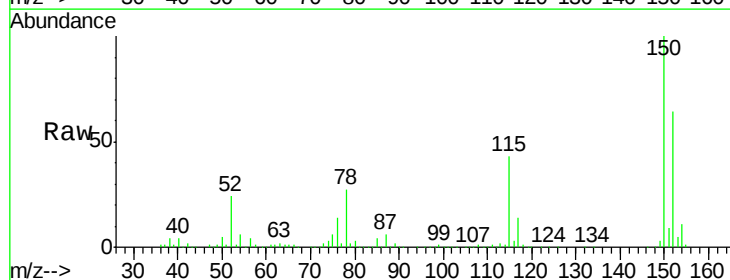

Abundance Ion 107.00 (106.70 to 107.70): E
Ion 108.00 (107.70 to 108.70): E
Ion 77.00 (76.70 to 77.70): BF1
Ion 79.00 (78.70 to 79.70): BF1

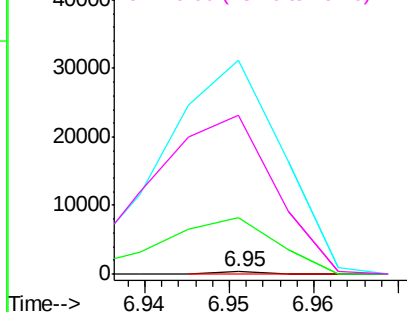



#19

n-Nitroso-di-n-propylamine

Concen: 18.082 ng

RT: 7.36 min Scan# 897

Delta R.T. 0.15 min

Lab File: BF105150.D

Acq: 8 May 2018 18:06

Instrument :

BNA_F

ClientSampled :

Tot Ion: 70 Resp: 209297





Ion Ratio Lower Upper

70 100

42 51.6 47.5 71.3

101 0.0 7.4 11.2#

130 1.9 16.6 25.0#

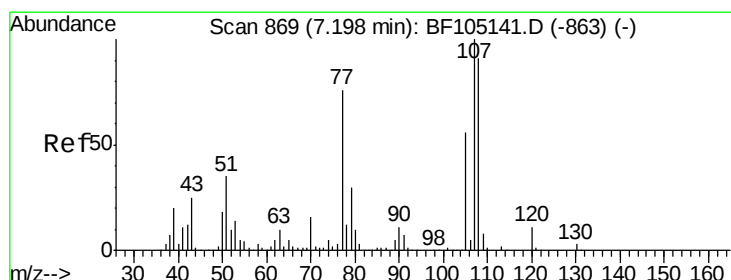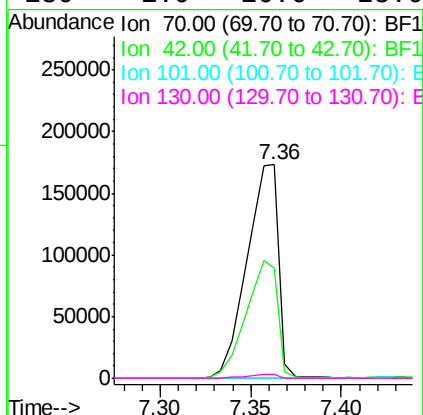

#20

3+4-Methylphenols

Concen: 0.008 ng

RT: 6.95 min Scan# 827

Delta R.T. -0.25 min

Lab File: BF105150.D

Acq: 8 May 2018 18:06

Tgt Ion: 107 Resp: 122


Ion Ratio Lower Upper


107 100

108 2359.2 68.2 108.2#

77 9008.1 26.7 66.7#

79 6707.5 6.3 46.3#




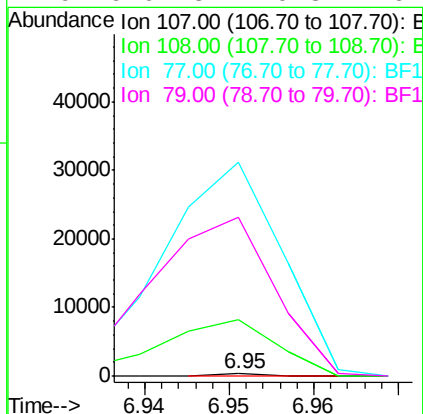




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.07 min Scan# 1018
Delta R.T. -0.00 min
Lab File: BF105150.D
Acq: 8 May 2018 18:06




Instrument :
BNA_F
ClientSampleId :


Tot Ion:136	Resp:	959145
Ion Ratio	Lower	Upper
136 100		
137 11.0	8.9	13.3
54 9.3	6.6	9.8
68 6.2	5.0	7.4

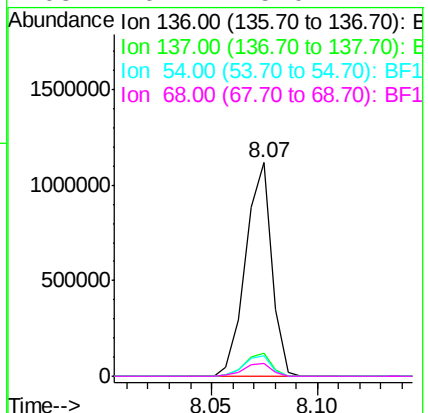

#22
Acetophenone
Concen: 0.015 ng
RT: 7.19 min Scan# 868
Delta R.T. -0.02 min
Lab File: BF105150.D
Acq: 8 May 2018 18:06

Tgt Ion:105	Resp:	325
Ion Ratio	Lower	Upper
105 100		
71 0.0	4.4	6.6#
51 94.7	22.3	33.5#
120 0.0	16.9	25.3#

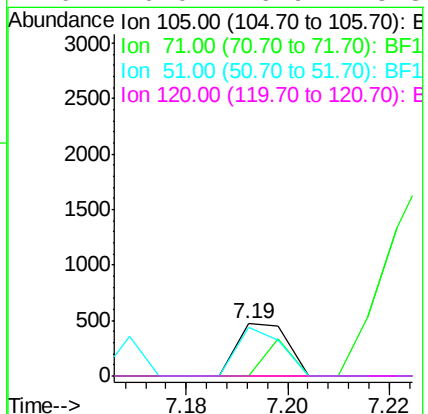







#23
Nitrobenzene-d5
Concen: 106.489 ng
RT: 7.36 min Scan# 897
Delta R.T. -0.00 min
Lab File: BF105150.D
Acq: 8 May 2018 18:06

Instrument :
BNA_F
ClientSampleId :

Tot Ion: 82 Resp: 1507047
Ion Ratio Lower Upper
82 100
128 47.5 36.1 54.1
54 57.4 41.4 62.2




Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): BF1
Ion 54.00 (53.70 to 54.70): BF1

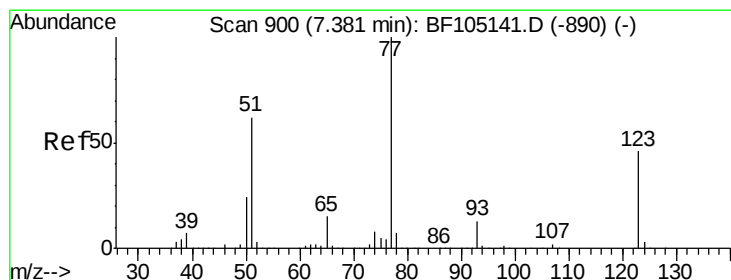
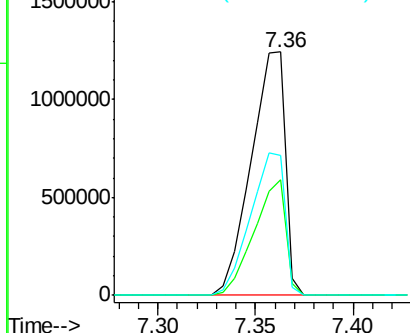



#24
Nitrobenzene
Concen: 0.313 ng
RT: 7.36 min Scan# 896
Delta R.T. -0.02 min
Lab File: BF105150.D
Acq: 8 May 2018 18:06

Tgt Ion: 77 Resp: 5018
Ion Ratio Lower Upper
77 100
123 0.0 37.9 56.9#
65 39.2 11.0 16.4#



Abundance Ion 77.00 (76.70 to 77.70): BF1
Ion 123.00 (122.70 to 123.70): BF1
Ion 65.00 (64.70 to 65.70): BF1

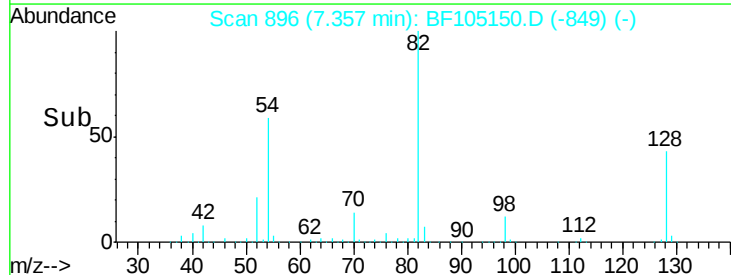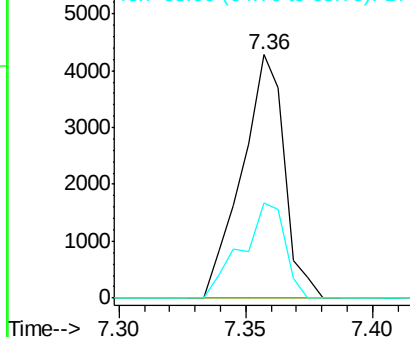



#25

Isophorone

Concen: 47.580 ng

RT: 7.36 min Scan# 897

Delta R.T. -0.25 min

Lab File: BF105150.D

Acq: 8 May 2018 18:06

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 82 Resp: 1505905

Ion Ratio Lower Upper




82 100

95 0.0 5.2 7.8#

138 0.0 14.9 22.3#



Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 95.00 (94.70 to 95.70): BF1
Ion 138.00 (137.70 to 138.70): BF1

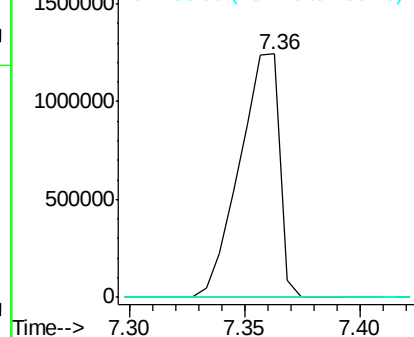

#27

2,4-Dimethylphenol

Concen: 0.014 ng

RT: 7.74 min Scan# 961

Delta R.T. 0.01 min

Lab File: BF105150.D

Acq: 8 May 2018 18:06


Tgt Ion: 122 Resp: 196

Ion Ratio Lower Upper



122 100


107 0.0 91.2 136.8#

121 0.0 47.2 70.8#



Abundance Ion 122.00 (121.70 to 122.70): E
Ion 107.00 (106.70 to 107.70): E
Ion 121.00 (120.70 to 121.70): E




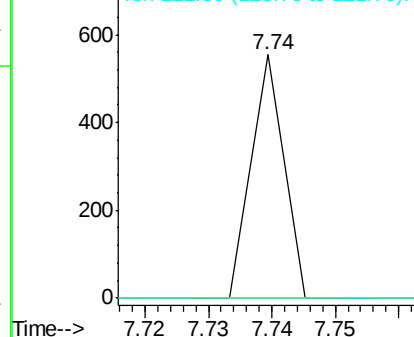


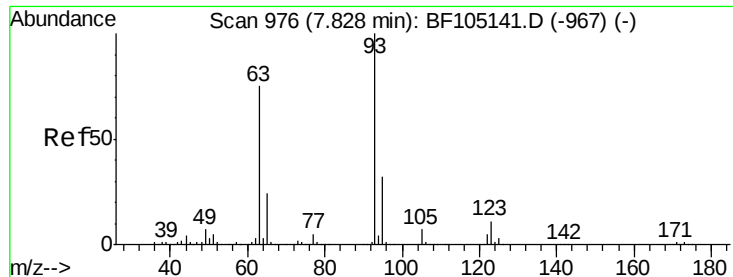

#28
bis(2-Chloroethoxy)methane
Concen: 0.013 ng
RT: 8.07 min Scan# 1018
Delta R.T. 0.25 min
Lab File: BF105150.D
Acq: 8 May 2018 18:06




Instrument :
BNA_F
ClientSampleId :


Tot Ion: 93 Resp: 256
Ion Ratio Lower Upper
93 100
95 177.5 26.3 39.5#
123 0.0 9.8 14.6#

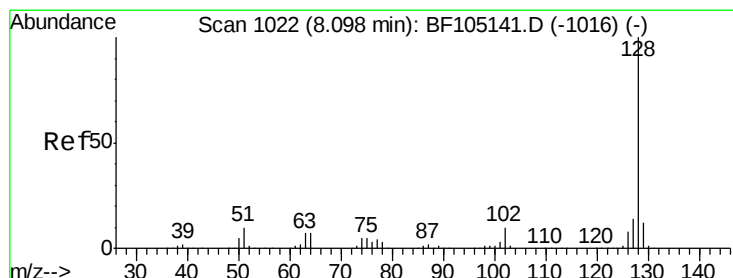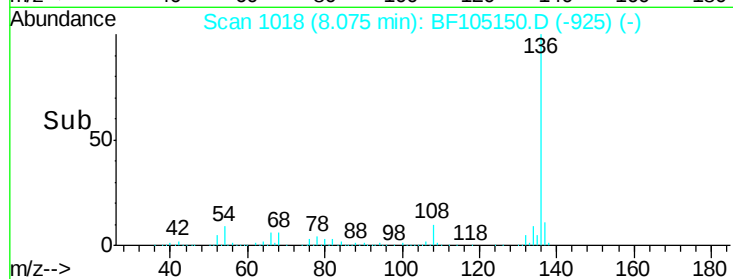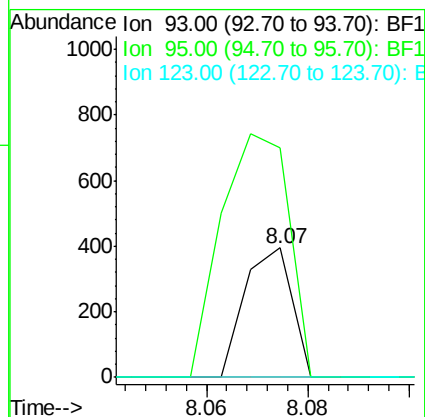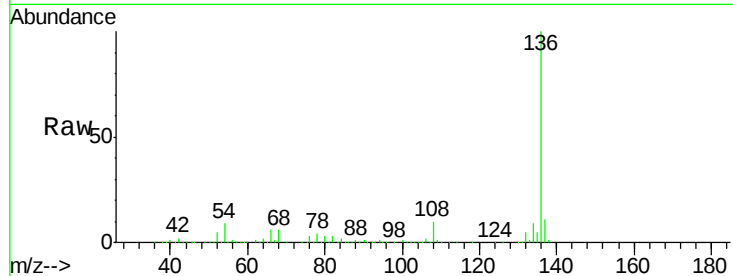

#31
Naphthalene
Concen: 0.019 ng
RT: 8.09 min Scan# 1021
Delta R.T. -0.01 min
Lab File: BF105150.D
Acq: 8 May 2018 18:06

Tgt Ion: 128 Resp: 888
Ion Ratio Lower Upper
128 100
129 0.0 8.8 13.2#
127 0.0 10.9 16.3#

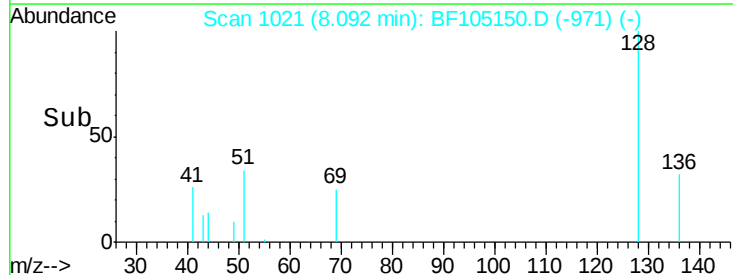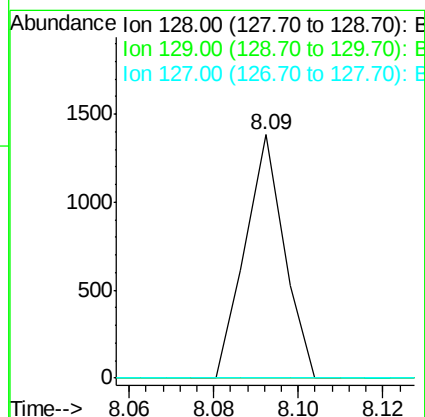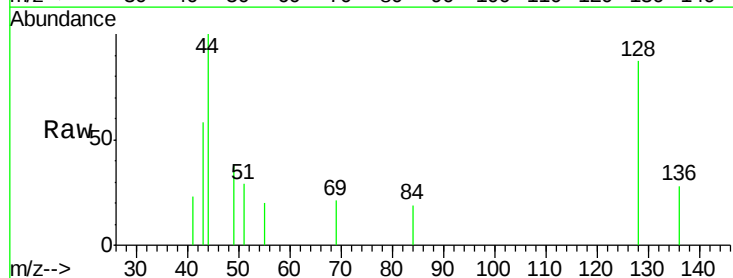







#32
Benzoic acid
Concen: 9.165 ng
RT: 7.74 min Scan# 961
Delta R.T. -0.10 min
Lab File: BF105150.D
Acq: 8 May 2018 18:06

Instrument :
BNA_F
ClientSampleId :

Tot Ion:122 Resp: 196
Ion Ratio Lower Upper
122 100
105 159.5 101.1 141.1#
77 116.2 70.7 110.7#




Abundance Ion 122.00 (121.70 to 122.70): E
Ion 105.00 (104.70 to 105.70): E
Ion 77.00 (76.70 to 77.70): BF1


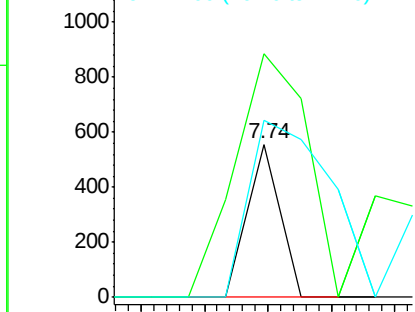



#36
4-Chloro-3-methylphenol
Concen: 0.021 ng
RT: 8.35 min Scan# 1065
Delta R.T. -0.27 min
Lab File: BF105150.D
Acq: 8 May 2018 18:06

Tgt Ion:107 Resp: 283
Ion Ratio Lower Upper
107 100
144 0.0 20.5 30.7#
142 0.0 62.0 93.0#



Abundance Ion 107.00 (106.70 to 107.70): E
Ion 144.00 (143.70 to 144.70): E
Ion 142.00 (141.70 to 142.70): E




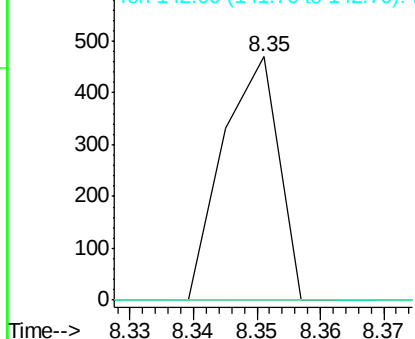




#37
2-Methylnaphthalene
Concen: 0.011 ng
RT: 8.79 min Scan# 1139
Delta R.T. -0.00 min
Lab File: BF105150.D
Acq: 8 May 2018 18:06




Instrument :
BNA_F
ClientSampleId :


Tot Ion:142 Resp: 339
Ion Ratio Lower Upper
142 100
141 0.0 70.8 106.2#
115 0.0 26.1 39.1#

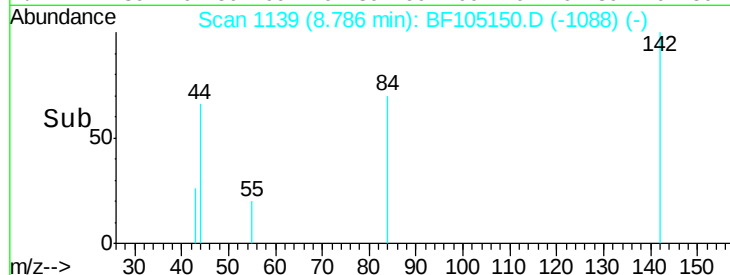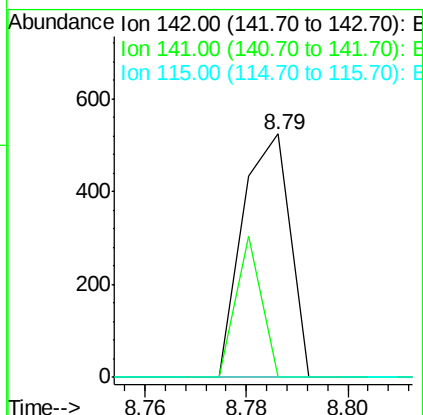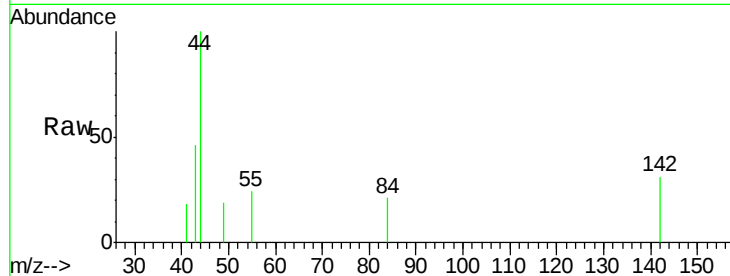

#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.83 min Scan# 1316
Delta R.T. -0.01 min
Lab File: BF105150.D
Acq: 8 May 2018 18:06

Tgt Ion:164 Resp: 472725
Ion Ratio Lower Upper
164 100
162 99.5 86.1 129.1
160 45.5 38.3 57.5



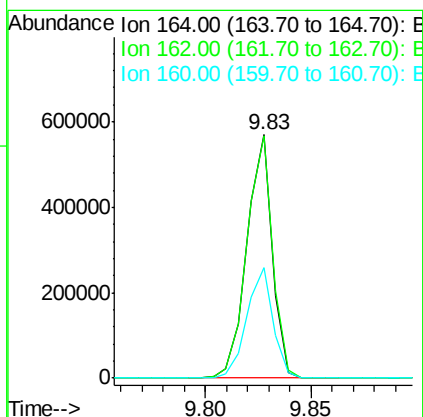





#41
 2,4,6-Tribromophenol
 Concen: 102.795 ng
 RT: 10.62 min Scan# 1450
 Delta R.T. -0.01 min
 Lab File: BF105150.D
 Acq: 8 May 2018 18:06




Instrument :
 BNA_F
 ClientSampleId :


Tot Ion	Ratio	Lower	Upper
330	100		
332	96.4	77.0	115.6
141	26.7	29.9	44.9#

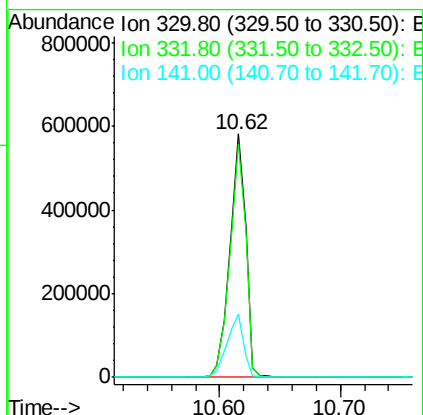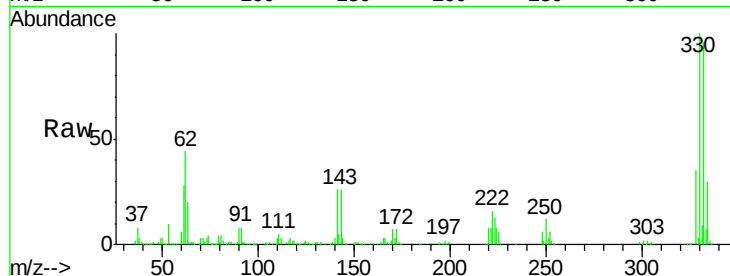

#44
 2-Fluorobiphenyl
 Concen: 86.570 ng
 RT: 9.16 min Scan# 1202
 Delta R.T. -0.00 min
 Lab File: BF105150.D
 Acq: 8 May 2018 18:06

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.9	29.7	44.5
170	24.1	19.6	29.4

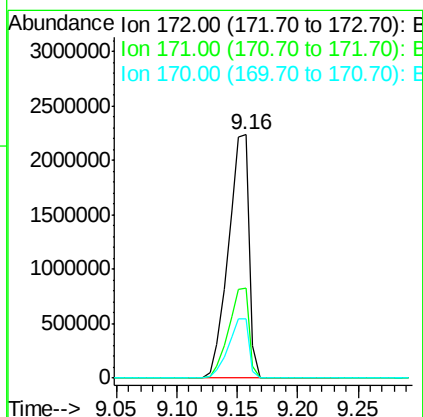







#45
 1,1'-Biphenyl
 Concen: 0.256 ng
 RT: 9.25 min Scan# 1217
 Delta R.T. -0.01 min
 Lab File: BF105150.D
 Acq: 8 May 2018 18:06

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:154 Resp: 9877
 Ion Ratio Lower Upper
 154 100
 153 40.3 21.3 61.3
 76 13.9 0.0 34.0




Abundance Ion 154.00 (153.70 to 154.70): E
 Ion 153.00 (152.70 to 153.70): E
 Ion 76.00 (75.70 to 76.70): BF1


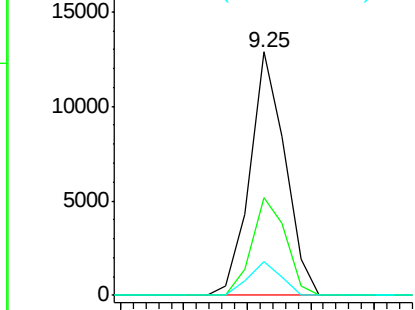



#46
 2-Chloronaphthalene
 Concen: 0.037 ng
 RT: 9.54 min Scan# 1267
 Delta R.T. 0.26 min
 Lab File: BF105150.D
 Acq: 8 May 2018 18:06

Tgt Ion:162 Resp: 1072
 Ion Ratio Lower Upper
 162 100
 127 0.0 33.9 50.9#
 164 1139.7 26.5 39.7#



Abundance Ion 162.00 (161.70 to 162.70): E
 Ion 127.00 (126.70 to 127.70): E
 Ion 164.00 (163.70 to 164.70): E



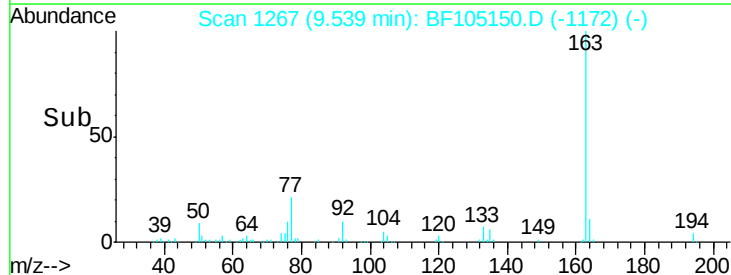
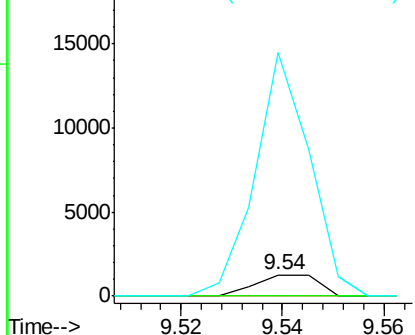




#47
2-Nitroaniline
Concen: 5.926 ng
RT: 9.54 min Scan# 1267
Delta R.T. 0.17 min
Lab File: BF105150.D
Acq: 8 May 2018 18:06




Instrument :
BNA_F
ClientSampleId :


Tot Ion: 65 Resp: 1200
Ion Ratio Lower Upper
65 100
92 684.8 55.8 83.6#
138 0.0 91.2 136.8#

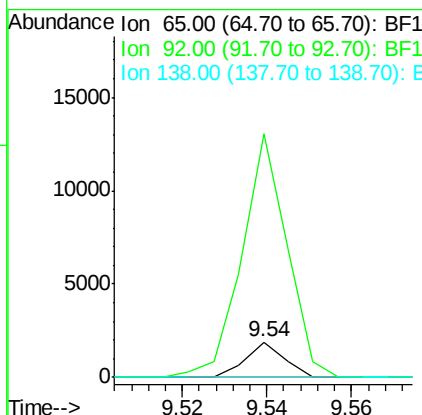

#49
Dimethylphthalate
Concen: 3.234 ng
RT: 9.54 min Scan# 1267
Delta R.T. -0.02 min
Lab File: BF105150.D
Acq: 8 May 2018 18:06

Tgt Ion:163 Resp: 103481
Ion Ratio Lower Upper
163 100
194 3.8 2.7 4.1
164 10.6 8.2 12.2

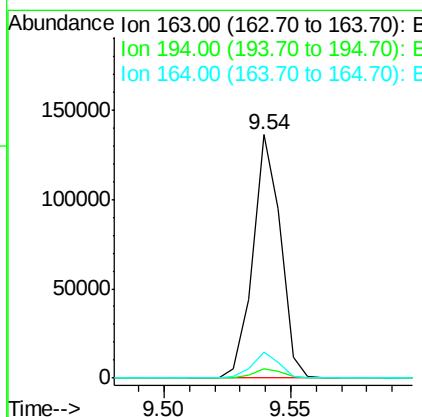







#50
 2,6-Dinitrotoluene
 Concen: 8.722 ng
 RT: 9.83 min Scan# 1316
 Delta R.T. 0.21 min
 Lab File: BF105150.D
 Acq: 8 May 2018 18:06

Instrument :
 BNA_F
 ClientSampled :

Tot Ion:165 Resp: 60569
 Ion Ratio Lower Upper
 165 100
 63 1.4 44.7 67.1#
 89 1.7 44.0 66.0#




Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BF1
 Ion 89.00 (88.70 to 89.70): BF1


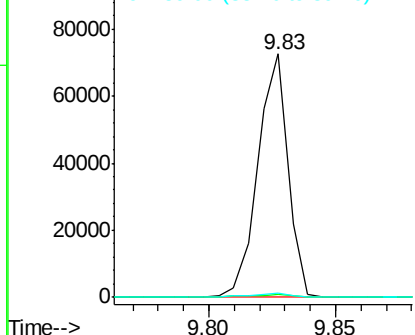



#51
 Acenaphthene
 Concen: 0.004 ng
 RT: 9.86 min Scan# 1321
 Delta R.T. -0.01 min
 Lab File: BF105150.D
 Acq: 8 May 2018 18:06

Tgt Ion:154 Resp: 110
 Ion Ratio Lower Upper
 154 100
 153 0.0 91.2 136.8#
 152 0.0 43.8 65.8#



Abundance Ion 154.00 (153.70 to 154.70): E
 Ion 153.00 (152.70 to 153.70): E
 Ion 152.00 (151.70 to 152.70): E

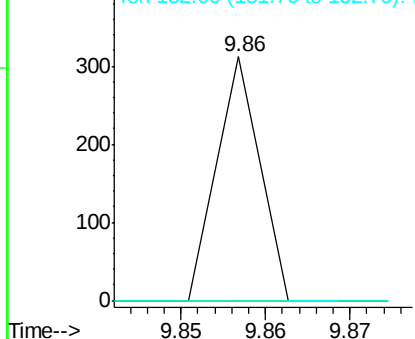



#52

3-Nitroaniline

Concen: 0.100 ng

RT: 9.93 min Scan# 1333

Delta R.T. 0.14 min

Lab File: BF105150.D

Acq: 8 May 2018 18:06

Instrument :

BNA_F

ClientSampleId :


Tot Ion:138 Resp: 732

Ion Ratio Lower Upper

138 100

108 0.0 9.4 14.0#




92 0.0 89.4 134.2#



Abundance Ion 138.00 (137.70 to 138.70): E

Ion 108.00 (107.70 to 108.70): E

Ion 92.00 (91.70 to 92.70): BF1

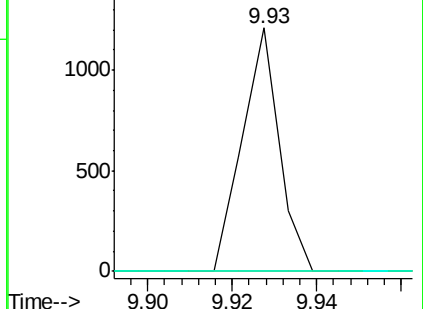

#54

Dibenzofuran

Concen: 0.008 ng

RT: 10.03 min Scan# 1350

Delta R.T. -0.01 min

Lab File: BF105150.D

Acq: 8 May 2018 18:06


Tgt Ion:168 Resp: 340

Ion Ratio Lower Upper

168 100

139 0.0 30.1 45.1#



169 0.0 10.9 16.3#




Abundance Ion 168.00 (167.70 to 168.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 169.00 (168.70 to 169.70): E




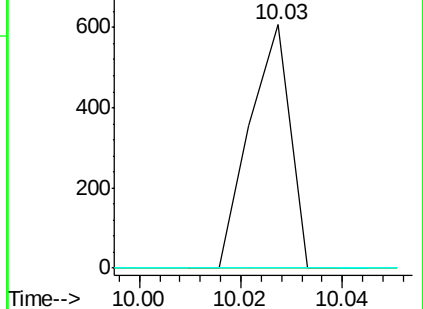




#56
 2,4-Dinitrotoluene
 Concen: 9.675 ng
 RT: 9.83 min Scan# 1316
 Delta R.T. -0.19 min
 Lab File: BF105150.D
 Acq: 8 May 2018 18:06




Instrument :
 BNA_F
 ClientSampled :


Tot Ion:165 Resp: 60569
 Ion Ratio Lower Upper
 165 100
 63 1.4 36.4 54.6#
 89 1.7 57.8 86.6#
 182 0.0 1.6 2.4#

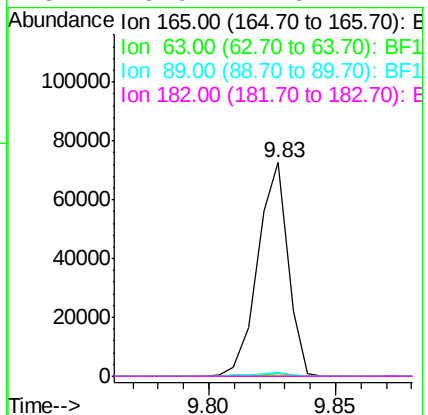

#57
 Fluorene
 Concen: 0.634 ng
 RT: 10.62 min Scan# 1450
 Delta R.T. 0.23 min
 Lab File: BF105150.D
 Acq: 8 May 2018 18:06

Tgt Ion:166 Resp: 19474
 Ion Ratio Lower Upper
 166 100
 165 99.3 79.8 119.8
 167 39.8 10.6 16.0#


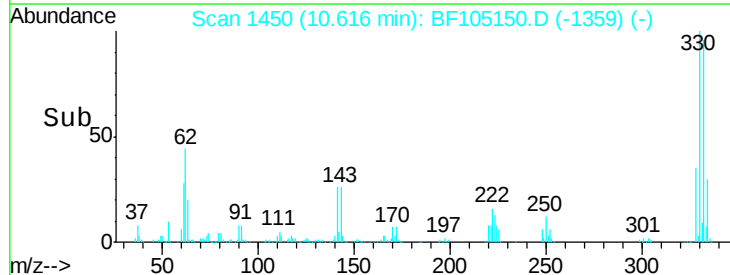
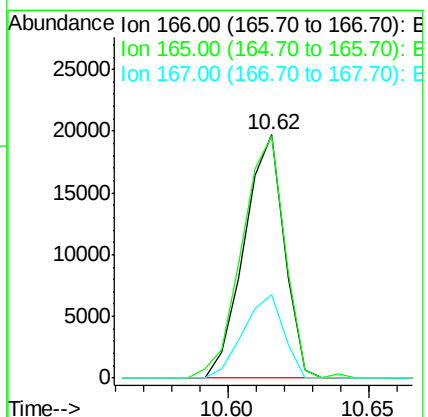





#59
 Diethylphthalate
 Concen: 0.334 ng
 RT: 10.25 min Scan# 1387
 Delta R.T. -0.01 min
 Lab File: BF105150.D
 Acq: 8 May 2018 18:06




Instrument :
 BNA_F
 ClientSampleId :


Tot Ion:149 Resp: 10518
 Ion Ratio Lower Upper
 149 100
 177 28.7 16.1 24.1#
 150 13.3 10.1 15.1

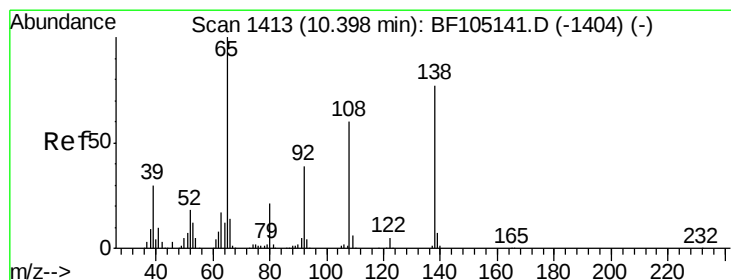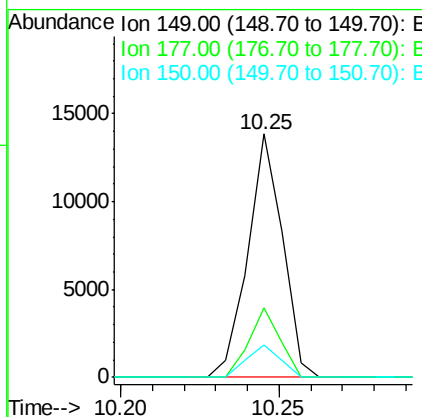

#61
 4-Nitroaniline
 Concen: 0.019 ng
 RT: 10.51 min Scan# 1432
 Delta R.T. 0.11 min
 Lab File: BF105150.D
 Acq: 8 May 2018 18:06

Tgt Ion:138 Resp: 137
 Ion Ratio Lower Upper
 138 100
 92 0.0 30.2 70.2#
 108 0.0 52.5 92.5#

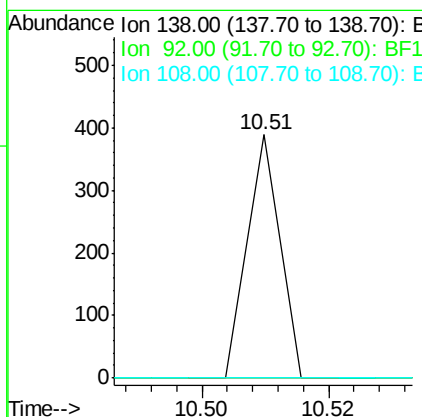







#62
Azobenzene
Concen: 0.033 ng
RT: 10.54 min Scan# 1438
Delta R.T. 0.01 min
Lab File: BF105150.D
Acq: 8 May 2018 18:06

Instrument :
BNA_F
ClientSampled :

Tot Ion: 77 Resp: 1085
Ion Ratio Lower Upper
77 100
182 0.0 1.7 41.7#
105 160.1 3.0 43.0#
51 70.0 9.9 49.9#




Abundance Ion 77.00 (76.70 to 77.70): BF1
Ion 182.00 (181.70 to 182.70): E
Ion 105.00 (104.70 to 105.70): E
Ion 51.00 (50.70 to 51.70): BF1

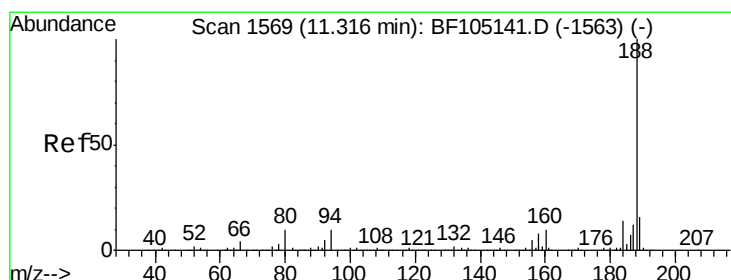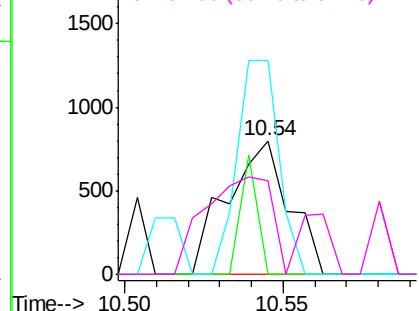




#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.32 min Scan# 1569
Delta R.T. -0.00 min
Lab File: BF105150.D
Acq: 8 May 2018 18:06

Tgt Ion: 188 Resp: 932522
Ion Ratio Lower Upper
188 100
94 8.4 8.5 12.7#
80 9.1 9.2 13.8#



Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF1
Ion 80.00 (79.70 to 80.70): BF1

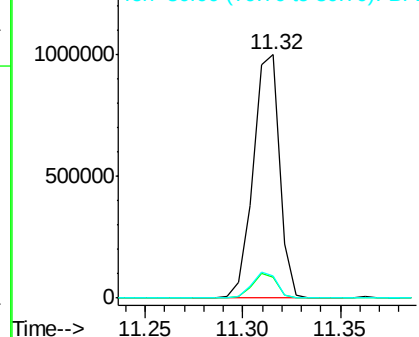



#64

4,6-Dinitro-2-methylphenol

Concen: 9.111 ng

RT: 10.62 min Scan# 1450

Delta R.T. 0.19 min

Lab File: BF105150.D

Acq: 8 May 2018 18:06

Instrument :

BNA_F

ClientSampleId :


Tot Ion:198 Resp: 1150

Ion Ratio Lower Upper

198 100

51 185.7 37.7 77.7#




105 153.8 36.3 76.3#

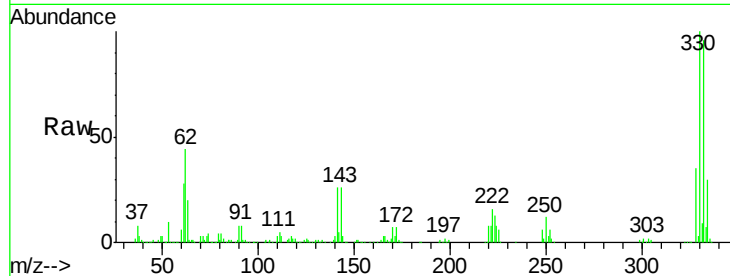

Abundance Ion 198.00 (197.70 to 198.70): E

Ion 51.00 (50.70 to 51.70): BF1

Ion 105.00 (104.70 to 105.70): E

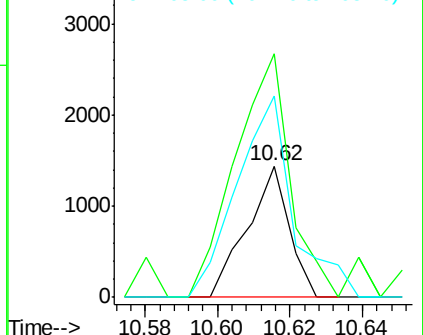

#65

n-Nitrosodiphenylamine

Concen: 0.483 ng

RT: 10.62 min Scan# 1450

Delta R.T. 0.12 min

Lab File: BF105150.D

Acq: 8 May 2018 18:06


Tgt Ion:169 Resp: 14047

Ion Ratio Lower Upper

169 100

168 7.5 54.4 81.6#



167 55.1 29.8 44.6#




Abundance Ion 169.00 (168.70 to 169.70): E

Ion 168.00 (167.70 to 168.70): E

Ion 167.00 (166.70 to 167.70): E

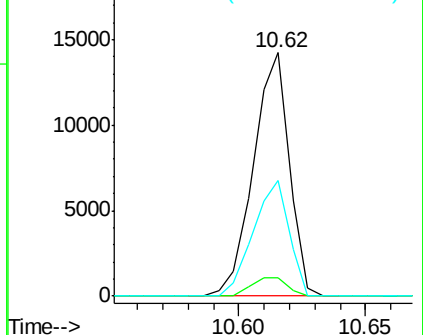







#66
4-Bromophenyl-phenylether
Concen: 3.085 ng
RT: 10.62 min Scan# 1450
Delta R.T. -0.25 min
Lab File: BF105150.D
Acq: 8 May 2018 18:06

Instrument :
BNA_F
ClientSampleId :

Tot Ion:248 Resp: 30684
Ion Ratio Lower Upper
248 100
250 206.0 76.9 115.3#
141 449.8 74.4 111.6#




Abundance Ion 248.00 (247.70 to 248.70): E
Ion 250.00 (249.70 to 250.70): E
Ion 141.00 (140.70 to 141.70): E


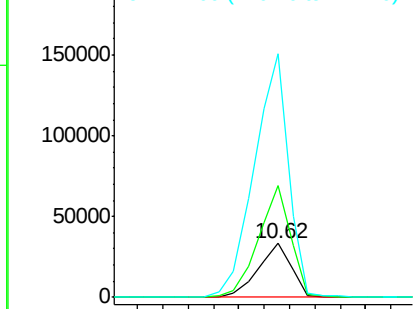



#70
Phenanthrene
Concen: 0.033 ng
RT: 11.33 min Scan# 1572
Delta R.T. -0.01 min
Lab File: BF105150.D
Acq: 8 May 2018 18:06

Tgt Ion:178 Resp: 1605
Ion Ratio Lower Upper
178 100
176 23.1 15.8 23.8
179 19.7 13.0 19.6#



Abundance Ion 178.00 (177.70 to 178.70): E
Ion 176.00 (175.70 to 176.70): E
Ion 179.00 (178.70 to 179.70): E




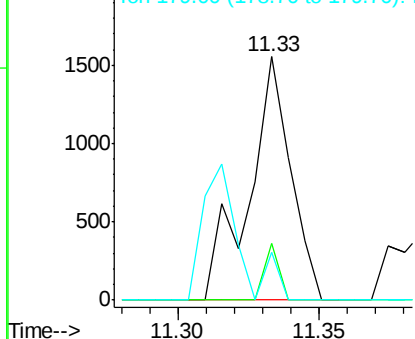




#71
 Anthracene
 Concen: 0.008 ng
 RT: 11.39 min Scan# 1581
 Delta R.T. -0.01 min
 Lab File: BF105150.D
 Acq: 8 May 2018 18:06




Instrument :
 BNA_F
 ClientSampled :


Tot Ion:178 Resp: 376
 Ion Ratio Lower Upper
 178 100
 176 0.0 15.4 23.2#
 179 0.0 12.6 19.0#

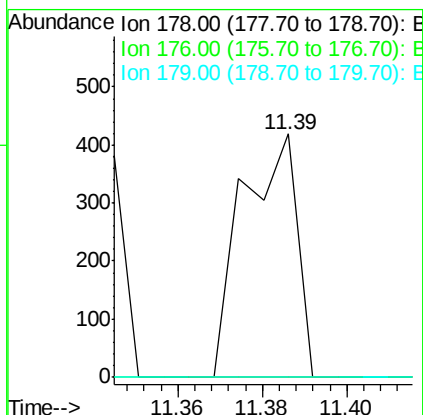

#73
 Di-n-butylphthalate
 Concen: 0.193 ng
 RT: 11.88 min Scan# 1665
 Delta R.T. -0.00 min
 Lab File: BF105150.D
 Acq: 8 May 2018 18:06

Tgt Ion:149 Resp: 9304
 Ion Ratio Lower Upper
 149 100
 150 13.0 7.8 11.6#
 104 6.5 3.8 5.8#



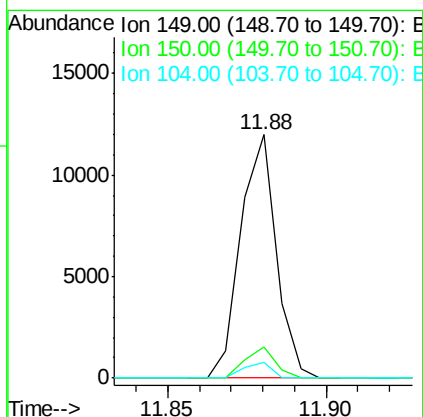





#74
Fluoranthene
Concen: 0.012 ng
RT: 12.52 min Scan# 1774
Delta R.T. -0.01 min
Lab File: BF105150.D
Acq: 8 May 2018 18:06




Instrument :
BNA_F
ClientSampled :


Tot Ion:202 Resp: 639
Ion Ratio Lower Upper
202 100
101 0.0 0.0 34.1
203 0.0 0.0 38.1

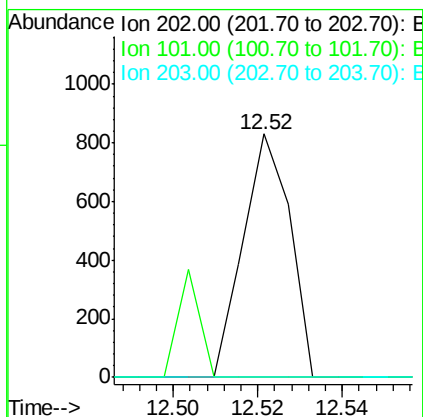

#75
Chrysene-d12
Concen: 20.000 ng
RT: 14.00 min Scan# 2026
Delta R.T. -0.01 min
Lab File: BF105150.D
Acq: 8 May 2018 18:06

Tgt Ion:240 Resp: 816944
Ion Ratio Lower Upper
240 100
120 10.7 9.5 14.3
236 26.5 20.7 31.1



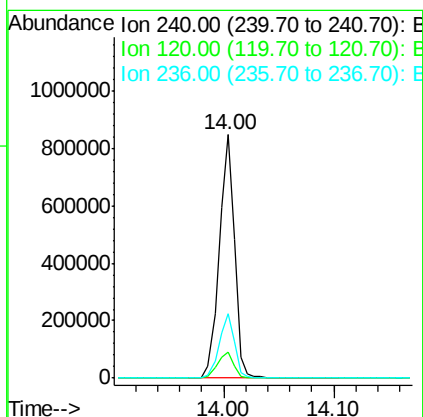





#76
Benzidine
Concen: 1.239 ng
RT: 12.91 min Scan# 1840
Delta R.T. 0.25 min
Lab File: BF105150.D
Acq: 8 May 2018 18:06




Instrument :
BNA_F
ClientSampleId :


Tot Ion:184 Resp: 37790
Ion Ratio Lower Upper
184 100
185 15.4 12.6 18.8
183 8.1 9.3 13.9#

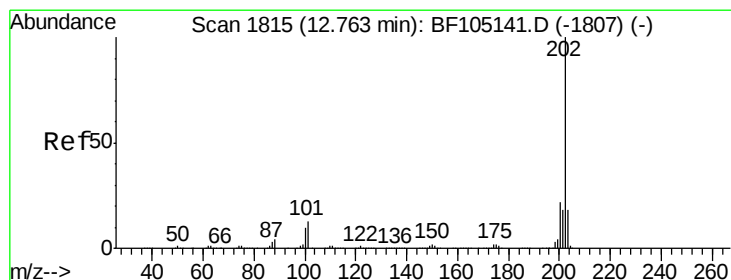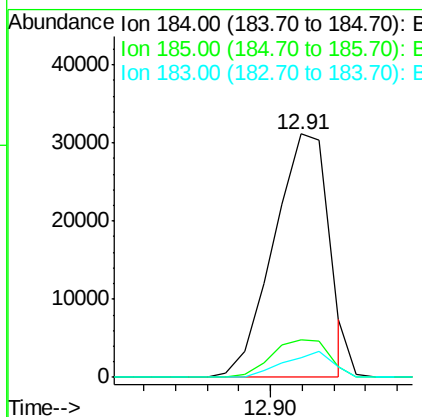

#77
Pyrene
Concen: 0.009 ng
RT: 12.74 min Scan# 1812
Delta R.T. -0.02 min
Lab File: BF105150.D
Acq: 8 May 2018 18:06

Tgt Ion:202 Resp: 514
Ion Ratio Lower Upper
202 100
200 0.0 17.4 26.2#
203 0.0 14.3 21.5#


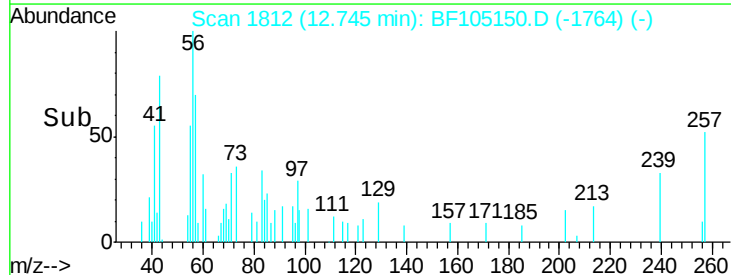
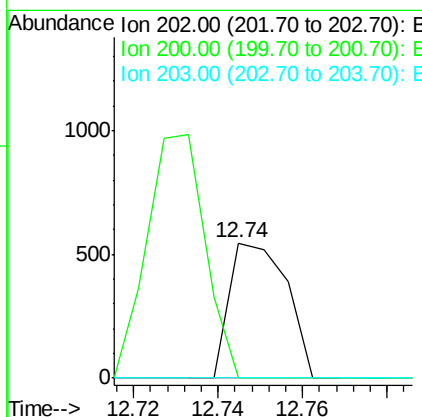
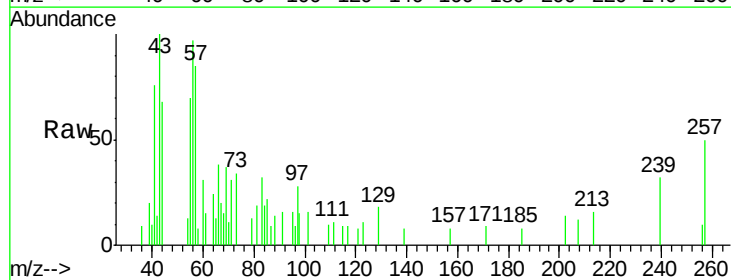




#78
 Terphenyl-d14
 Concen: 83.880 ng
 RT: 12.92 min Scan# 1841
 Delta R.T. 0.01 min
 Lab File: BF105150.D
 Acq: 8 May 2018 18:06




Instrument :
 BNA_F
 ClientSampleId :


Tot Ion:244 Resp: 2950037
 Ion Ratio Lower Upper
 244 100
 212 7.3 5.4 8.0
 122 9.9 11.0 16.4#

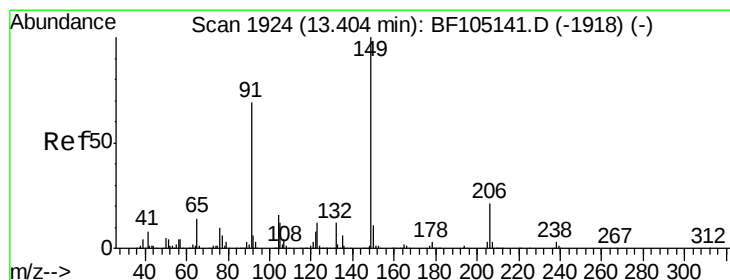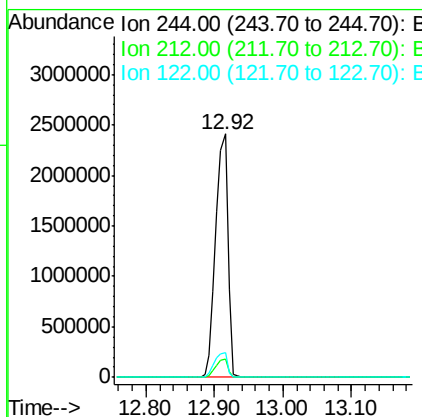

#79
 Butylbenzylphthalate
 Concen: 6.919 ng
 RT: 13.39 min Scan# 1922
 Delta R.T. -0.01 min
 Lab File: BF105150.D
 Acq: 8 May 2018 18:06

Tgt Ion:149 Resp: 480
 Ion Ratio Lower Upper
 149 100
 91 101.4 56.8 85.2#
 206 0.0 14.1 21.1#

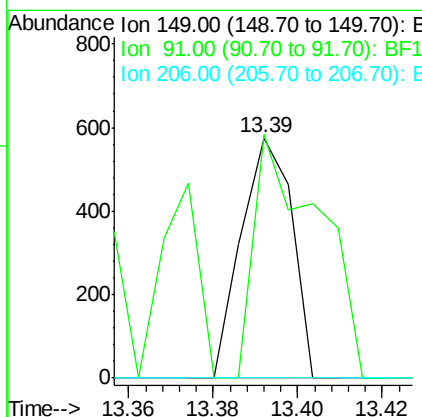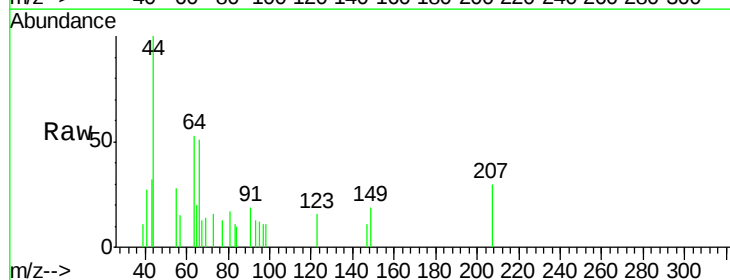



#80

Benzo(a)anthracene

Concen: 0.046 ng

RT: 14.00 min Scan# 2026

Delta R.T. 0.01 min

Lab File: BF105150.D

Acq: 8 May 2018 18:06

Instrument :

BNA_F

ClientSampleId :


Tot Ion:228 Resp: 2284

Ion Ratio Lower Upper

228 100

226 0.0 22.6 33.8#




229 34.1 15.8 23.6#



Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

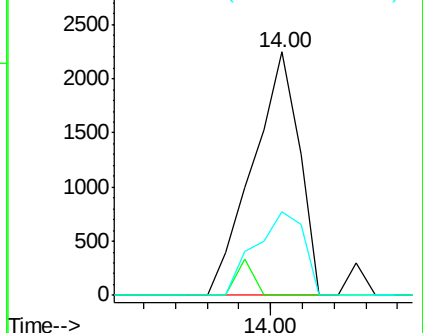

#82

Chrysene

Concen: 0.002 ng

RT: 14.03 min Scan# 2030

Delta R.T. -0.01 min

Lab File: BF105150.D

Acq: 8 May 2018 18:06


Tgt Ion:228 Resp: 107

Ion Ratio Lower Upper

228 100

226 0.0 25.0 37.6#



229 0.0 16.2 24.4#




Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

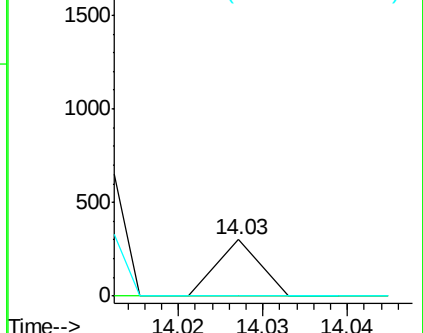



#83

Bis(2-ethylhexyl)phthalate

Concen: 0.117 ng

RT: 13.99 min Scan# 2024

Delta R.T. -0.01 min

Lab File: BF105150.D

Acq: 8 May 2018 18:06

Instrument :

BNA_F

ClientSampleId :


Tot Ion:149 Resp: 2886

Ion Ratio Lower Upper

149 100

167 21.3 21.3 31.9




279 0.0 3.0 4.4#



Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

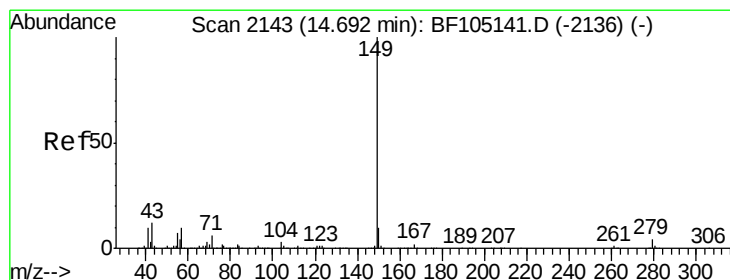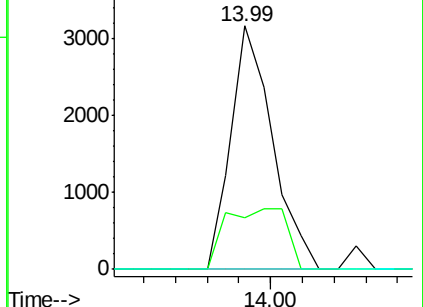

#84

Di-n-octyl phthalate

Concen: 6.937 ng

RT: 14.64 min Scan# 2135

Delta R.T. -0.05 min

Lab File: BF105150.D

Acq: 8 May 2018 18:06


Tgt Ion:149 Resp: 109

Ion Ratio Lower Upper

149 100

167 0.0 1.2 1.8#



43 0.0 8.4 12.6#




Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 43.00 (42.70 to 43.70): BF1




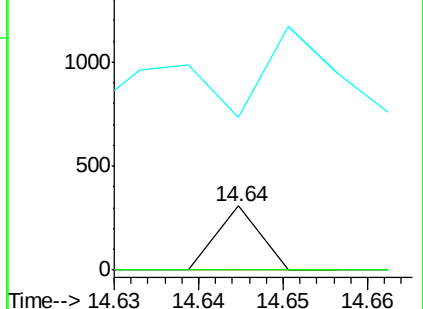




#86
Pervlene-d12
Concen: 20.000 ng
RT: 15.56 min Scan# 2290
Delta R.T. -0.00 min
Lab File: BF105150.D
Acq: 8 May 2018 18:06




Instrument :
BNA_F
ClientSampleId :


Tot Ion:264 Resp: 644378
Ion Ratio Lower Upper
264 100
260 24.9 19.2 28.8
265 21.4 17.5 26.3

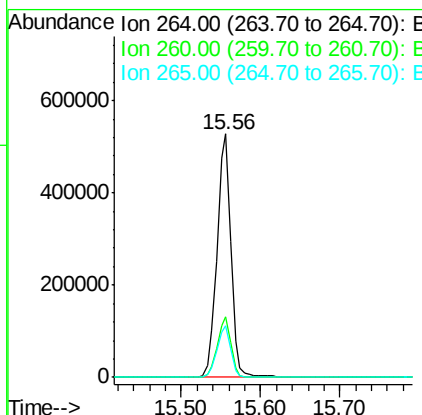

#87
Benzo(b)fluoranthene
Concen: 0.003 ng
RT: 15.12 min Scan# 2216
Delta R.T. -0.01 min
Lab File: BF105150.D
Acq: 8 May 2018 18:06

Tgt Ion:252 Resp: 122
Ion Ratio Lower Upper
252 100
253 0.0 17.0 25.6#
125 0.0 9.0 13.6#

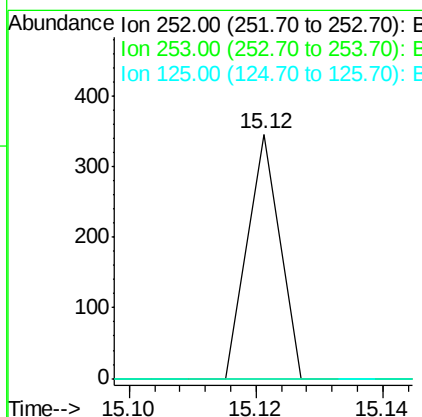







#88
Benzo(k)fluoranthene
Concen: 0.003 ng
RT: 15.12 min Scan# 2216
Delta R.T. -0.05 min
Lab File: BF105150.D
Acq: 8 May 2018 18:06

Instrument :
BNA_F
ClientSampleId :

Tot Ion:252 Resp: 122
Ion Ratio Lower Upper
252 100
253 0.0 17.9 26.9#
125 0.0 10.2 15.2#




Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

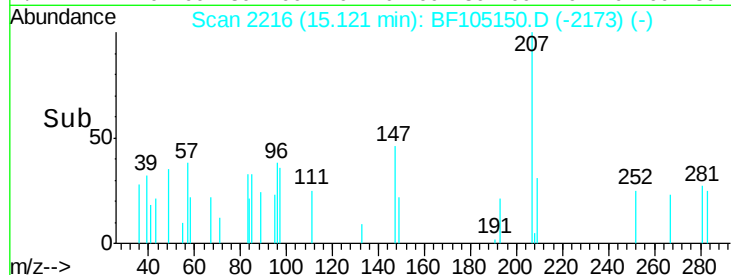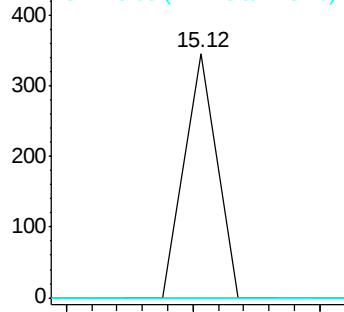

#89
Benzo(a)pyrene
Concen: 0.060 ng
RT: 15.55 min Scan# 2289
Delta R.T. 0.05 min
Lab File: BF105150.D
Acq: 8 May 2018 18:06

Tgt Ion:252 Resp: 2140
Ion Ratio Lower Upper
252 100
253 32.5 17.1 25.7#
125 23.2 9.8 14.6#



Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

