



Method Name: Z:\HPCHEM1\BNA\_F\METHODS\8270-BF050818.M  
Calibration Table Last Updated: Wed May 09 12:00:41 2018

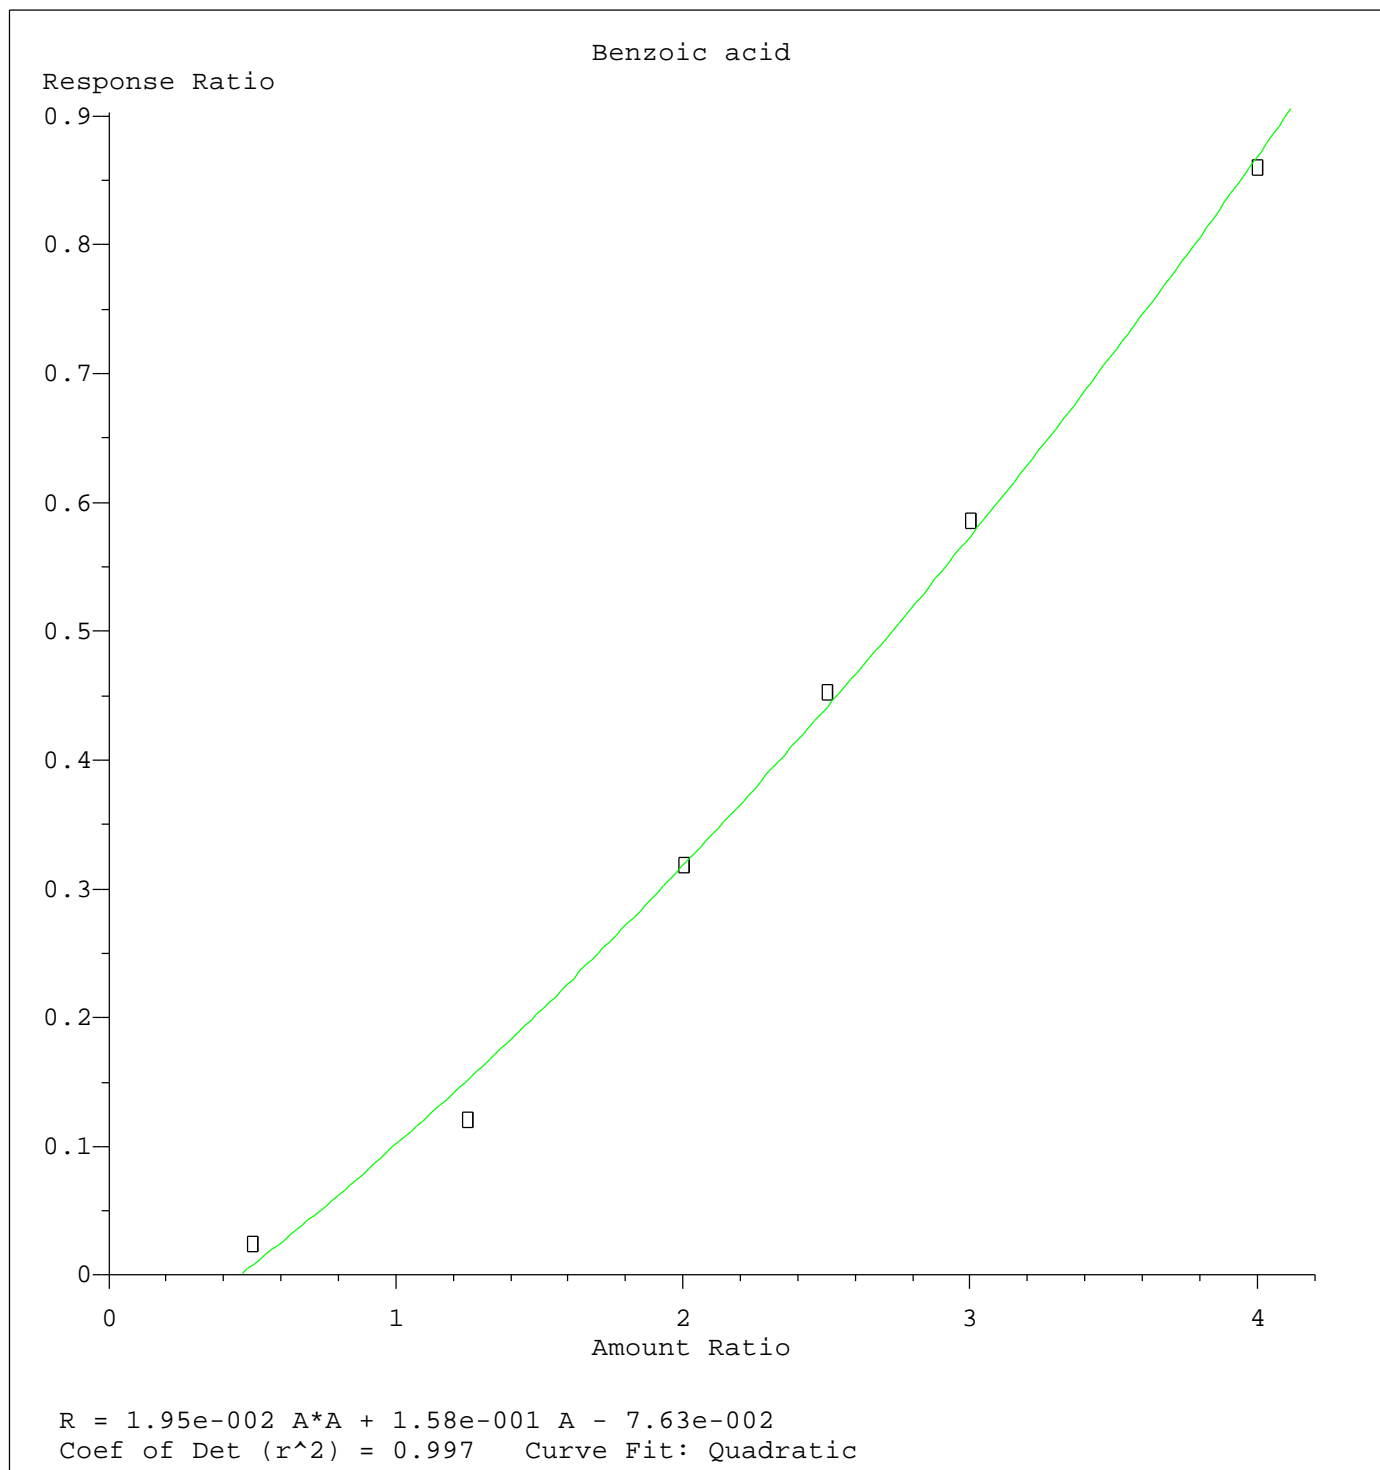

Method Name: Z:\HPCHEM1\BNA\_F\METHODS\8270-BF050818.M  
Calibration Table Last Updated: Wed May 09 12:00:41 2018

# 2-Nitroaniline


Response Ratio

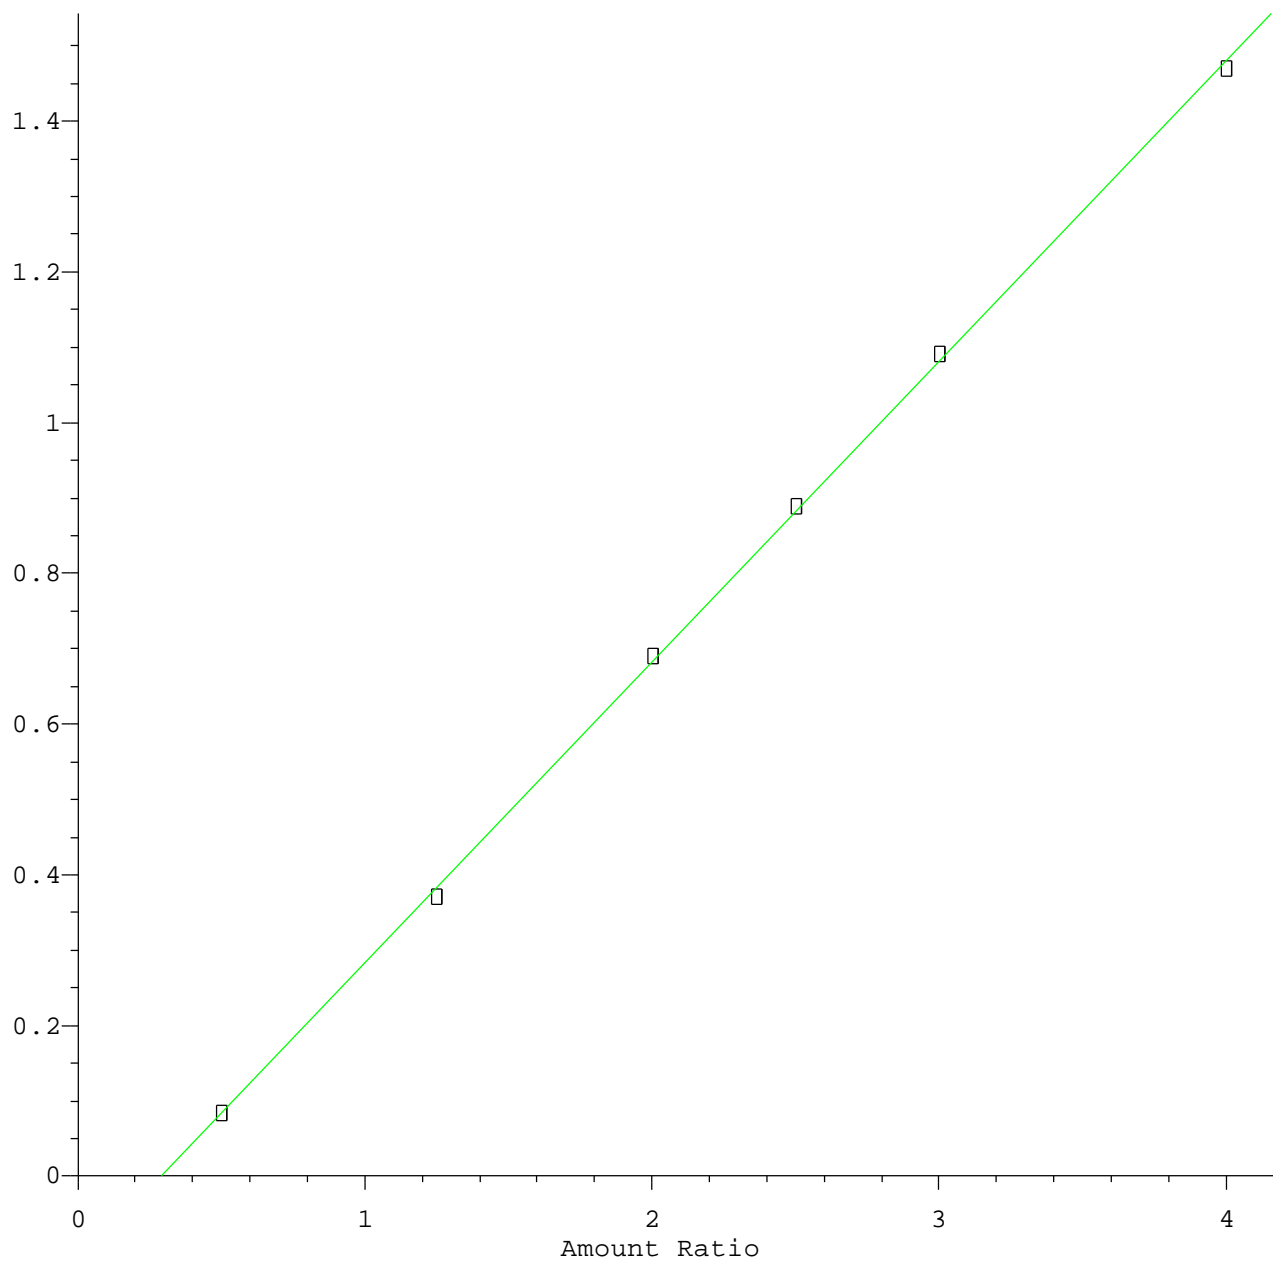

Resp Ratio = 3.99e-001 \* Amt - 1.16e-001  
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA\_F\METHODS\8270-BF050818.M  
Calibration Table Last Updated: Wed May 09 12:00:41 2018

# 2,4-Dinitrophenol

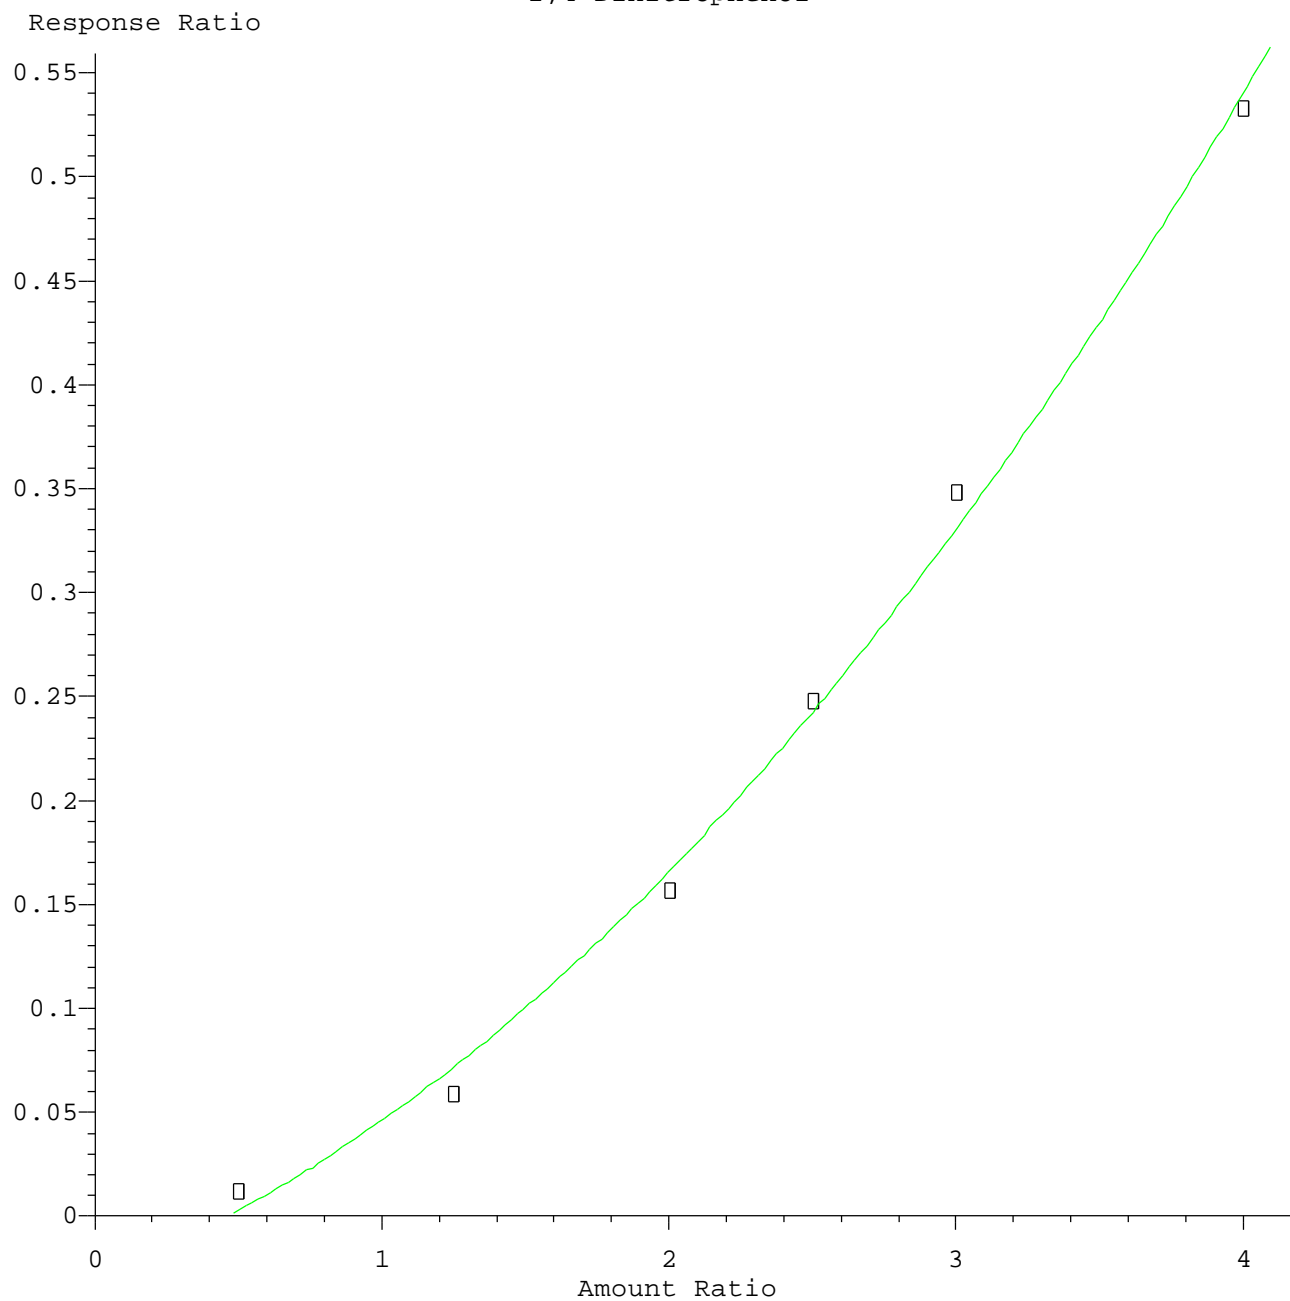


$R = 2.24e-002 A^2 + 5.28e-002 A - 2.94e-002$   
Coef of Det ( $r^2$ ) = 0.996    Curve Fit: Quadratic

Method Name: Z:\HPCHEM1\BNA\_F\METHODS\8270-BF050818.M  
Calibration Table Last Updated: Wed May 09 12:00:41 2018

# 4-Nitrophenol

Response Ratio

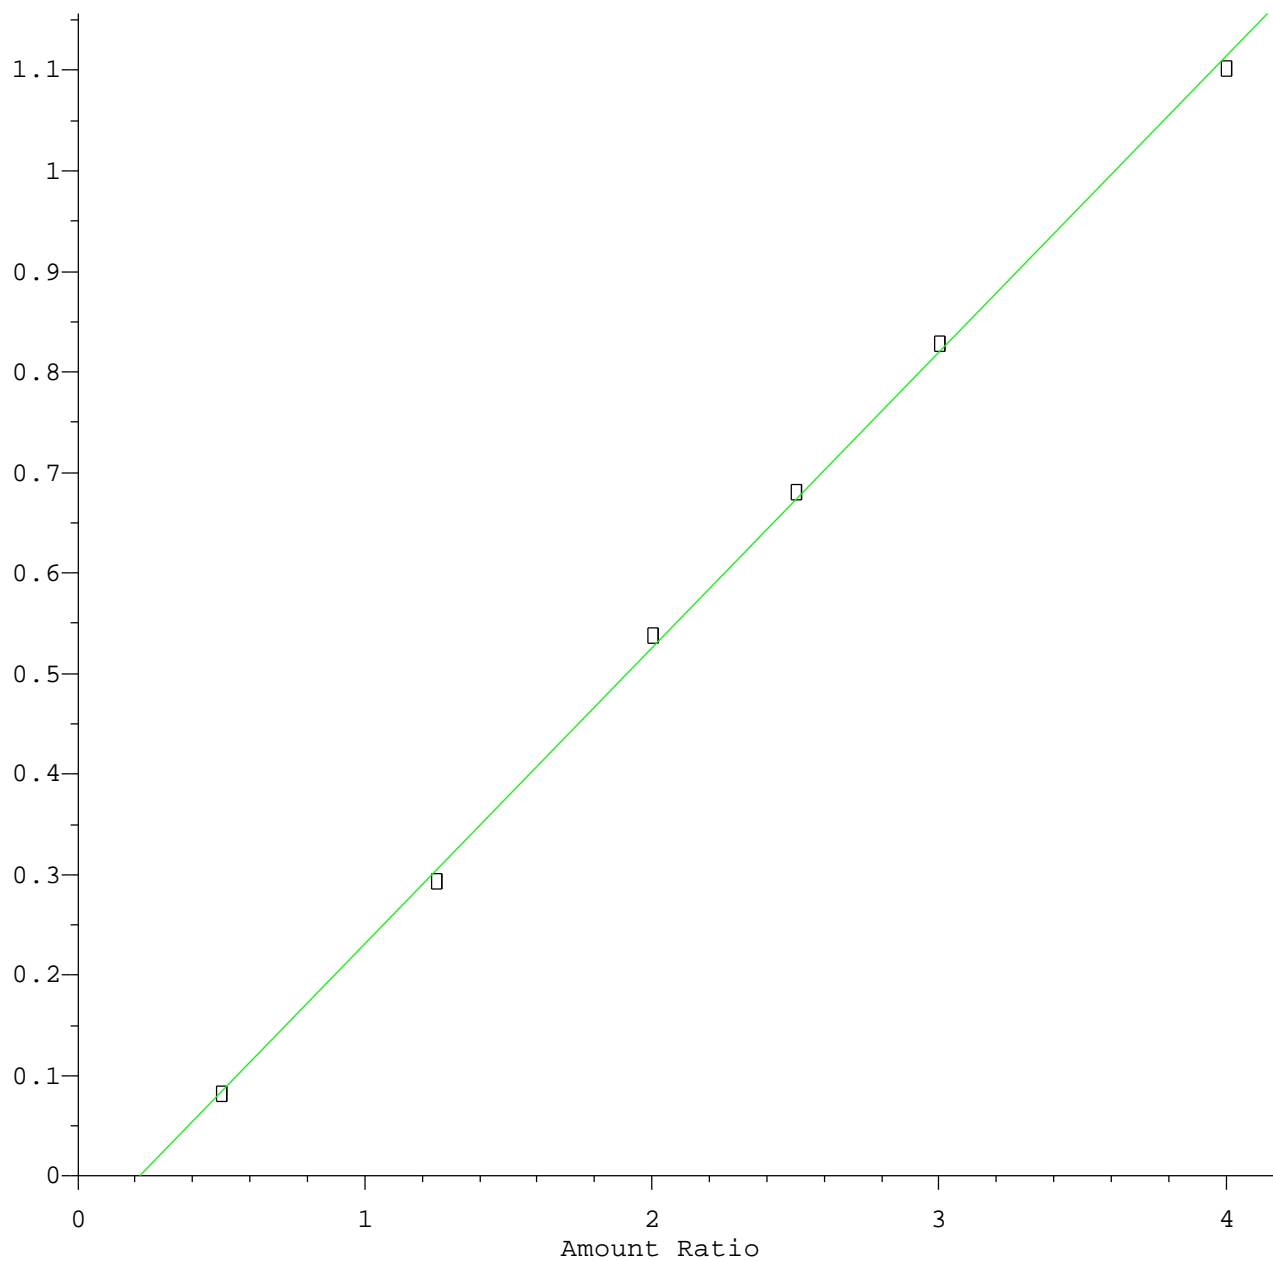


Resp Ratio =  $2.94 \times 10^{-1} \times \text{Amt} - 6.33 \times 10^{-2}$   
Coef of Det ( $r^2$ ) = 0.999    Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA\_F\METHODS\8270-BF050818.M  
Calibration Table Last Updated: Wed May 09 12:00:41 2018

2,4-Dinitrotoluene


Response Ratio

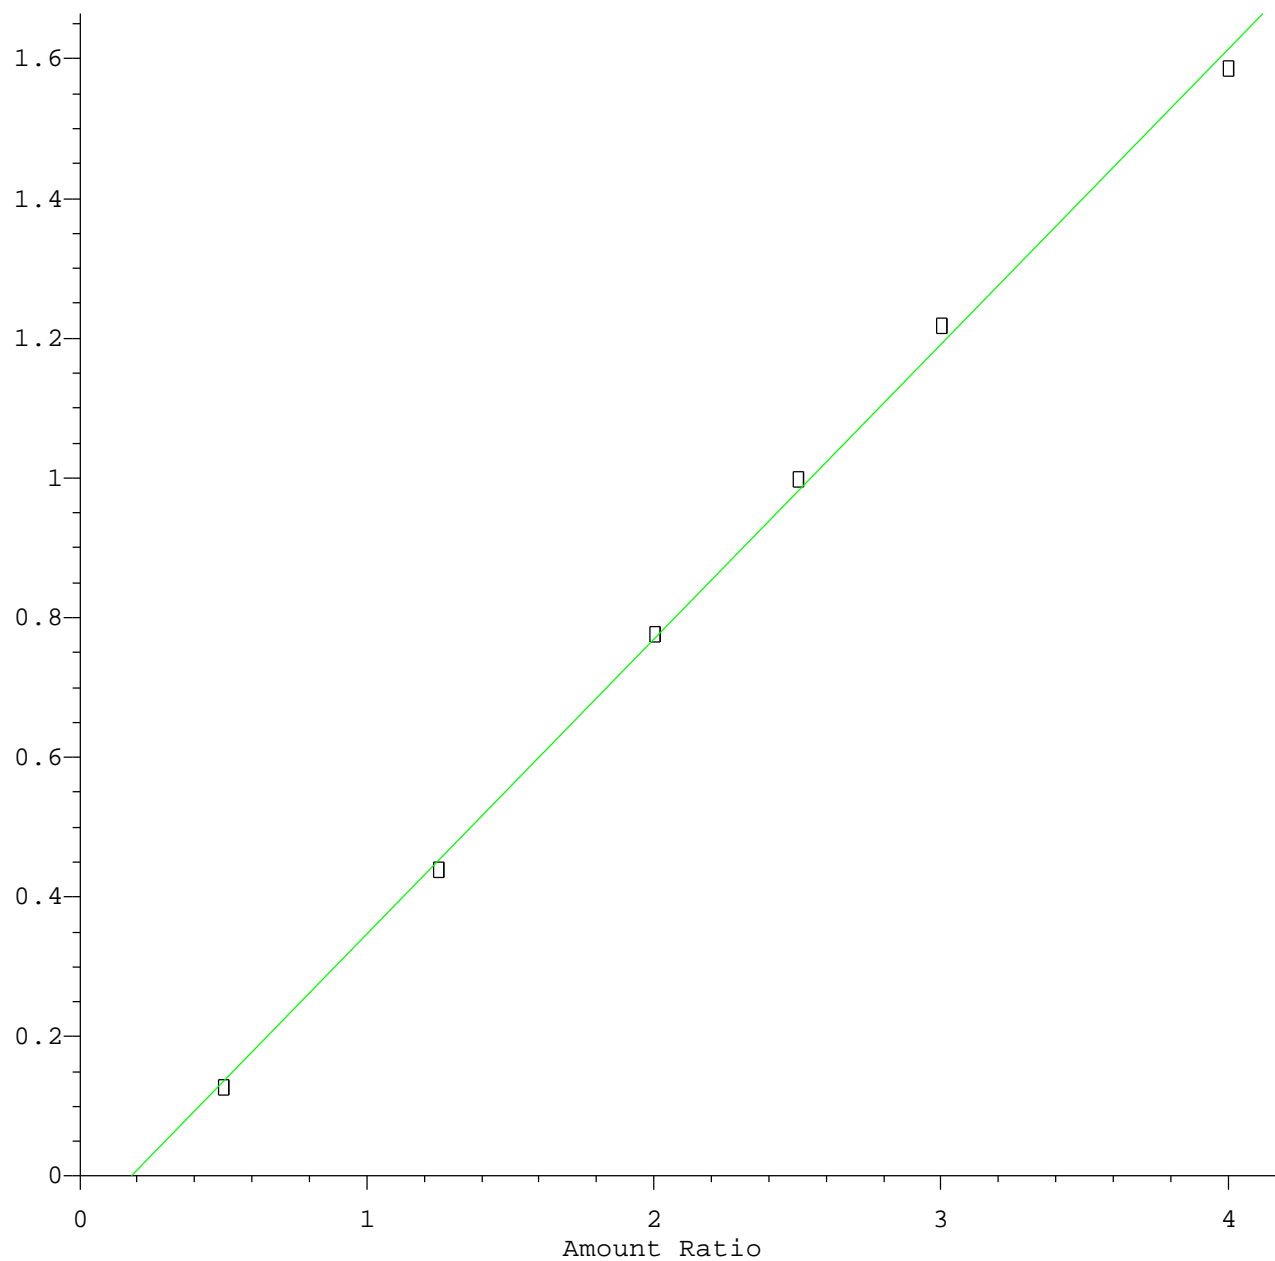

Resp Ratio = 4.22e-001 \* Amt - 7.62e-002  
Coef of Det (r^2) = 0.999 Curve Fit: Linear


Method Name: Z:\HPCHEM1\BNA\_F\METHODS\8270-BF050818.M  
Calibration Table Last Updated: Wed May 09 12:00:41 2018

4,6-Dinitro-2-methylphenol

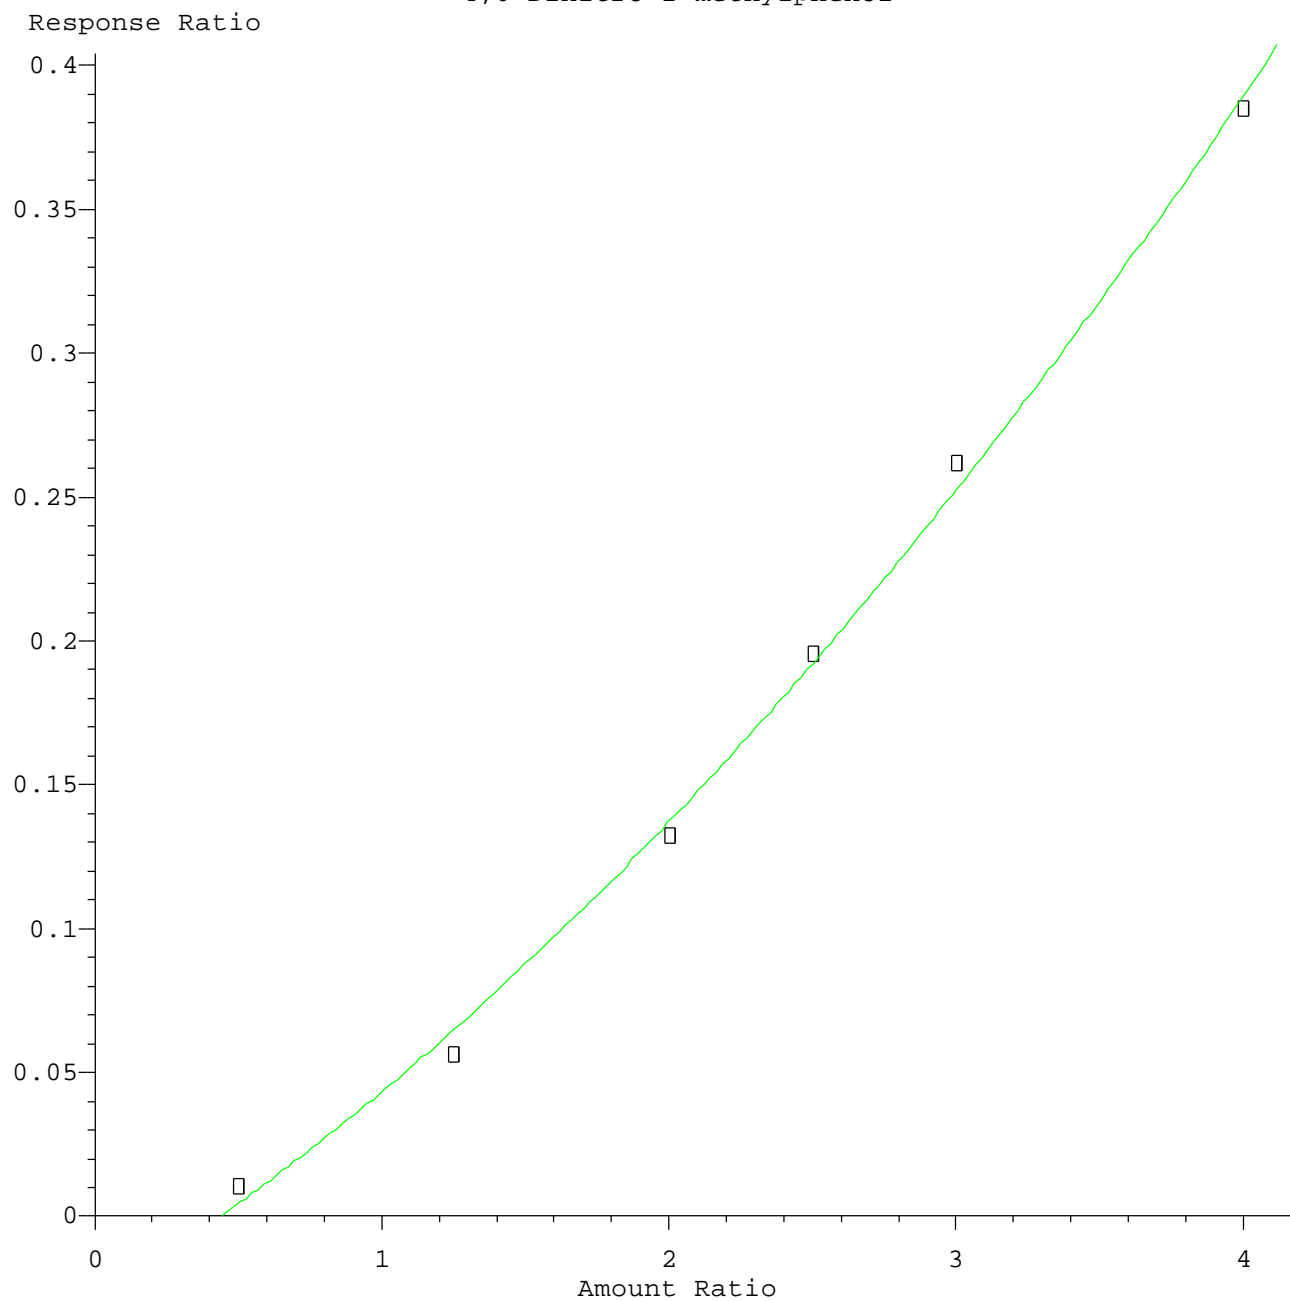


$R = 1.07e-002 A^2 + 6.16e-002 A - 2.91e-002$   
Coef of Det ( $r^2$ ) = 0.997    Curve Fit: Quadratic

Method Name: Z:\HPCHEM1\BNA\_F\METHODS\8270-BF050818.M  
Calibration Table Last Updated: Wed May 09 12:00:41 2018

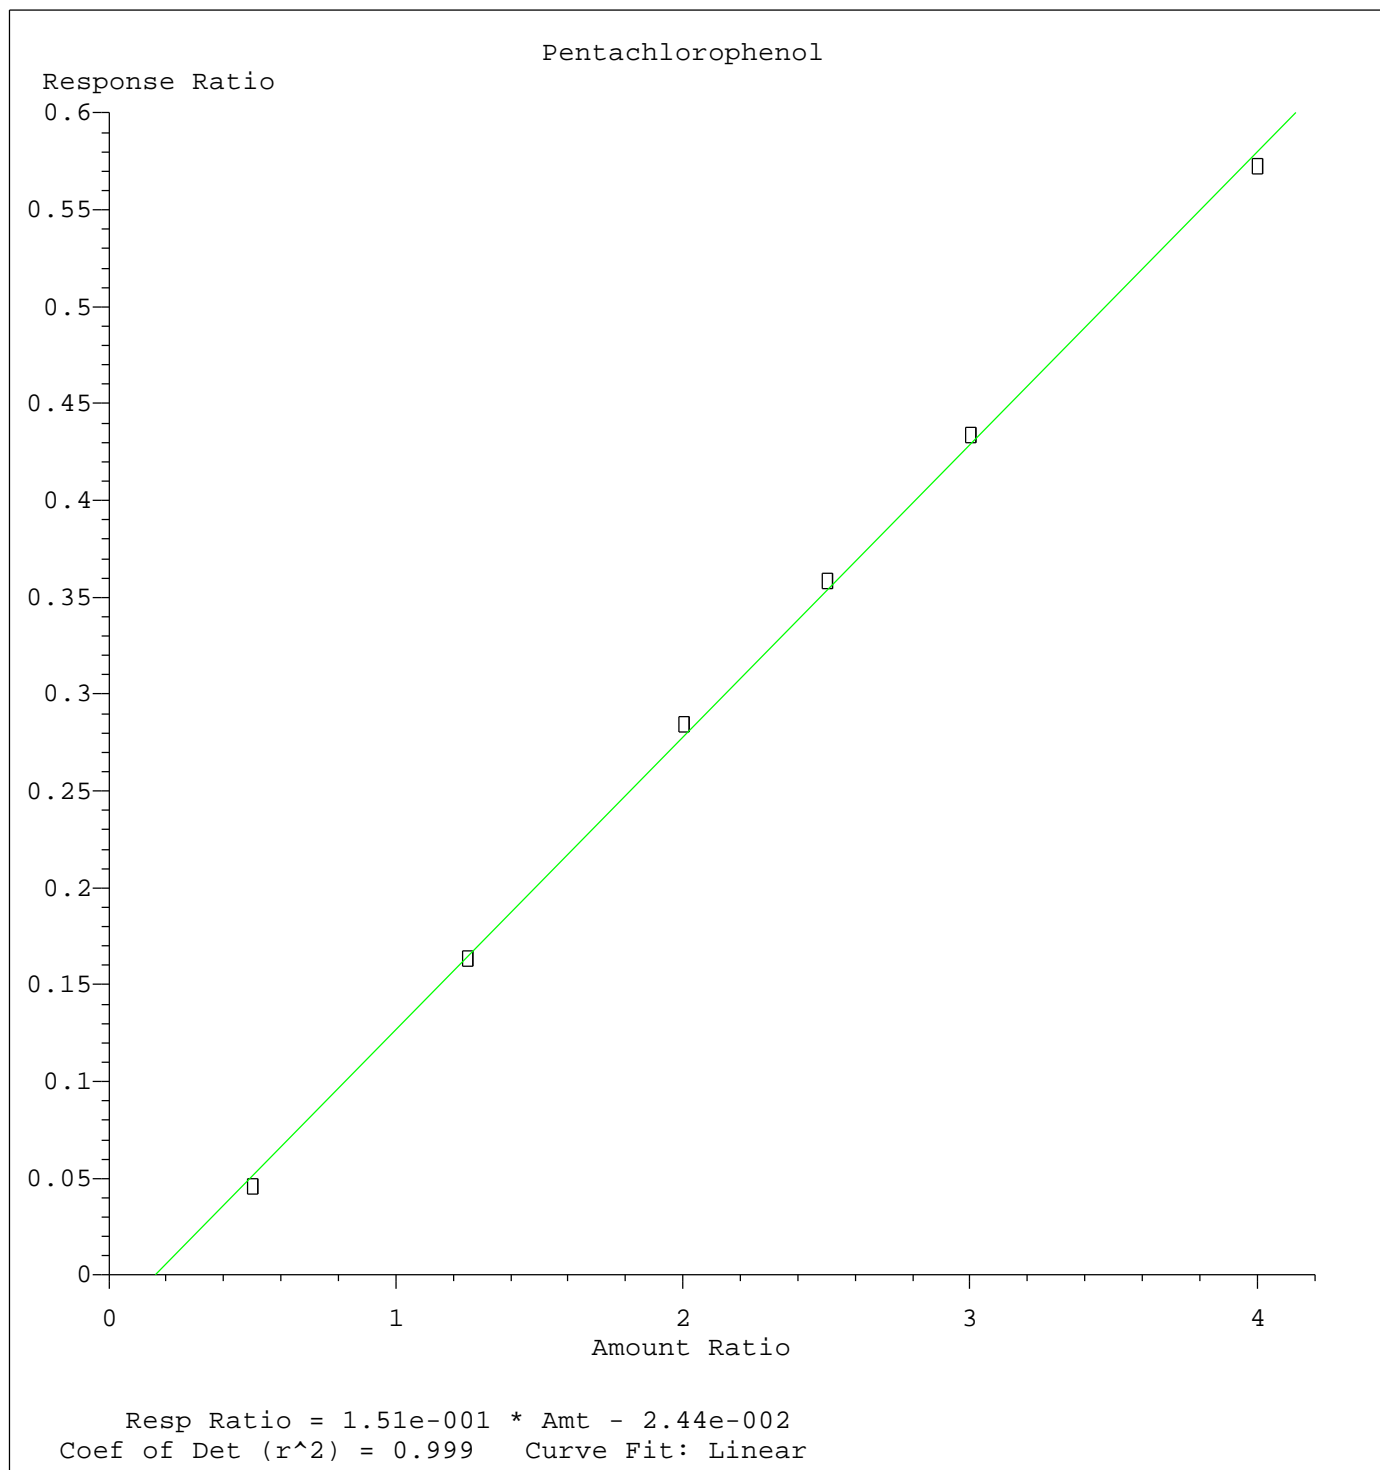


Method Name: Z:\HPCHEM1\BNA\_F\METHODS\8270-BF050818.M  
Calibration Table Last Updated: Wed May 09 12:00:41 2018



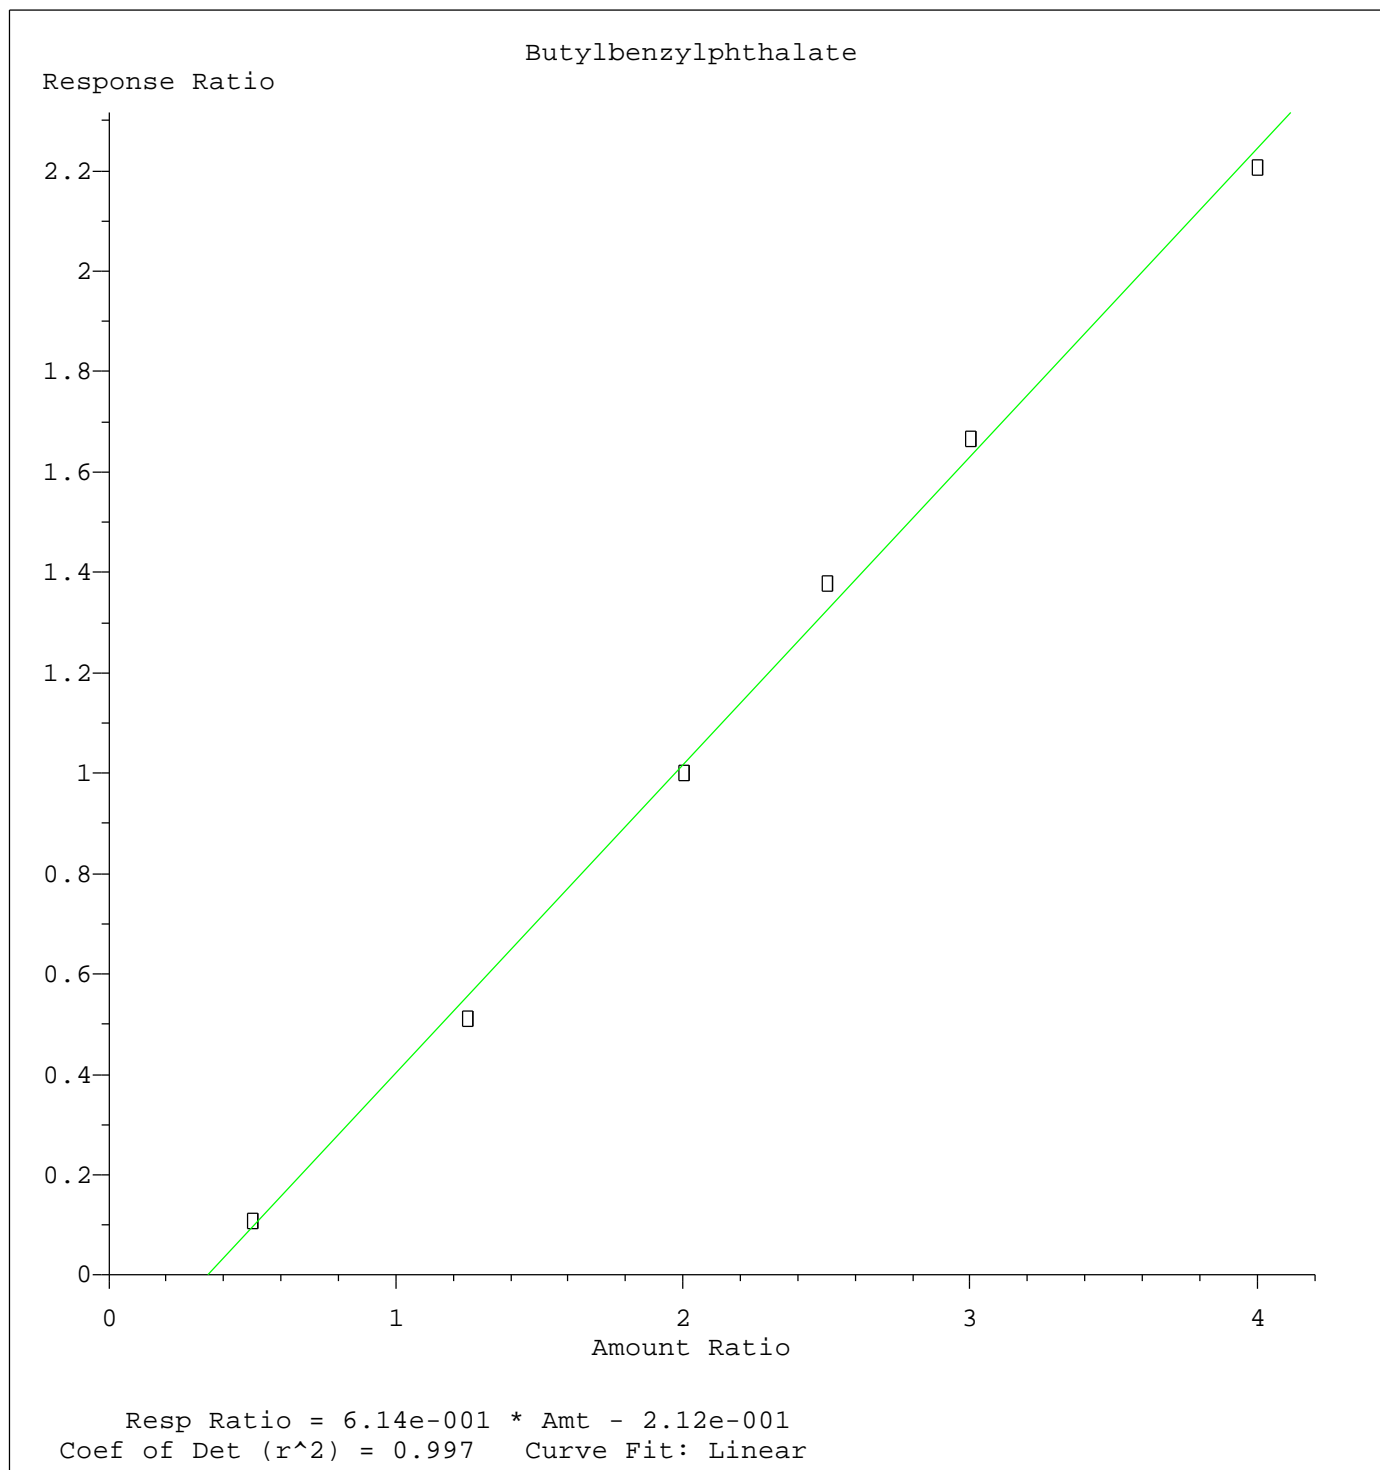

Method Name: Z:\HPCHEM1\BNA\_F\METHODS\8270-BF050818.M  
Calibration Table Last Updated: Wed May 09 12:00:41 2018

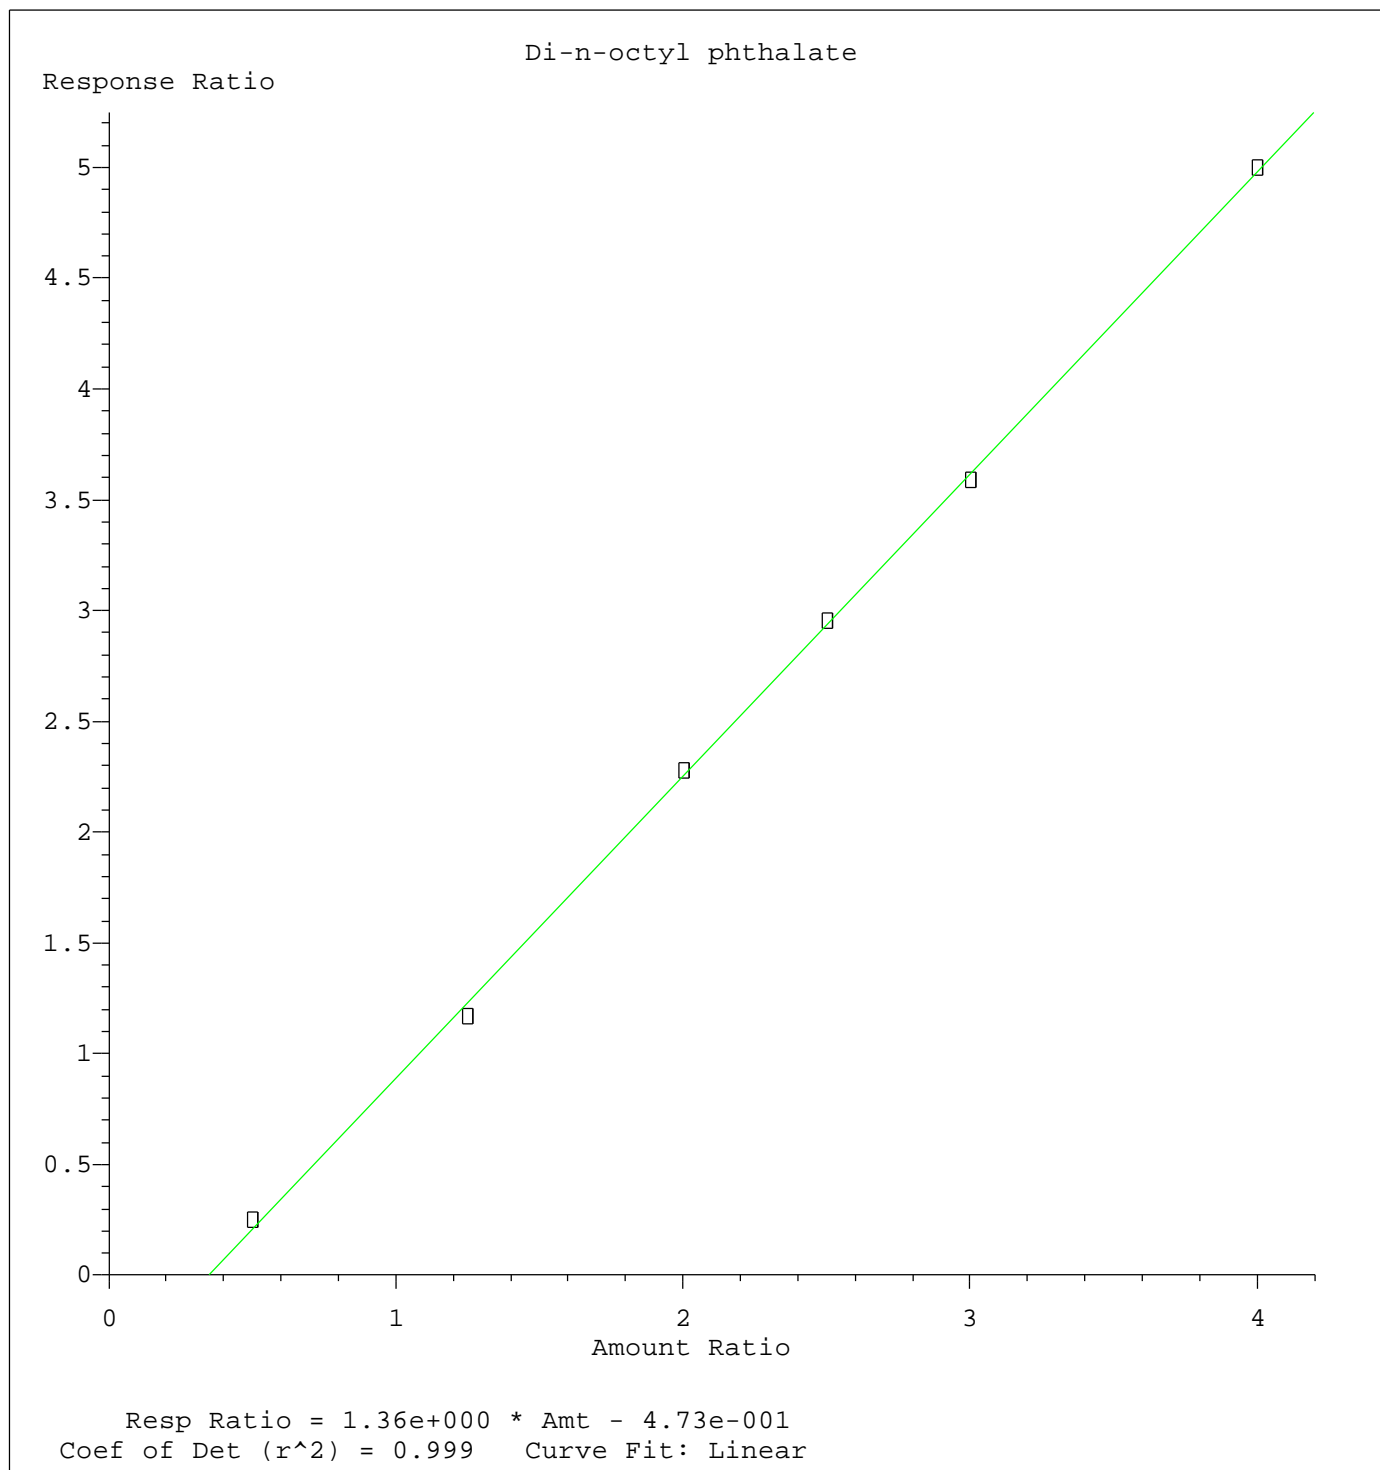

Method Name: Z:\HPCHEM1\BNA\_F\METHODS\8270-BF050818.M  
Calibration Table Last Updated: Wed May 09 12:00:41 2018