
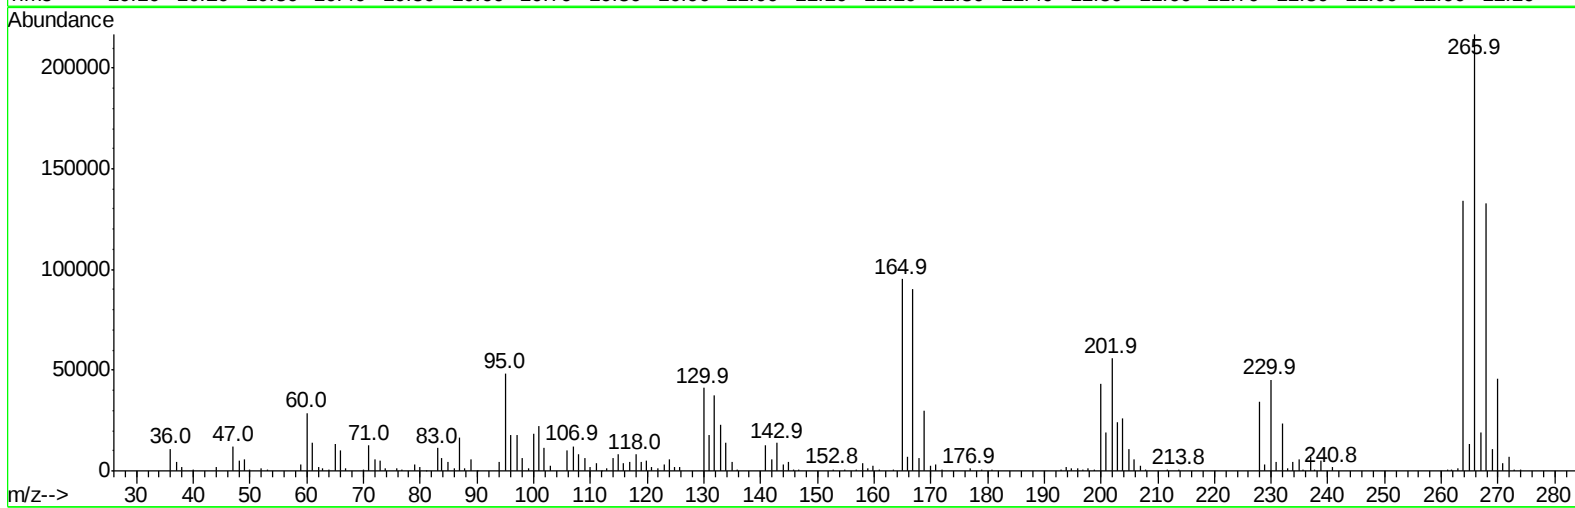


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA F\Data\BF050818\
Data File : BF105146.D
Acq On : 8 May 2018 16:22
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 25 09:14:18 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 09 17:52:28 2018
Response via : Initial Calibration

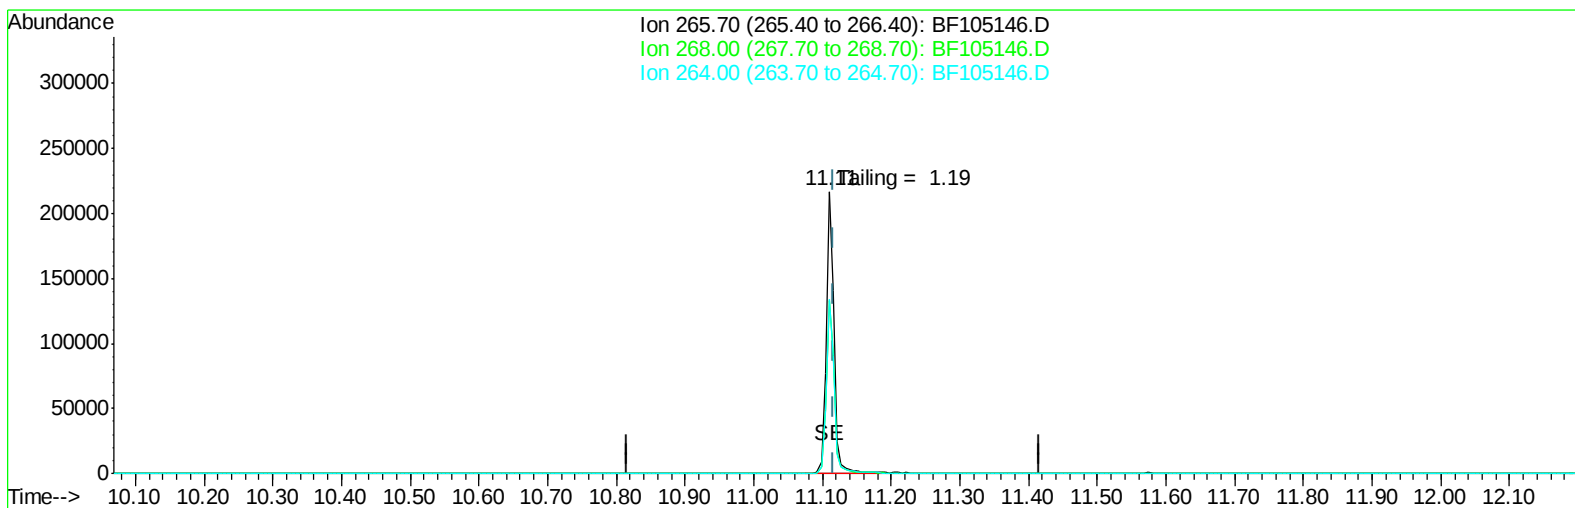

TIC: BF105146.D

(69) Pentachlorophenol (C)



11.110min (-0.006) 28617.48ng

response 174361

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	61.43
264.00	61.90	61.78
0.00	0.00	0.00

Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA F\Data\BF050818\
Data File : BF105146.D
Acq On : 8 May 2018 16:22
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 25 09:14:18 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 09 17:52:28 2018
Response via : Initial Calibration

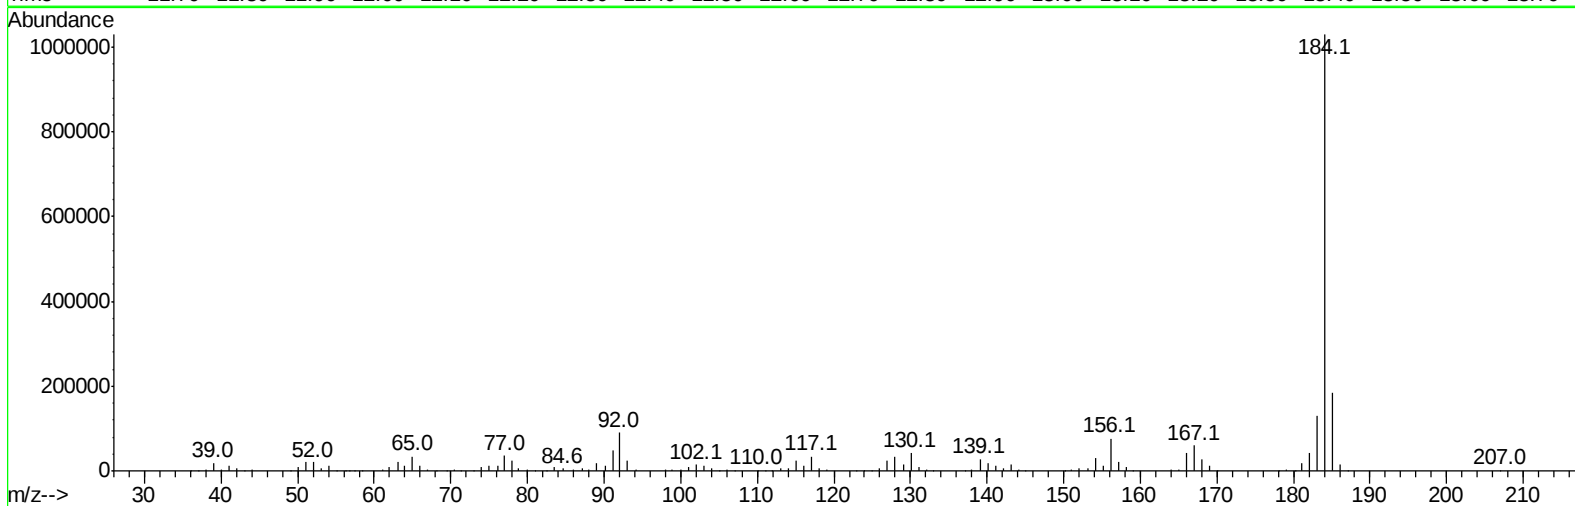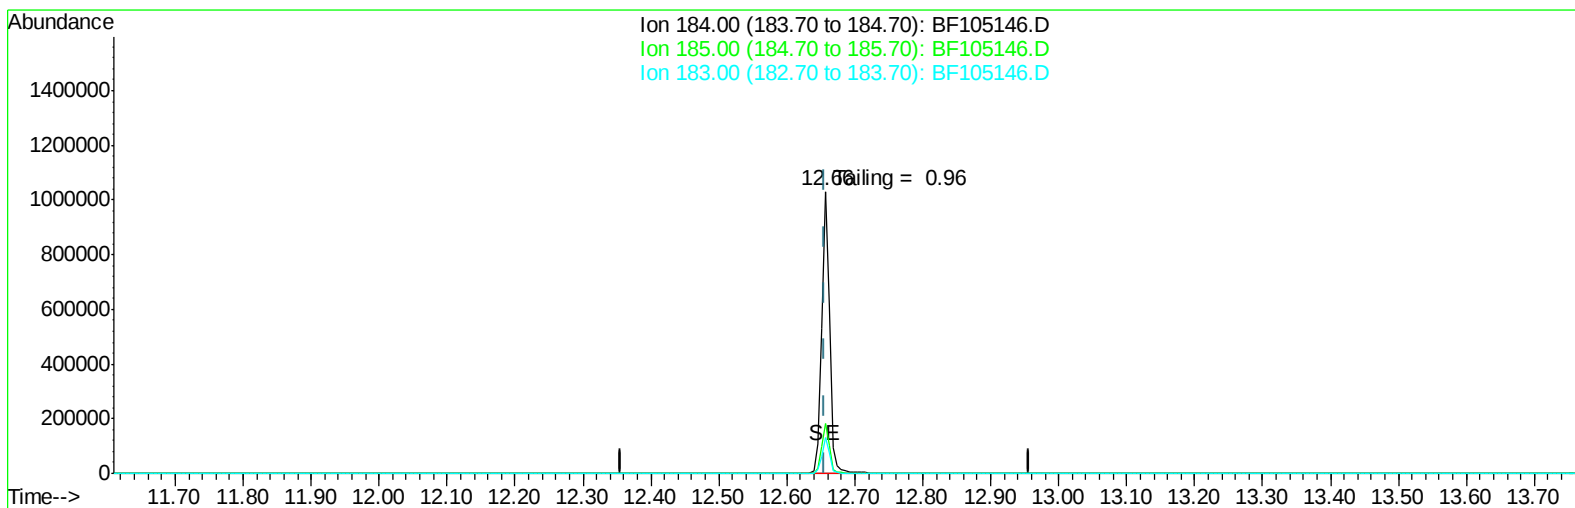

TIC: BF105146.D

(76) Benzidine

12.657min (-0.000) 0.00ng

response 872092

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	17.81
183.00	11.60	12.60
0.00	0.00	0.00