
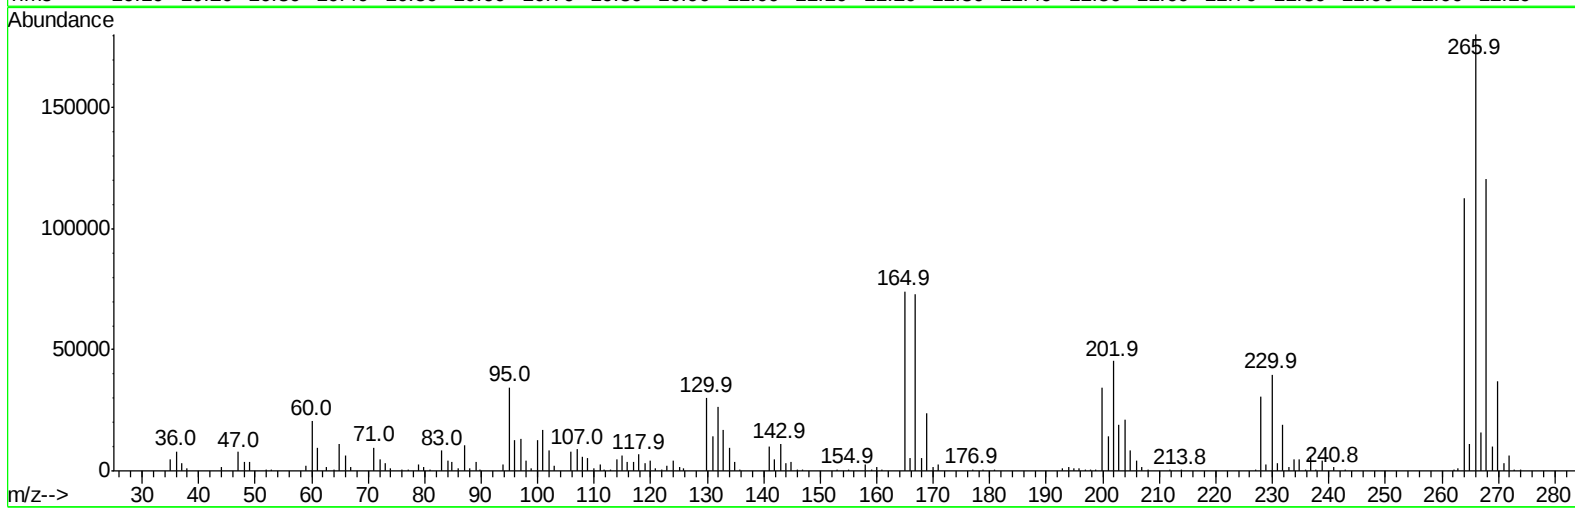


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA F\Data\BF050818\
Data File : BF105171.D
Acq On : 9 May 2018 3:24
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 25 09:15:15 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 09 17:52:28 2018
Response via : Initial Calibration

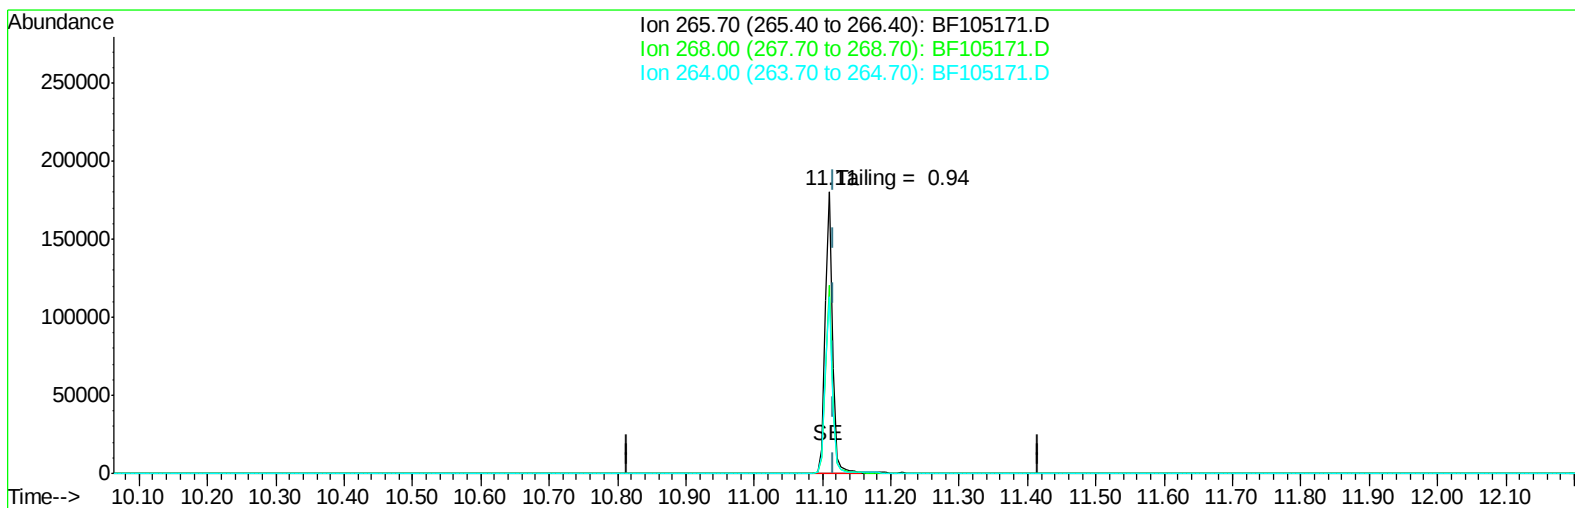

TIC: BF105171.D

(69) Pentachlorophenol (C)



11.110min (-0.006) 153024.66ng

response 141138

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	66.81
264.00	61.90	62.54
0.00	0.00	0.00

Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA F\Data\BF050818\
Data File : BF105171.D
Acq On : 9 May 2018 3:24
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 25 09:15:15 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 09 17:52:28 2018
Response via : Initial Calibration

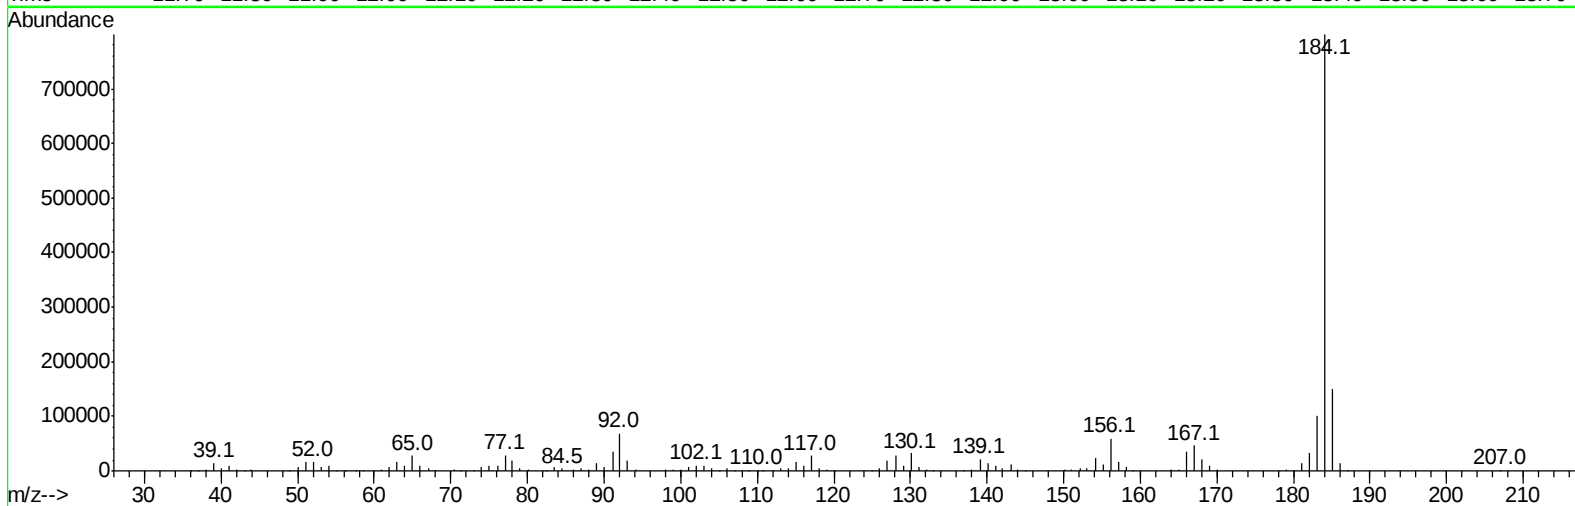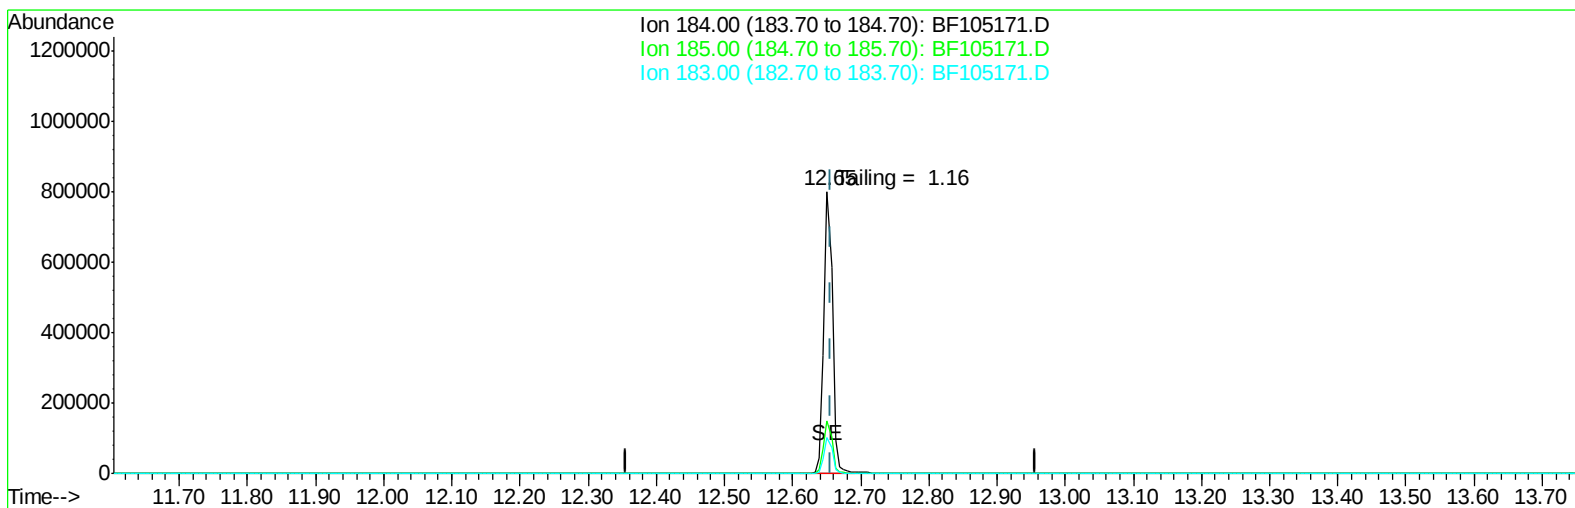

TIC: BF105171.D

(76) Benzidine

12.651min (-0.006) 0.00ng

response 679279

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	18.81
183.00	11.60	12.59
0.00	0.00	0.00