


Data Path : Z:\HPCHEM1\BNA F\Data\BF050818\
 Data File : BF105137.D
 Acq On : 8 May 2018 10:47
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 09 12:00:41 2018

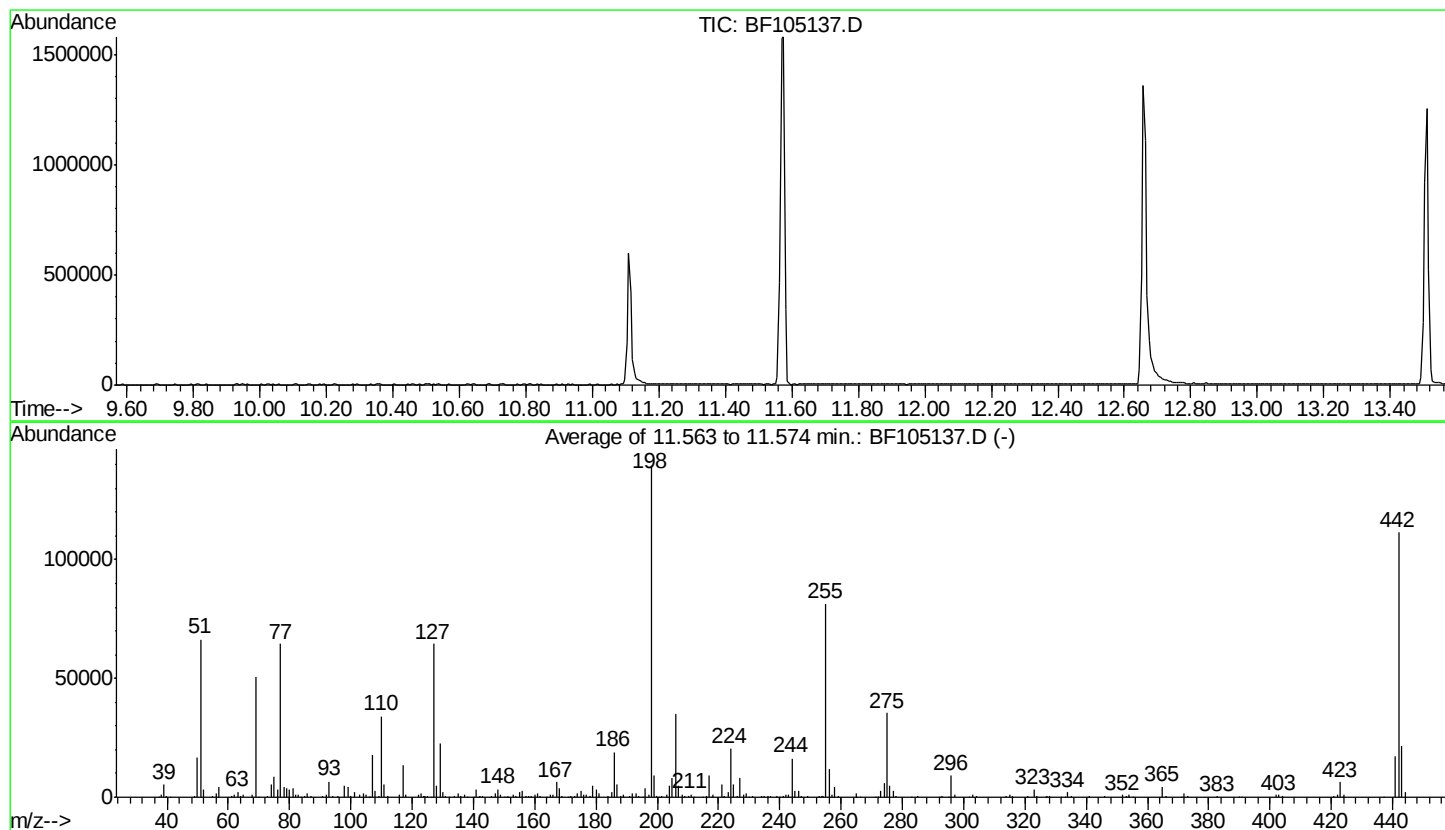

AutoFind: Scans 1611, 1612, 1613; Background Corrected with Scan 1607

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.5	66312	PASS
68	69	0.00	2	1.8	895	PASS
69	198	0.00	100	36.3	50682	PASS
70	69	0.00	2	0.5	231	PASS
127	198	10	80	46.2	64538	PASS
197	198	0.00	2	1.0	1339	PASS
198	198	100	100	100.0	139624	PASS
199	198	5	9	6.6	9176	PASS
275	198	10	60	25.4	35395	PASS
365	198	1	100	3.2	4526	PASS
441	443	0.01	100	80.7	17208	PASS
442	198	50	100	79.8	111359	PASS
443	442	15	24	19.1	21312	PASS