


Data Path : Z:\HPCHEM1\BNA F\Data\BF050818\  
 Data File : BF105171.D  
 Acq On : 9 May 2018 3:24  
 Operator : JU/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF050818.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Wed May 09 12:00:41 2018

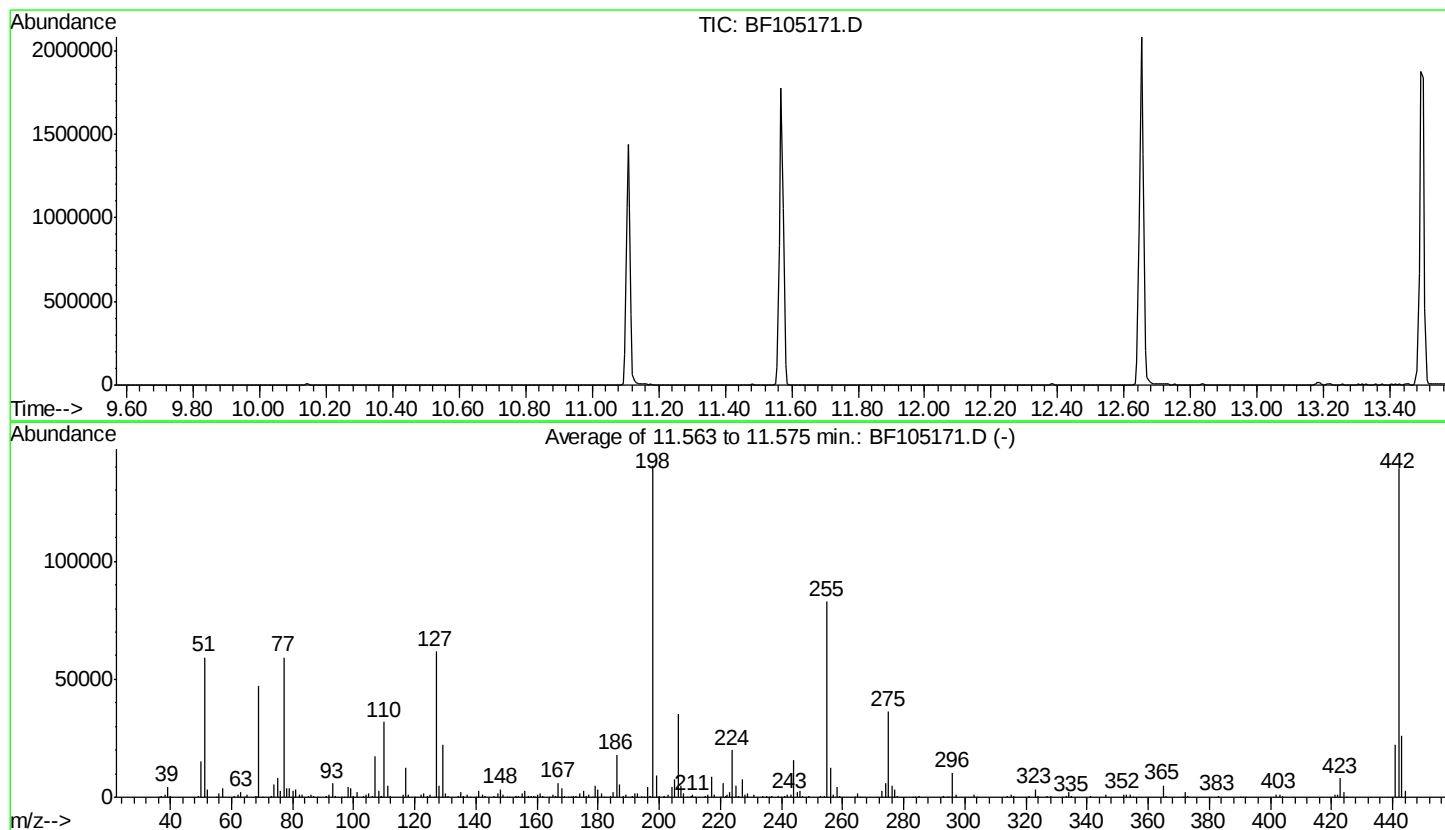

AutoFind: Scans 1611, 1612, 1613; Background Corrected with Scan 1606

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 42.3         | 59373      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.5          | 692        | PASS                |
| 69             | 198             | 0.00            | 100             | 33.5         | 47032      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.4          | 184        | PASS                |
| 127            | 198             | 10              | 80              | 43.9         | 61653      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.5          | 689        | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 140496     | PASS                |
| 199            | 198             | 5               | 9               | 6.5          | 9179       | PASS                |
| 275            | 198             | 10              | 60              | 25.7         | 36157      | PASS                |
| 365            | 198             | 1               | 100             | 3.6          | 5052       | PASS                |
| 441            | 443             | 0.01            | 100             | 84.9         | 22332      | PASS                |
| 442            | 198             | 50              | 100             | 99.1         | 139165     | PASS                |
| 443            | 442             | 15              | 24              | 18.9         | 26293      | PASS                |