
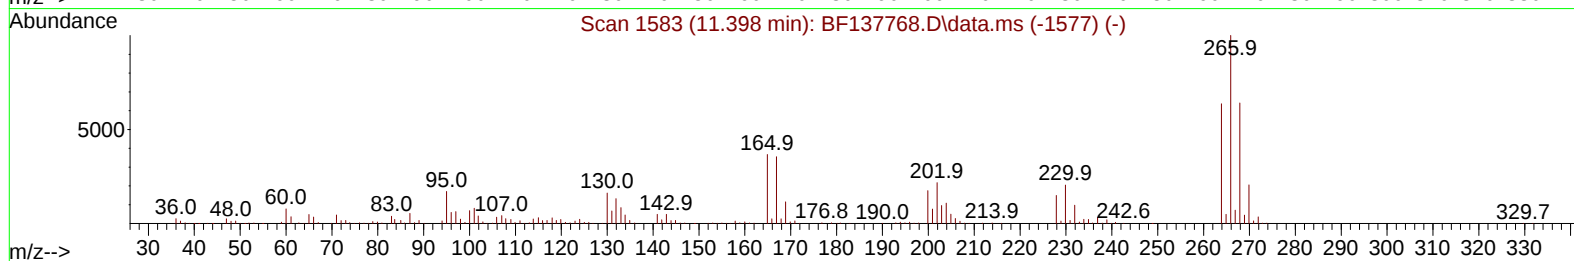
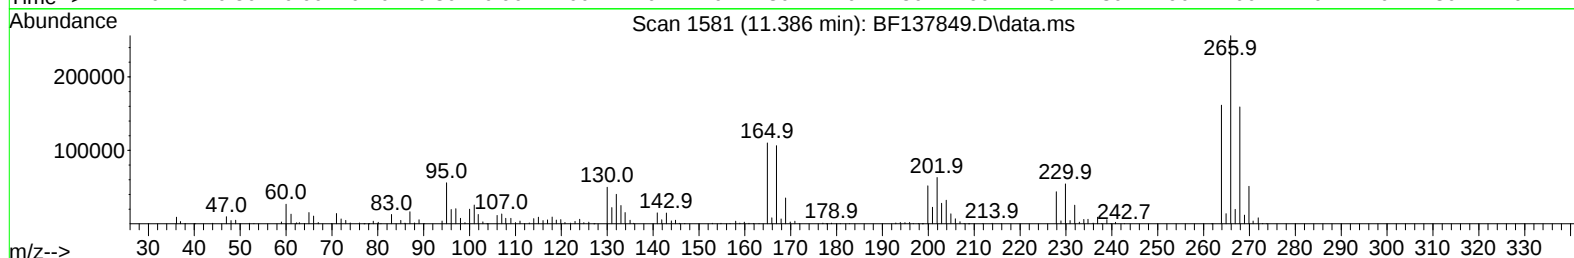


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF050824\  
Data File : BF137849.D  
Acq On : 08 May 2024 11:29  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 08 12:08:27 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF043024.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed May 01 03:25:08 2024  
Response via : Initial Calibration

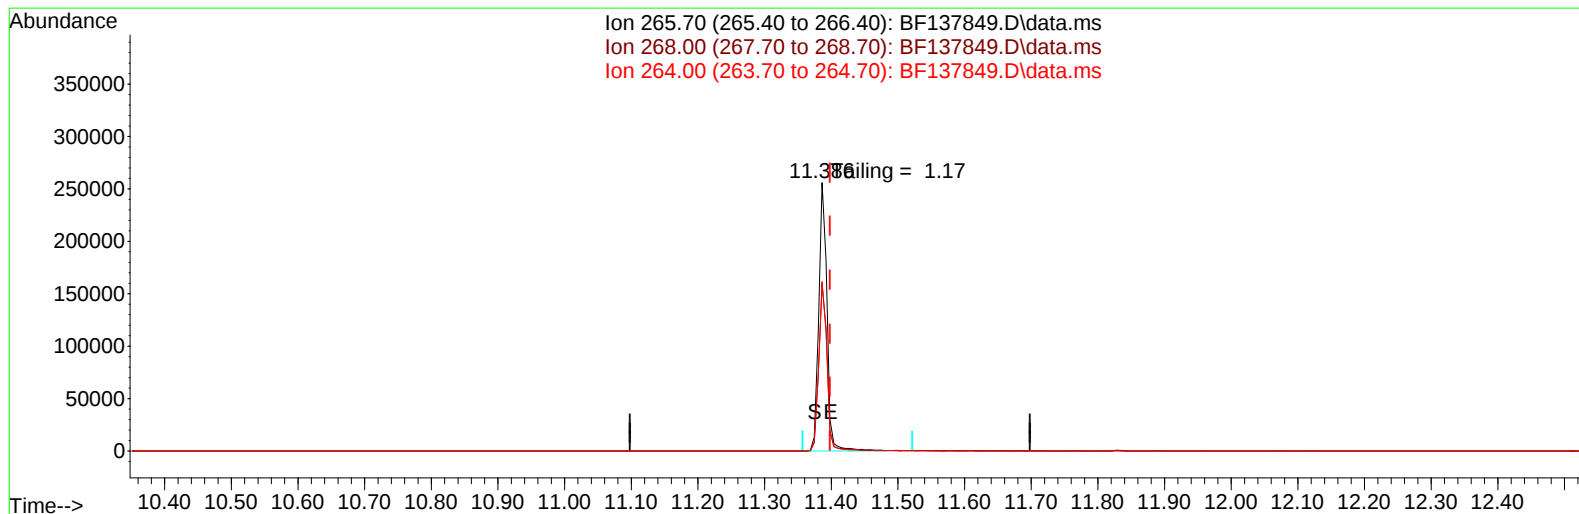

TIC: BF137849.D\data.ms

**(70) Pentachlorophenol (C)**




**11.386min (-0.012) 23549.73 ng**

**response 221236**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 64.10  | 62.15  |
| 264.00 | 63.70  | 63.10  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF050824\  
Data File : BF137849.D  
Acq On : 08 May 2024 11:29  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 08 12:08:27 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF043024.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed May 01 03:25:08 2024  
Response via : Initial Calibration

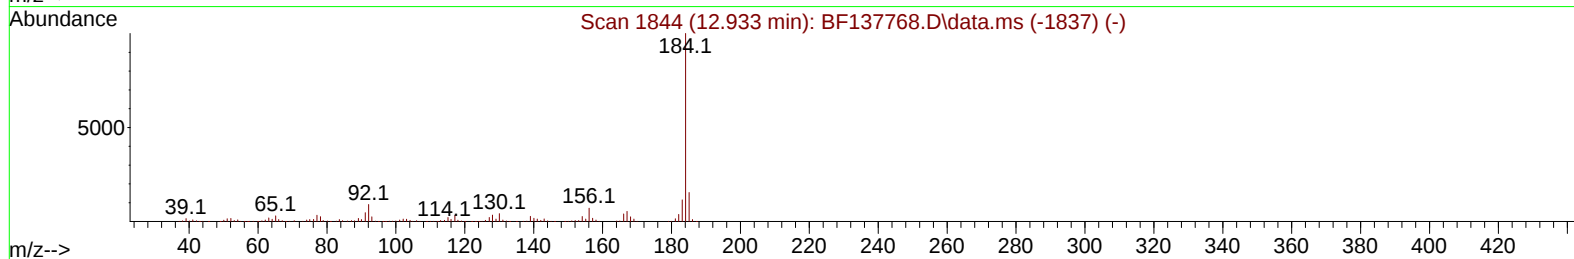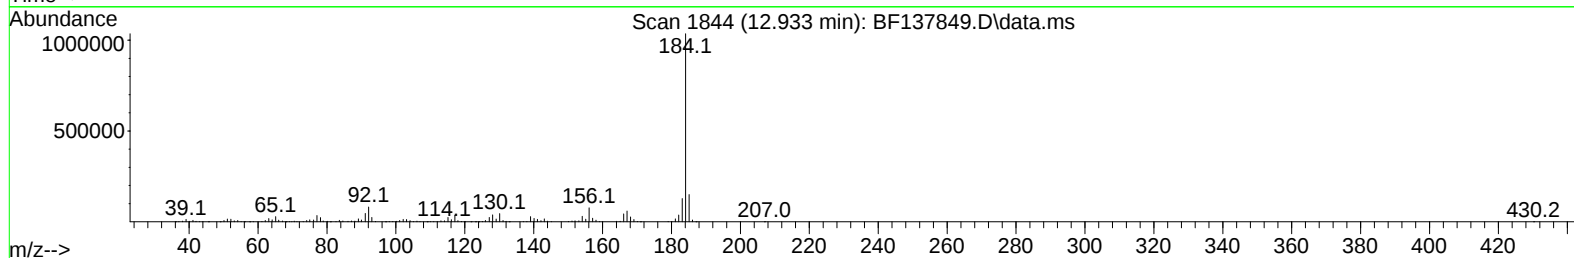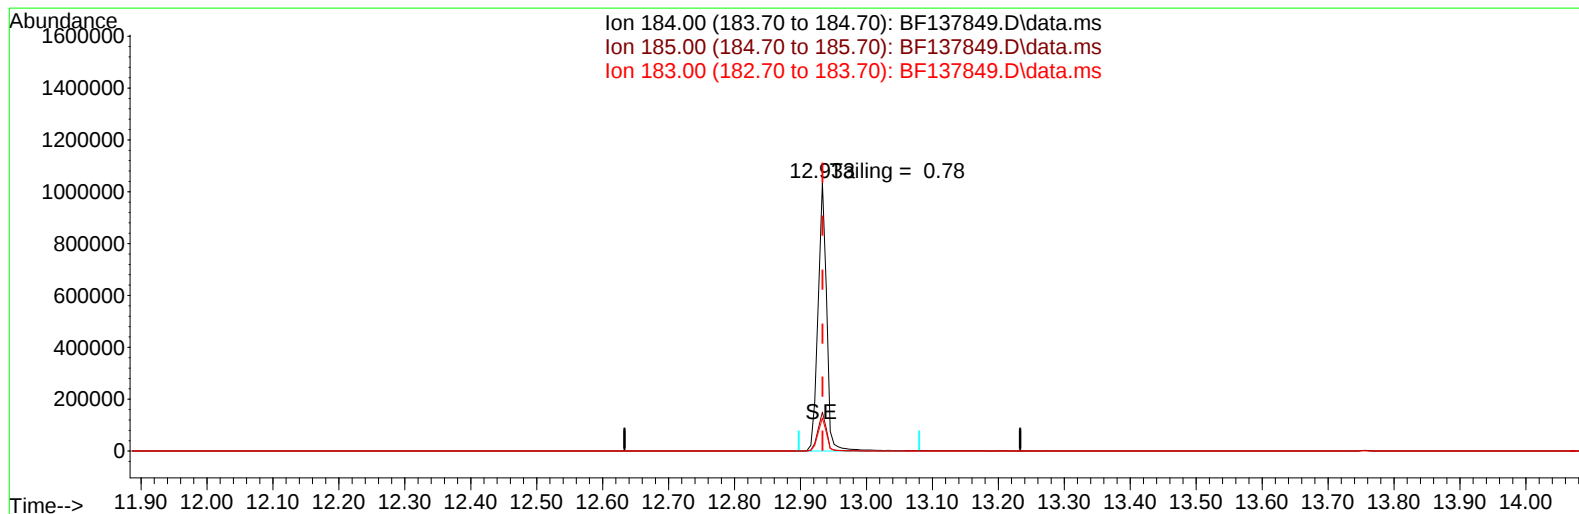

TIC: BF137849.D\data.ms

**(77) Benzidine**

12.933min (-0.000) 0.00 ng

response 947095

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.40  | 14.49  |
| 183.00 | 11.50  | 12.34  |
| 0.00   | 0.00   | 0.00   |