


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050824\
Data File : BF137849.D
Acq On : 08 May 2024 11:29
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed May 01 03:25:08 2024

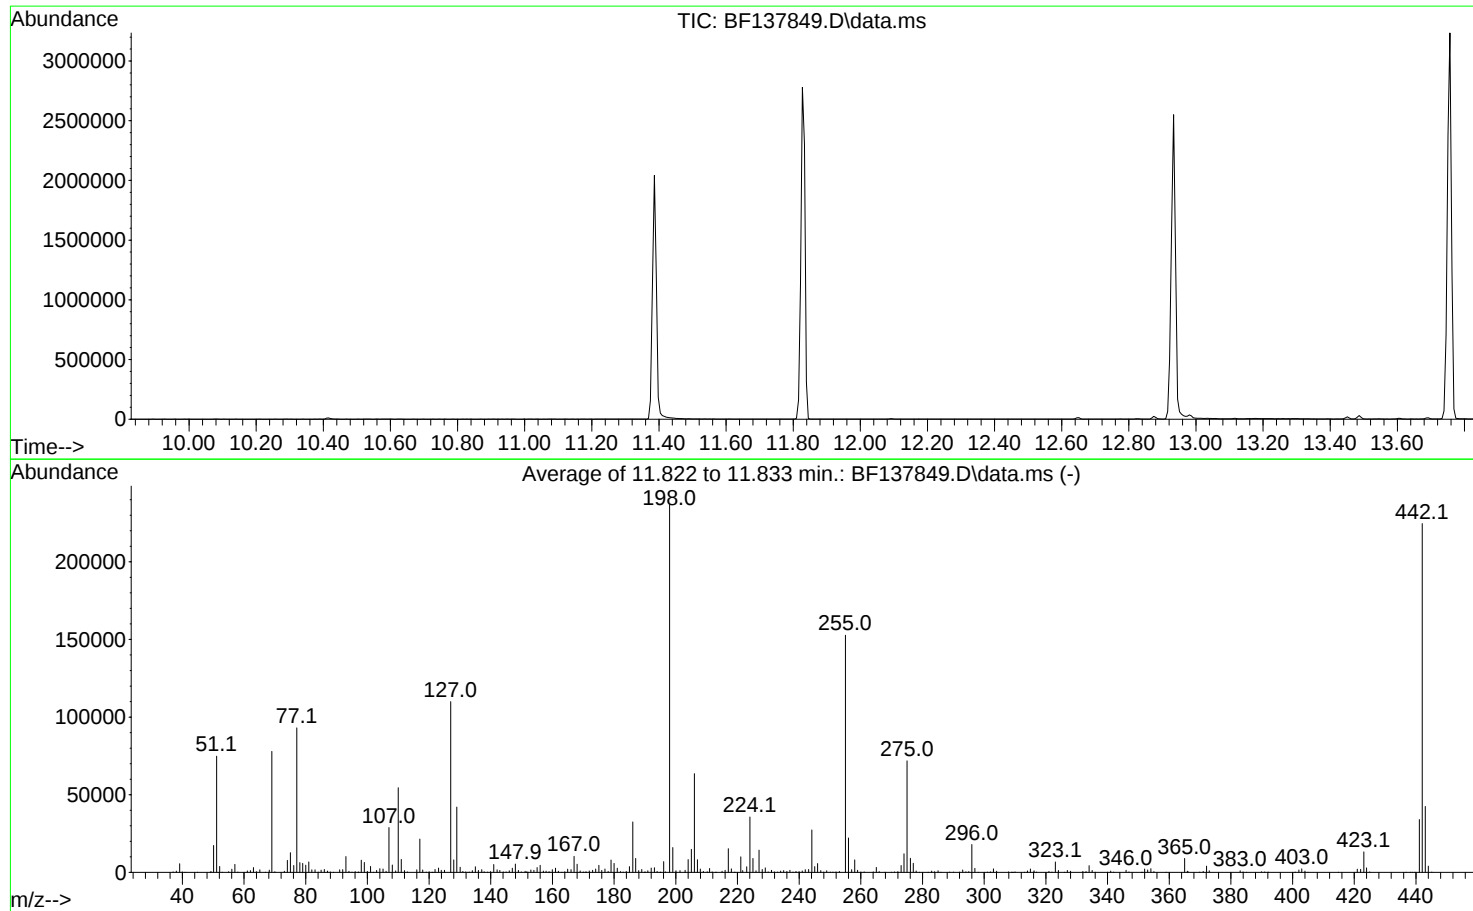

AutoFind: Scans 1655, 1656, 1657; Background Corrected with Scan 1650

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.6	74869	PASS
68	69	0.00	2	1.8	1425	PASS
69	198	0.00	100	32.9	77880	PASS
70	69	0.00	2	0.6	464	PASS
127	198	10	80	46.4	109923	PASS
197	198	0.00	2	0.1	302	PASS
198	198	100	100	100.0	236928	PASS
199	198	5	9	6.7	15944	PASS
275	198	10	60	30.3	71859	PASS
365	198	1	100	3.8	8964	PASS
441	198	0.01	100	14.3	33986	PASS
442	442	50	100	100.0	224680	PASS
443	442	15	24	18.9	42490	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/8/2024	BNA_F	<u>BF137849.D</u>
Compound Name	Response	Retention Time
DDT	560289	13.757
DDD	8074	13.486
DDE	850	13.116
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8924	569213	1.57

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050824\
Data File : BF137849.D
Acq On : 08 May 2024 11:29
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 08 12:08:27 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 03:25:08 2024
Response via : Initial Calibration

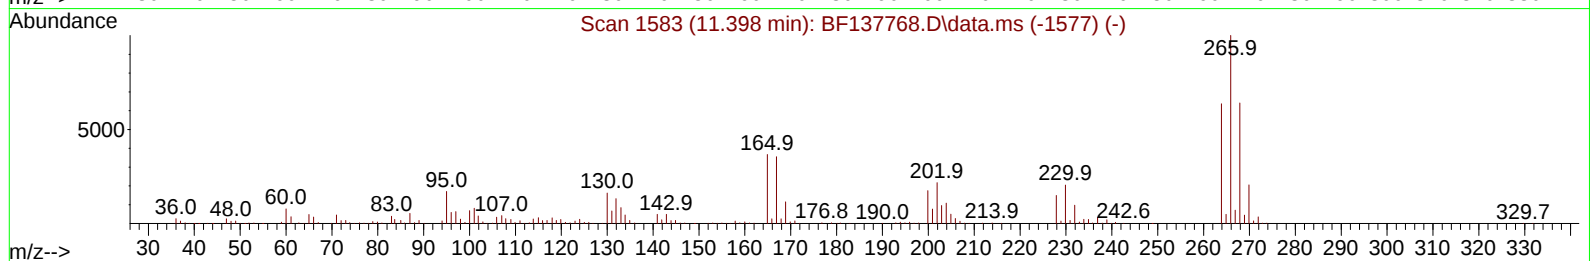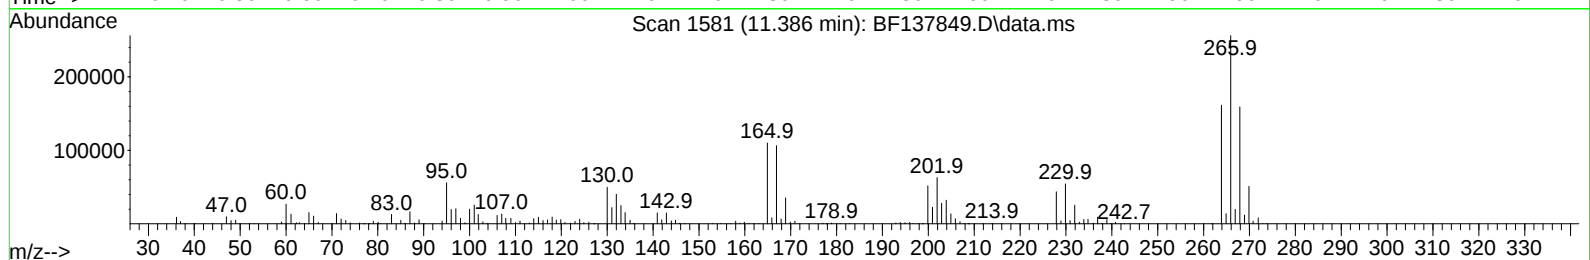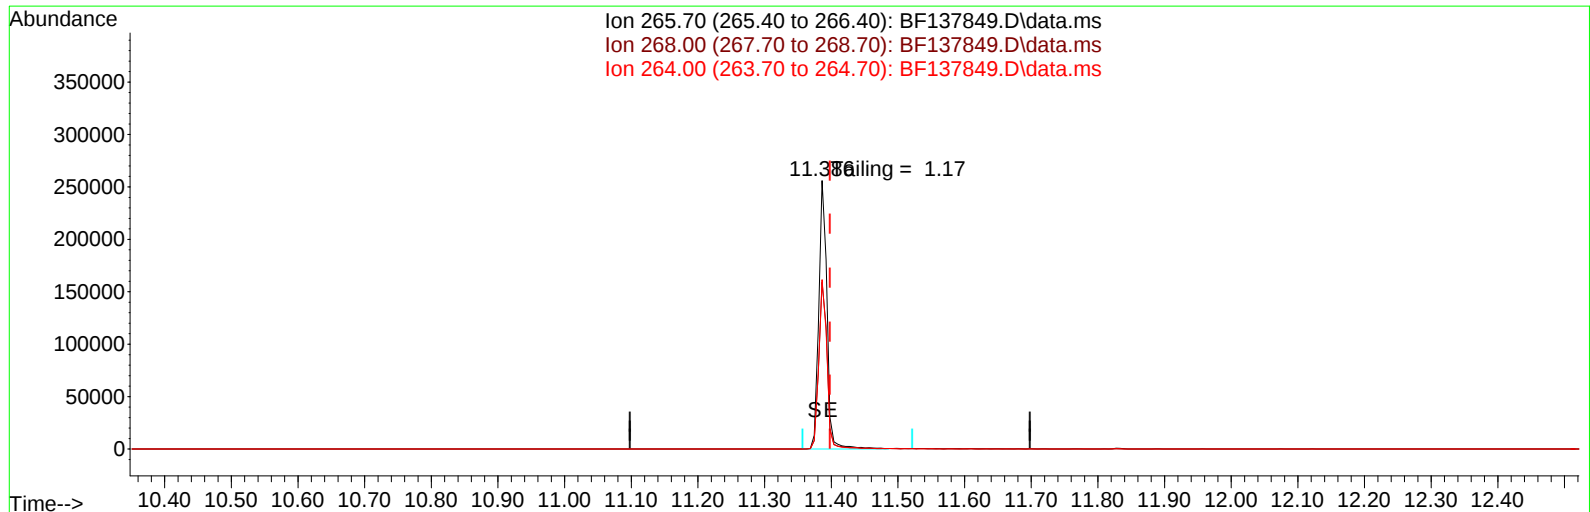

TIC: BF137849.D\data.ms

(70) Pentachlorophenol (C)

11.386min (-0.012) 23549.73 ng




response 221236

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.10	62.15
264.00	63.70	63.10
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050824\
Data File : BF137849.D
Acq On : 08 May 2024 11:29
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 08 12:08:27 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 03:25:08 2024
Response via : Initial Calibration

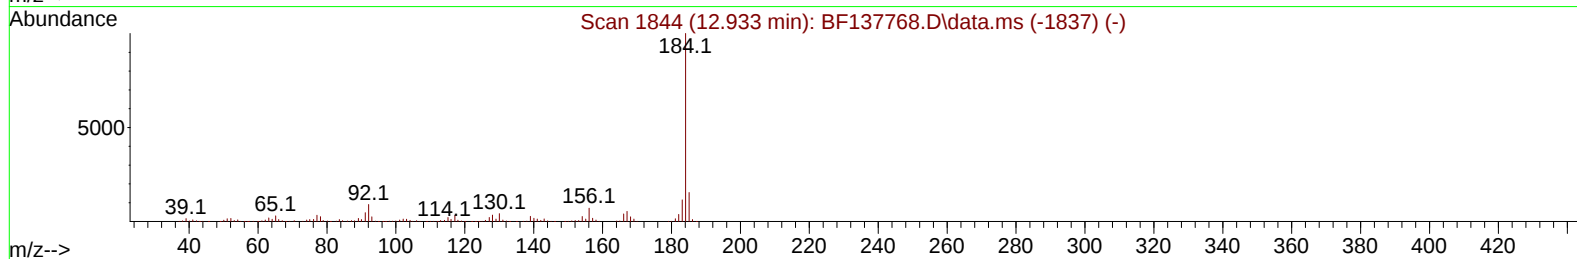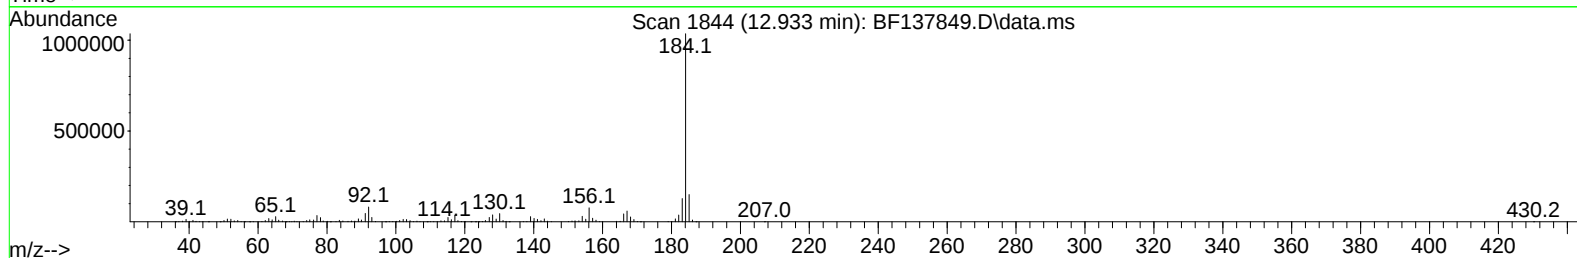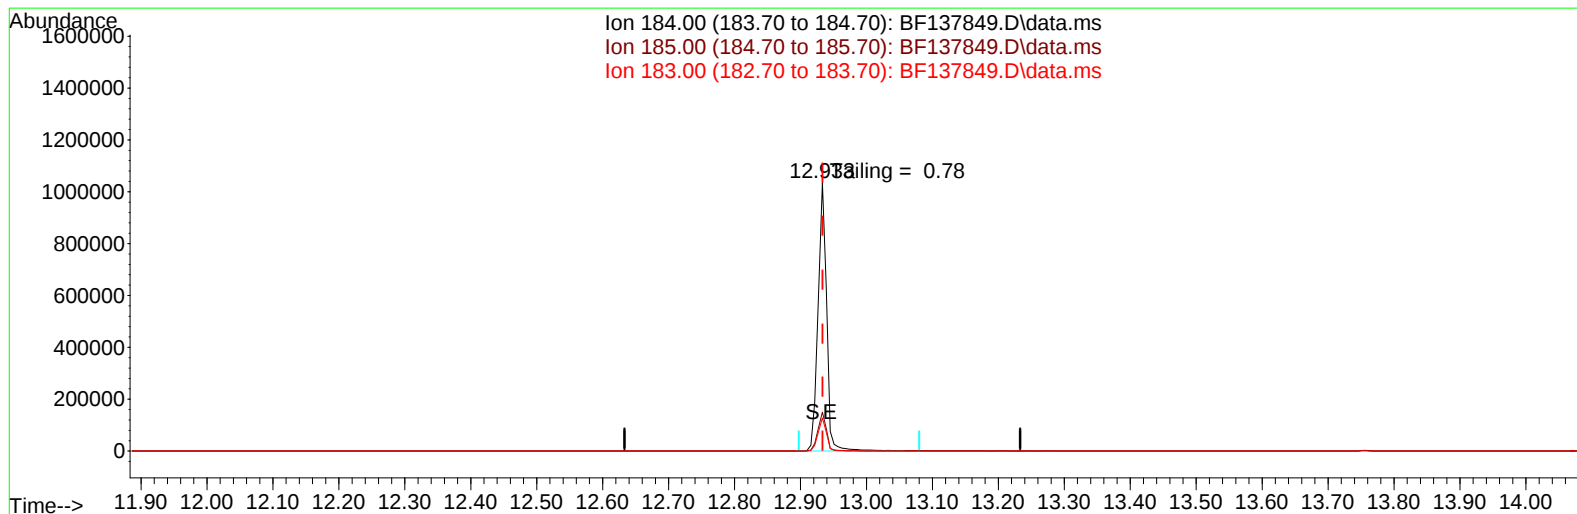

TIC: BF137849.D\data.ms

(77) Benzidine

12.933min (-0.000) 0.00 ng

response 947095

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.40	14.49
183.00	11.50	12.34
0.00	0.00	0.00