
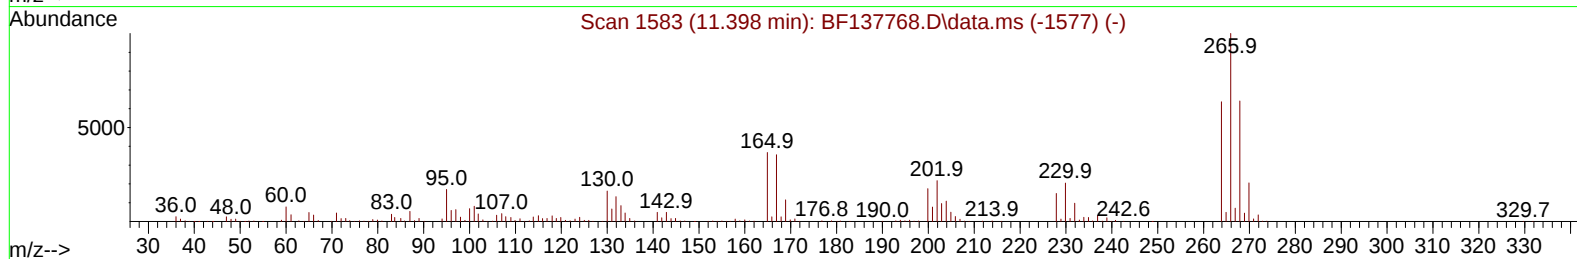
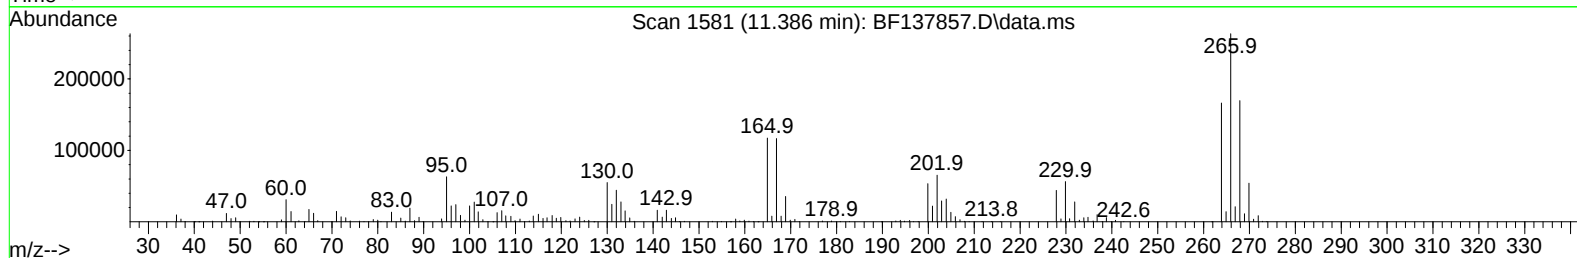


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050924\
Data File : BF137857.D
Acq On : 09 May 2024 10:51
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 09 11:28:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 03:25:08 2024
Response via : Initial Calibration

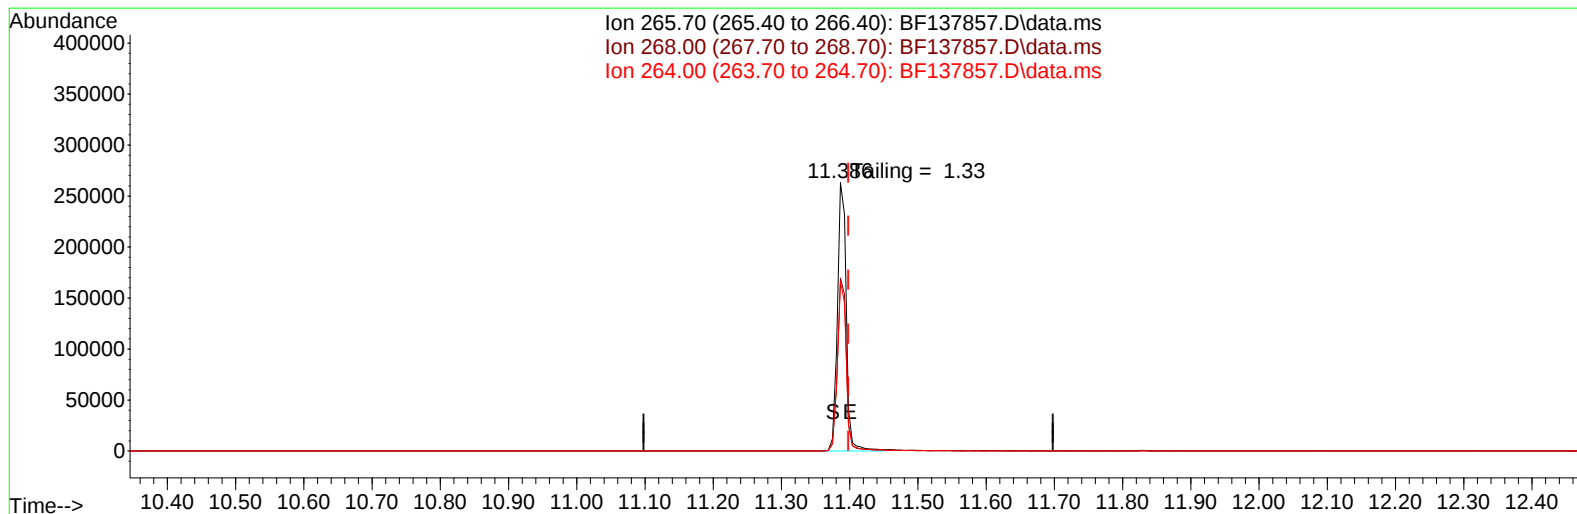

TIC: BF137857.D\data.ms

(70) Pentachlorophenol (C)




11.386min (-0.012) 551352.21 ng

response 239060

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.10	64.45
264.00	63.70	63.21
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050924\
Data File : BF137857.D
Acq On : 09 May 2024 10:51
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 09 11:28:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 03:25:08 2024
Response via : Initial Calibration

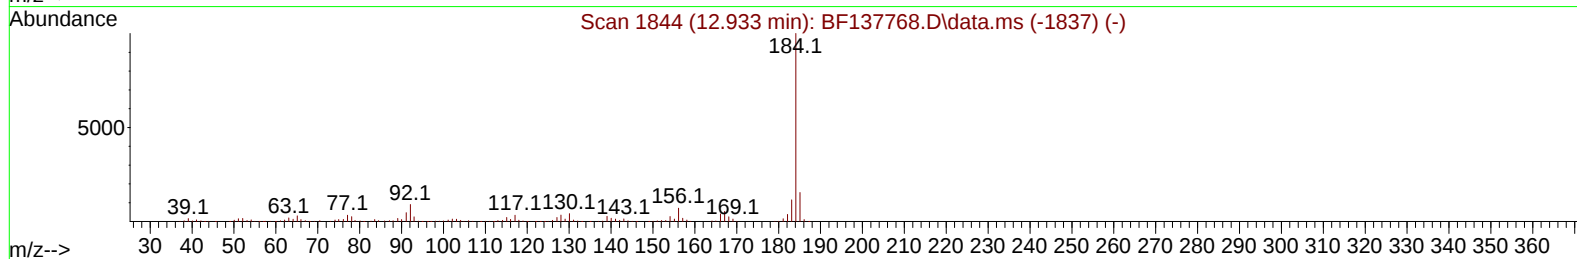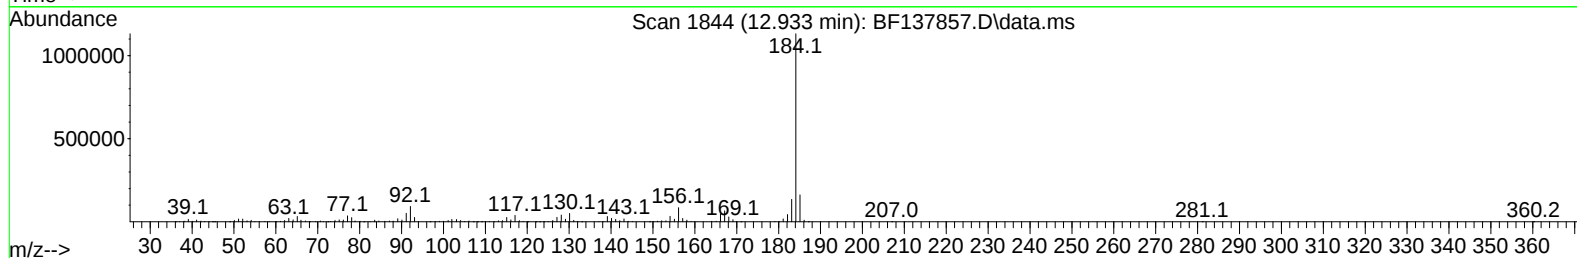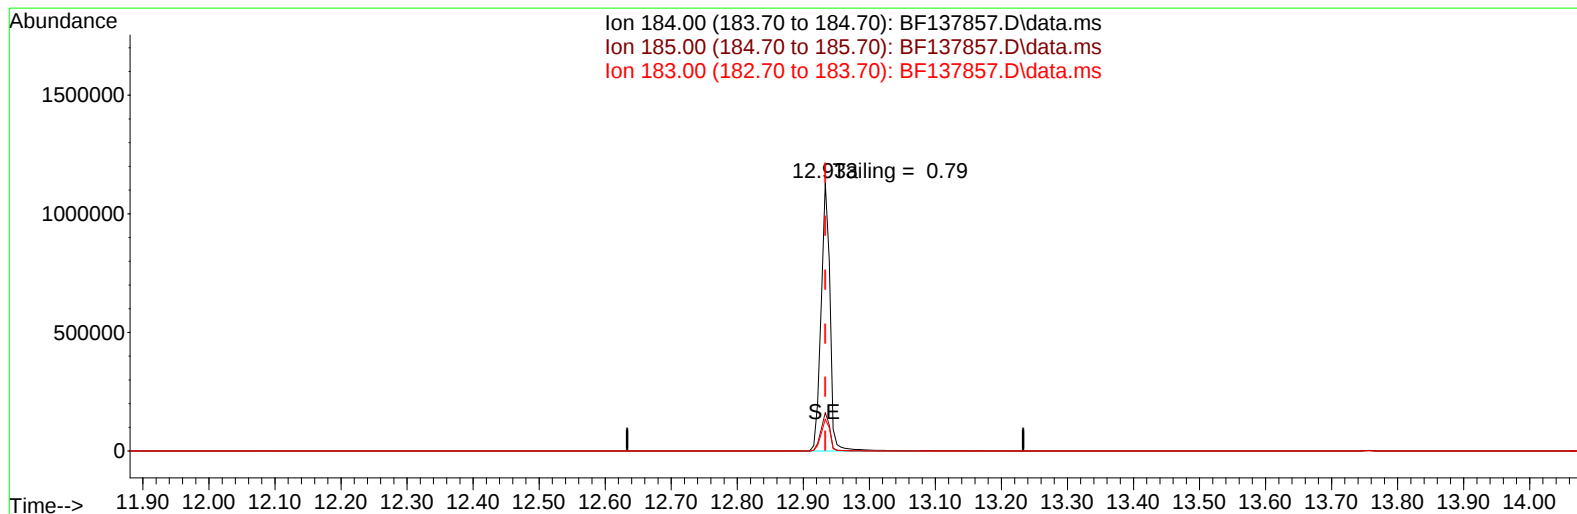

TIC: BF137857.D\data.ms

(77) Benzidine

12.933min (+ 0.000) 5468.36 ng m

response 1062226

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.40	14.32
183.00	11.50	11.91
0.00	0.00	0.00