


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050924\
Data File : BF137857.D
Acq On : 09 May 2024 10:51
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed May 01 03:25:08 2024

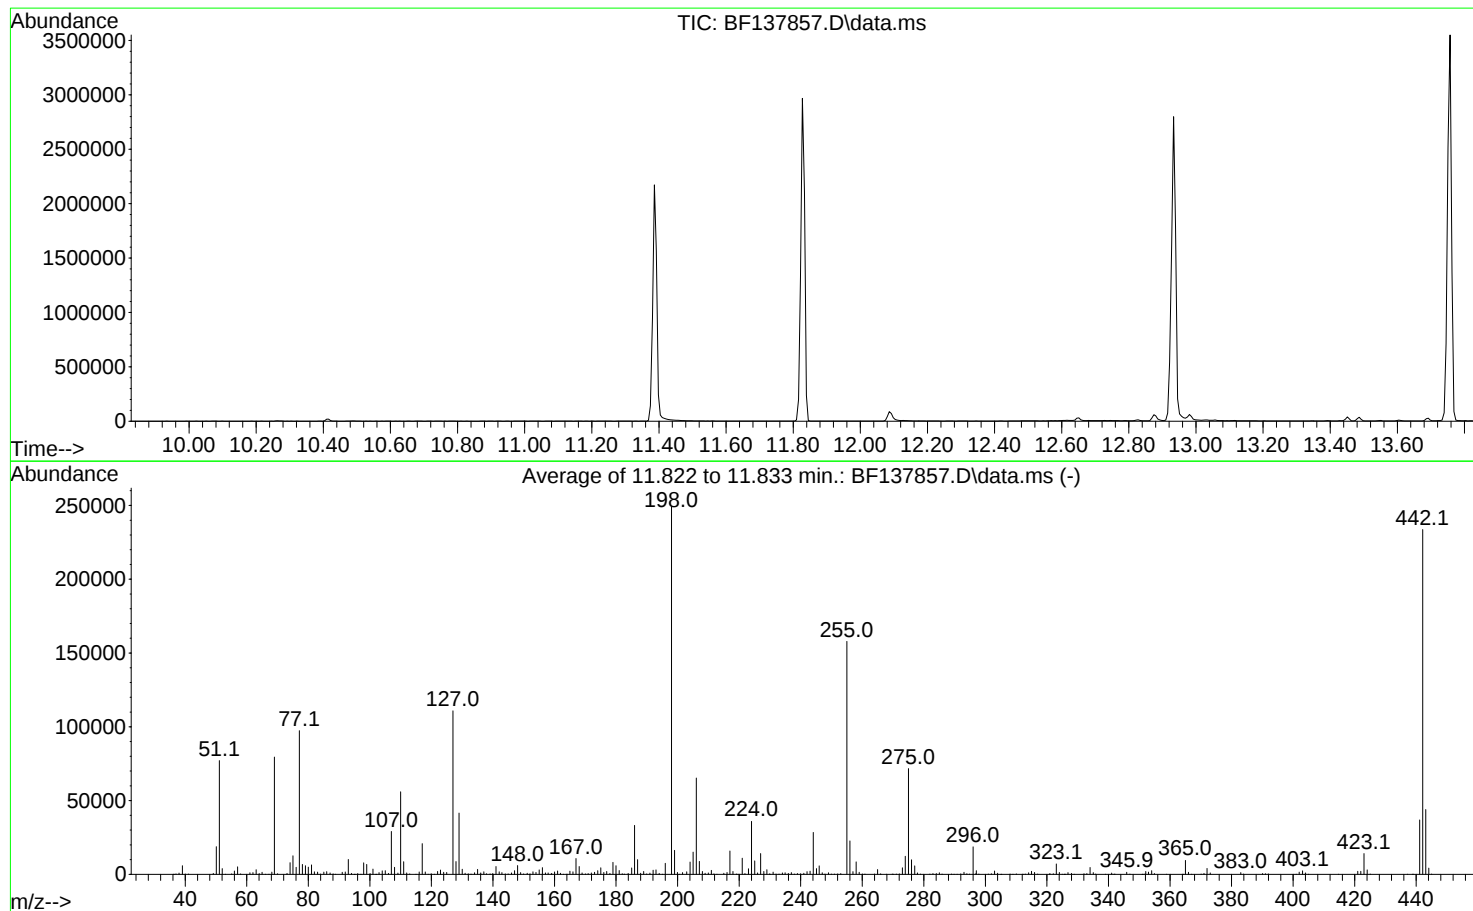

AutoFind: Scans 1655, 1656, 1657; Background Corrected with Scan 1650

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	30.9	77072	PASS
68	69	0.00	2	1.9	1530	PASS
69	198	0.00	100	31.9	79520	PASS
70	69	0.00	2	0.6	489	PASS
127	198	10	80	44.4	110781	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	249280	PASS
199	198	5	9	6.5	16323	PASS
275	198	10	60	28.8	71712	PASS
365	198	1	100	3.8	9492	PASS
441	198	0.01	100	14.8	36900	PASS
442	442	50	100	100.0	233693	PASS
443	442	15	24	18.8	43912	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/9/2024	BNA_F	<u>BF137857.D</u>
Compound Name	Response	Retention Time
DDT	611325	13.757
DDD	11725	13.451
DDE	694	13.116
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12419	623744	1.99

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050924\
Data File : BF137857.D
Acq On : 09 May 2024 10:51
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 09 11:28:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 03:25:08 2024
Response via : Initial Calibration

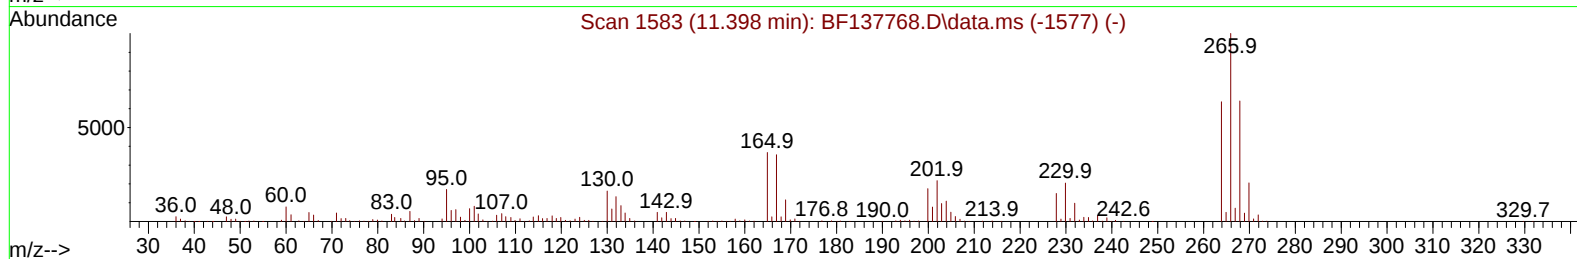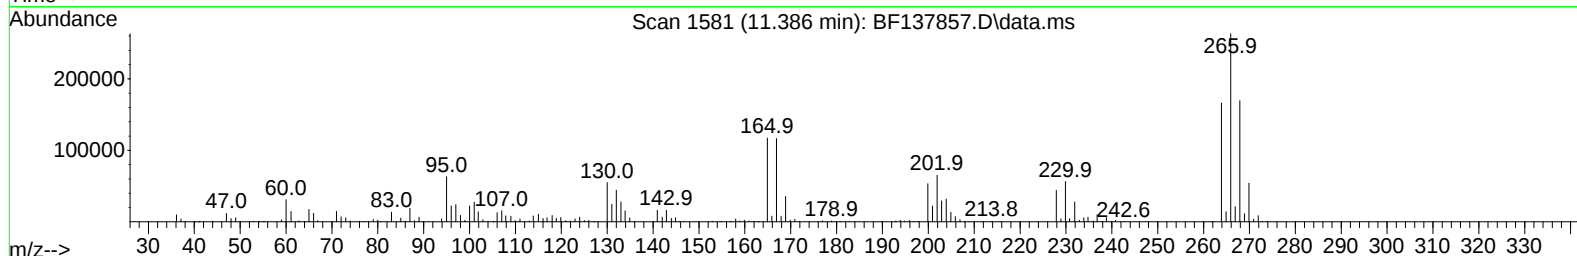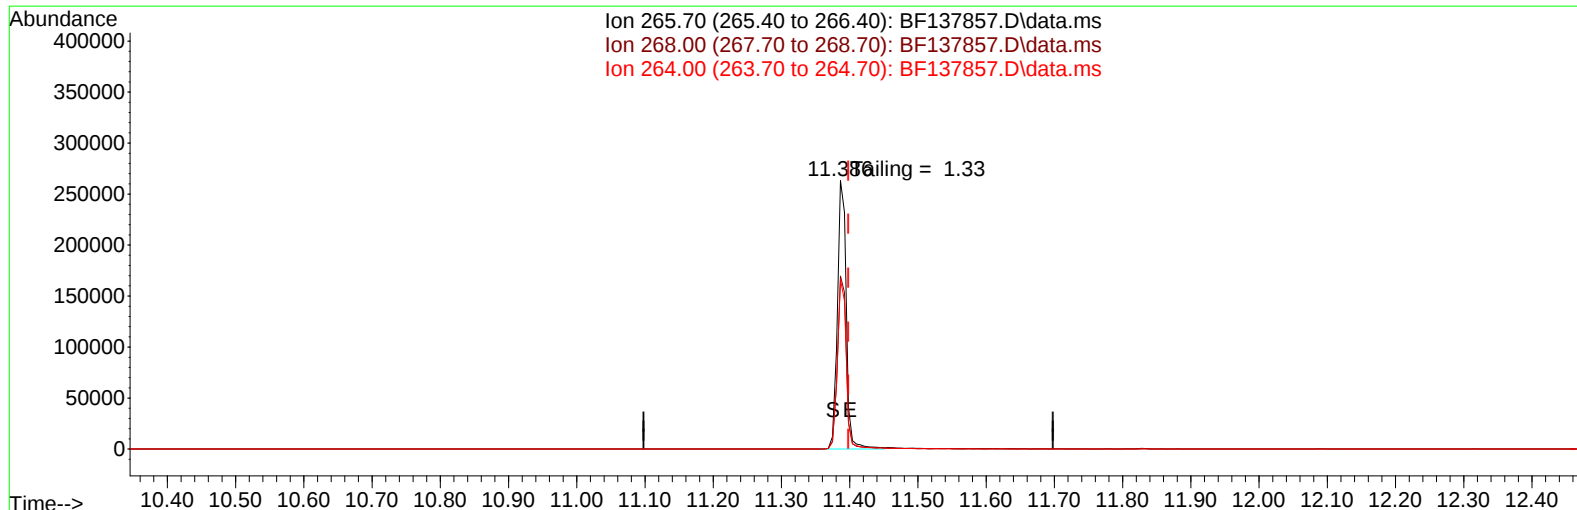

TIC: BF137857.D\data.ms

(70) Pentachlorophenol (C)

11.386min (-0.012) 551352.21 ng




response 239060

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.10	64.45
264.00	63.70	63.21
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050924\
Data File : BF137857.D
Acq On : 09 May 2024 10:51
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 09 11:28:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 03:25:08 2024
Response via : Initial Calibration

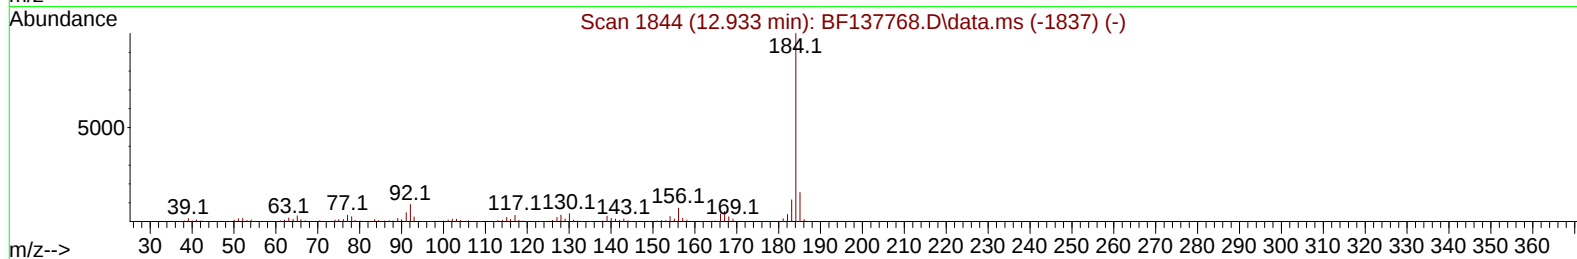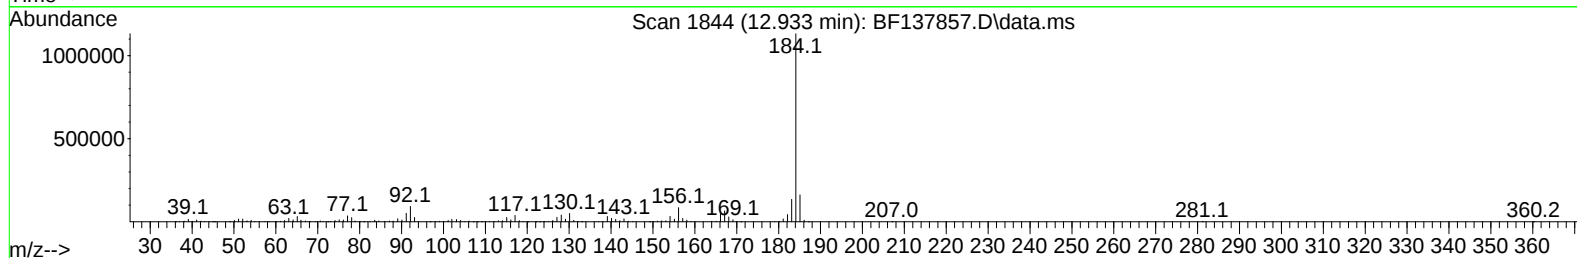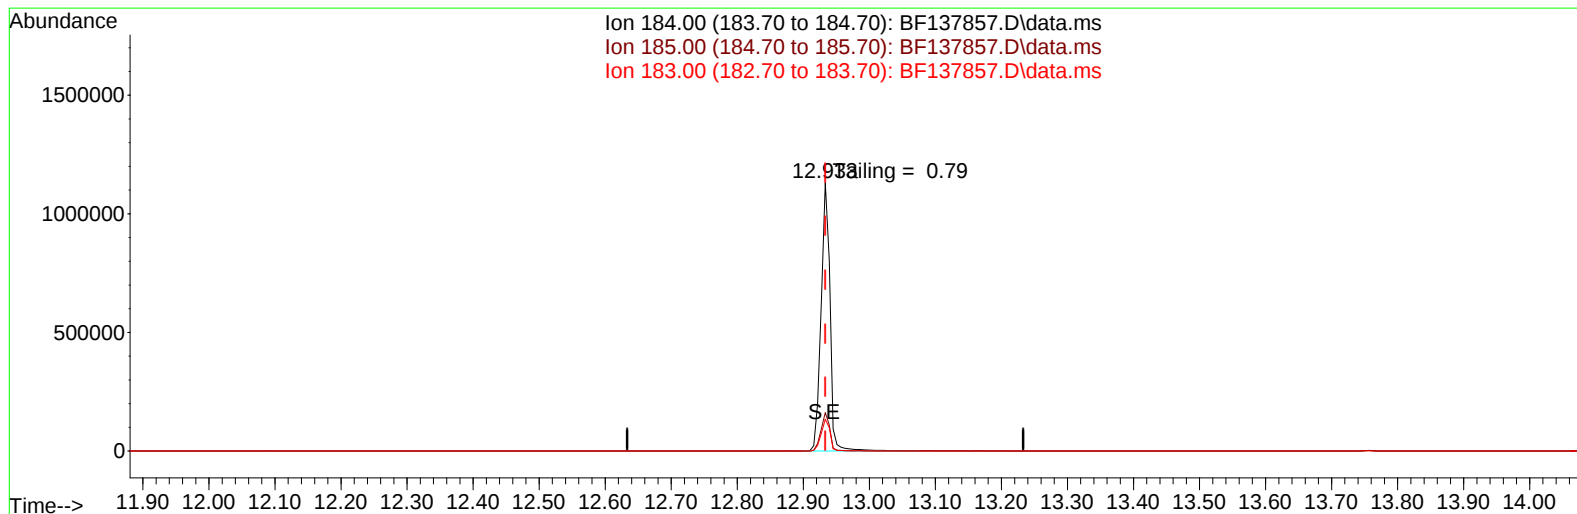

TIC: BF137857.D\data.ms

(77) Benzidine

12.933min (+ 0.000) 5468.36 ng m

response 1062226

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.40	14.32
183.00	11.50	11.91
0.00	0.00	0.00