


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF051019\
 Data File : BF114113.D
 Acq On : 10 May 2019 9:14
 Operator : JU/SJ
 Sample : DFTPP
 Misc : 8
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 10 15:56:46 2019

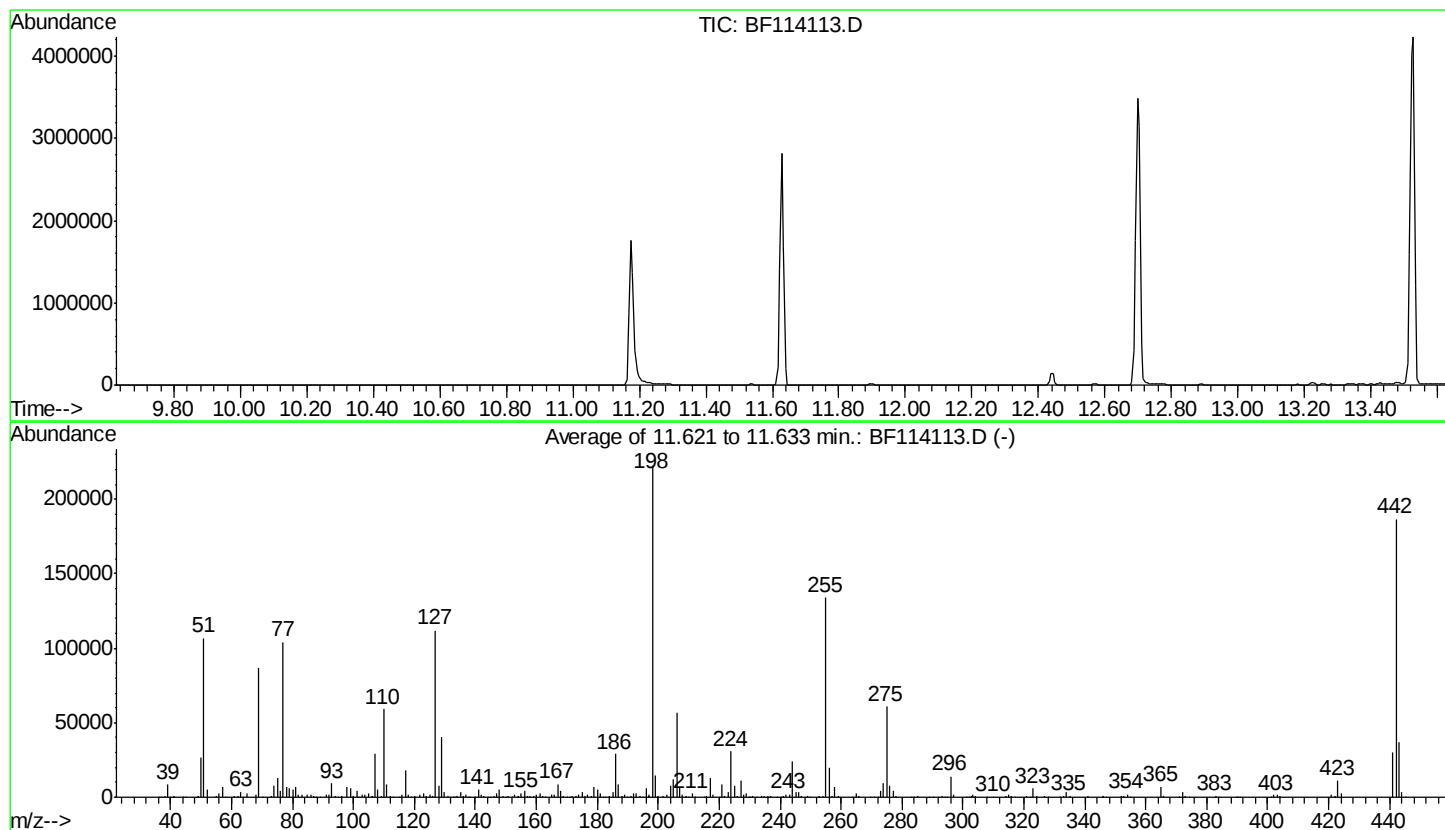

AutoFind: Scans 1621, 1622, 1623; Background Corrected with Scan 1616

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.0	106741	PASS
68	69	0.00	2	1.5	1342	PASS
69	198	0.00	100	38.9	86618	PASS
70	69	0.00	2	0.3	226	PASS
127	198	10	80	50.3	111898	PASS
197	198	0.00	2	0.6	1370	PASS
198	198	100	100	100.0	222485	PASS
199	198	5	9	6.7	14945	PASS
275	198	10	60	27.3	60664	PASS
365	198	1	100	3.1	7006	PASS
441	198	0.01	100	13.5	30138	PASS
442	198	50	100	84.0	186829	PASS
443	442	15	24	19.8	36998	PASS