


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF051019\
 Data File : BF114123.D
 Acq On : 10 May 2019 16:23
 Operator : JU/SJ
 Sample : DFTPP
 Misc : 8
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 10 15:56:46 2019

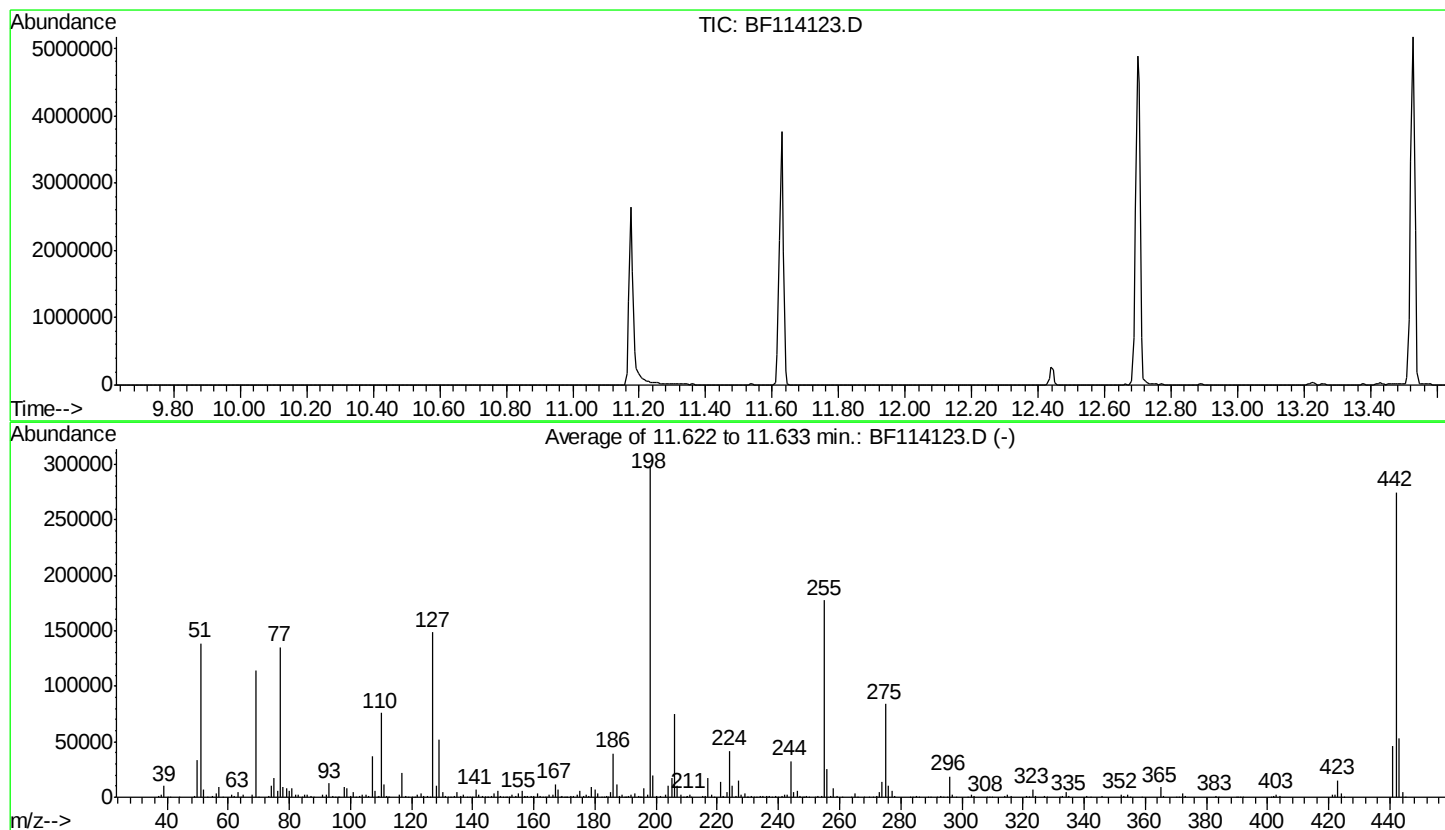

AutoFind: Scans 1621, 1622, 1623; Background Corrected with Scan 1615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.4	138664	PASS
68	69	0.00	2	1.6	1806	PASS
69	198	0.00	100	38.4	114773	PASS
70	69	0.00	2	0.5	529	PASS
127	198	10	80	49.7	148413	PASS
197	198	0.00	2	0.8	2490	PASS
198	198	100	100	100.0	298730	PASS
199	198	5	9	6.7	20158	PASS
275	198	10	60	28.0	83696	PASS
365	198	1	100	3.0	9058	PASS
441	198	0.01	100	15.3	45706	PASS
442	198	50	100	92.0	274914	PASS
443	442	15	24	19.2	52773	PASS