

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF051119\  
 Data File : BF114152.D  
 Acq On : 11 May 2019 12:56  
 Operator : JU/SJ  
 Sample : PB119622BL  
 Misc :  
 ALS Vial : 5 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 PB119622BL

Integration Parameters: rteint.p  
 Integrator: RTE  
 Smoothing : ON  
 Sampling : 1  
 Start Thrs: 0.2  
 Stop Thrs : 0  
 Filtering: 5  
 Min Area: 3 % of largest Peak  
 Max Peaks: 100  
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF051019.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 2.228       | 20            | 24          | 37           | rVB      | 173537         | 300981        | 3.28%           | 0.387%        |
| 2         | 5.492       | 574           | 579         | 582          | rBV      | 7181905        | 7633184       | 83.21%          | 9.814%        |
| 3         | 6.486       | 743           | 748         | 751          | rBV      | 7000400        | 8151285       | 88.86%          | 10.480%       |
| 4         | 6.622       | 767           | 771         | 775          | rBV      | 7476728        | 7853800       | 85.61%          | 10.098%       |
| 5         | 6.851       | 806           | 810         | 813          | rBV      | 2443923        | 2097823       | 22.87%          | 2.697%        |
| 6         | 7.010       | 832           | 837         | 840          | rBV      | 6488867        | 6251355       | 68.15%          | 8.037%        |
| 7         | 7.410       | 899           | 905         | 908          | rBV      | 5169168        | 5234473       | 57.06%          | 6.730%        |
| 8         | 8.127       | 1022          | 1027        | 1031         | rBV      | 2771830        | 2642985       | 28.81%          | 3.398%        |
| 9         | 9.204       | 1204          | 1210        | 1213         | rBV      | 8926374        | 8933158       | 97.38%          | 11.485%       |
| 10        | 9.880       | 1320          | 1325        | 1329         | rBV      | 3167466        | 3018331       | 32.90%          | 3.881%        |
| 11        | 10.674      | 1455          | 1460        | 1463         | rBV      | 5730697        | 5656390       | 61.66%          | 7.272%        |
| 12        | 11.368      | 1573          | 1578        | 1581         | rBV      | 3830705        | 3300971       | 35.98%          | 4.244%        |
| 13        | 12.951      | 1842          | 1847        | 1851         | rBV      | 8389022        | 9173432       | 100.00%         | 11.794%       |
| 14        | 14.004      | 2022          | 2026        | 2029         | rBV      | 3514747        | 3098122       | 33.77%          | 3.983%        |
| 15        | 14.468      | 2100          | 2105        | 2108         | rBV2     | 85877          | 111801        | 1.22%           | 0.144%        |
| 16        | 14.774      | 2153          | 2157        | 2161         | rBV      | 149773         | 158149        | 1.72%           | 0.203%        |
| 17        | 15.115      | 2210          | 2215        | 2219         | rBV      | 204981         | 244958        | 2.67%           | 0.315%        |
| 18        | 15.468      | 2269          | 2275        | 2283         | rBV      | 2362397        | 3318524       | 36.18%          | 4.267%        |
| 19        | 15.921      | 2347          | 2352        | 2358         | rVB      | 197181         | 303744        | 3.31%           | 0.391%        |
| 20        | 16.427      | 2432          | 2438        | 2450         | rVB      | 150274         | 295861        | 3.23%           | 0.380%        |


Sum of corrected areas: 77779327

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF051119\  
Data File : BF114152.D  
Acq On : 11 May 2019 12:56  
Operator : JU/SJ  
Sample : PB119622BL  
Misc :  
ALS Vial : 5 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
PB119622BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF051019.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

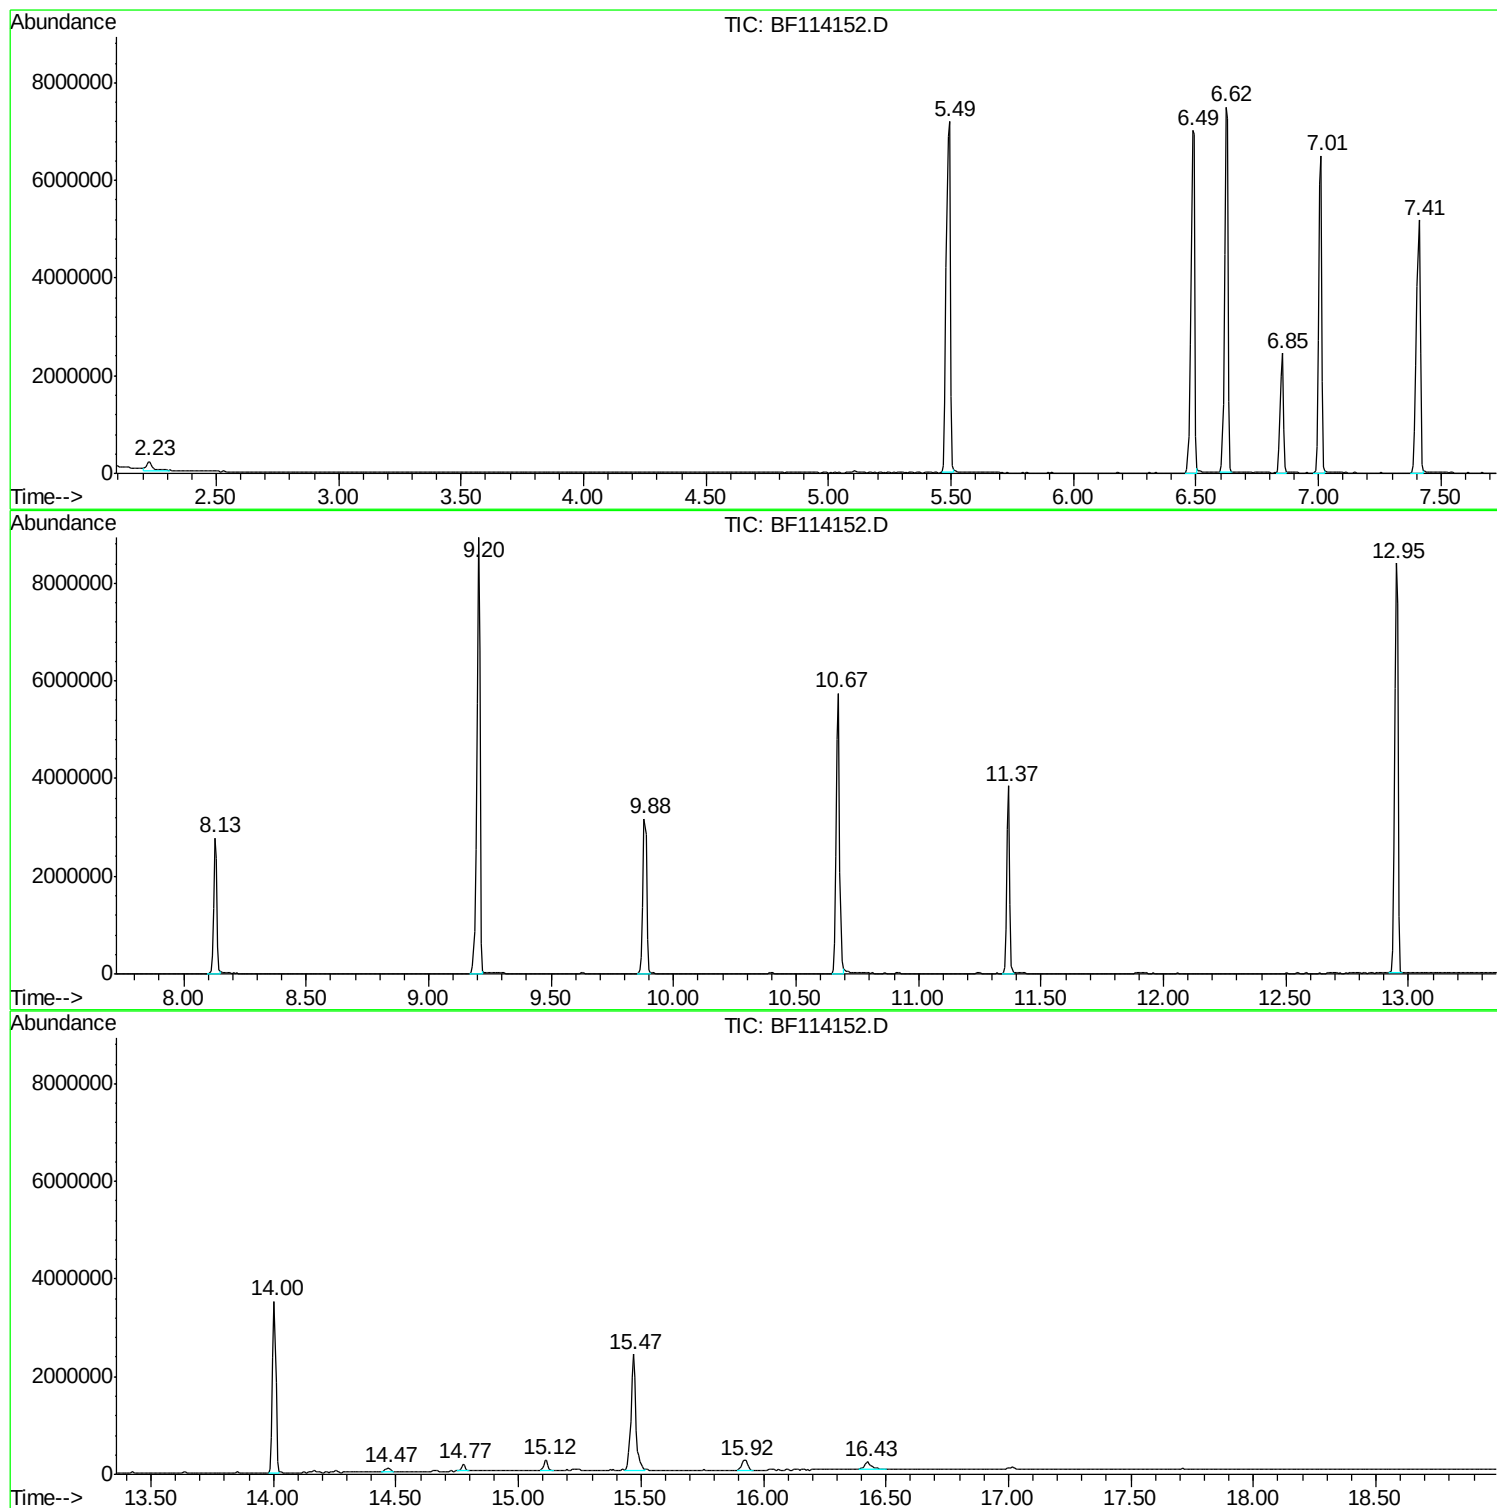

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF051119\  
Data File : BF114152.D  
Acq On : 11 May 2019 12:56  
Operator : JU/SJ  
Sample : PB119622BL  
Misc :  
ALS Vial : 5 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
PB119622BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF051019.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF051119\  
Data File : BF114152.D  
Acq On : 11 May 2019 12:56  
Operator : JU/SJ  
Sample : PB119622BL  
Misc :  
ALS Vial : 5 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
PB119622BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF051019.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |
|------------------|----|---------|-------|----------|-----------------------|
|                  |    |         |       |          | # RT Resp Conc        |