

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051119\
 Data File : BF114153.D
 Acq On : 11 May 2019 13:34
 Operator : JU/SJ
 Sample : K2781-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OUTFALL001-WK-2

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.475	572	576	592	rBV	3058211	3304900	15.81%	2.668%
2	6.481	744	747	760	rBV	2432100	2246034	10.74%	1.813%
3	6.622	767	771	775	rBV	6500805	6082012	29.09%	4.909%
4	6.851	806	810	813	rBV	2031062	1665768	7.97%	1.345%
5	7.010	832	837	840	rBV	6331382	5655184	27.05%	4.565%
6	7.410	900	905	908	rBV	5364359	5113527	24.46%	4.127%
7	8.127	1024	1027	1031	rBV	2435829	2158472	10.32%	1.742%
8	9.204	1205	1210	1213	rBV	9100987	8531860	40.80%	6.887%
9	9.880	1321	1325	1329	rBV	2654493	2514612	12.03%	2.030%
10	10.674	1455	1460	1463	rBV	4919972	4976879	23.80%	4.017%
11	10.727	1463	1469	1470	rVV	213571	335322	1.60%	0.271%
12	10.769	1474	1476	1481	rVB	295105	477002	2.28%	0.385%
13	11.368	1574	1578	1581	rBV	2809165	2488652	11.90%	2.009%
14	11.892	1660	1667	1687	rBV	1048884	1637489	7.83%	1.322%
15	12.604	1781	1788	1793	rBV6	117234	342022	1.64%	0.276%
16	12.680	1794	1801	1807	rBV	2497460	3676182	17.58%	2.967%
17	12.951	1842	1847	1851	rVB	7789620	8345245	39.91%	6.736%
18	13.310	1890	1908	1921	rBV	5734155	20909790	100.00%	16.878%
19	13.851	1996	2000	2002	rBV	211540	264788	1.27%	0.214%
20	13.909	2003	2010	2012	rBV2	380077	795686	3.81%	0.642%
21	14.004	2020	2026	2034	rVB	2452260	2665736	12.75%	2.152%
22	14.215	2050	2062	2079	rBV	4760702	14188536	67.86%	11.452%
23	14.474	2102	2106	2110	rBV	1473578	1436819	6.87%	1.160%
24	14.639	2130	2134	2141	rVB3	203435	389779	1.86%	0.315%
25	14.786	2153	2159	2163	rBV	2267989	2534633	12.12%	2.046%
26	14.892	2168	2177	2185	rVV	2422278	5399676	25.82%	4.358%
27	15.121	2211	2216	2225	rVB	2588354	3048272	14.58%	2.460%
28	15.292	2239	2245	2252	rBV5	289685	838731	4.01%	0.677%
29	15.474	2271	2276	2278	rBV	1610969	2264663	10.83%	1.828%
30	15.498	2278	2280	2289	rVB	2351000	2713943	12.98%	2.191%
31	15.639	2296	2304	2313	rVB	731895	1802092	8.62%	1.455%
32	15.933	2347	2354	2364	rBV	1499345	2404019	11.50%	1.940%
33	16.433	2433	2439	2445	rBV	798986	1413387	6.76%	1.141%
34	16.509	2446	2452	2463	rVB3	282657	762074	3.64%	0.615%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051119\
Data File : BF114153.D
Acq On : 11 May 2019 13:34
Operator : JU/SJ
Sample : K2781-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OUTFALL001-WK-2

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051019.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	17.021	2534	2539	2547	rVB2	247968	506745	2.42%	0.409%
----	--------	------	------	------	------	--------	--------	-------	--------


Sum of corrected areas: 123890531

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051119\
Data File : BF114153.D
Acq On : 11 May 2019 13:34
Operator : JU/SJ
Sample : K2781-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OUTFALL001-WK-2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

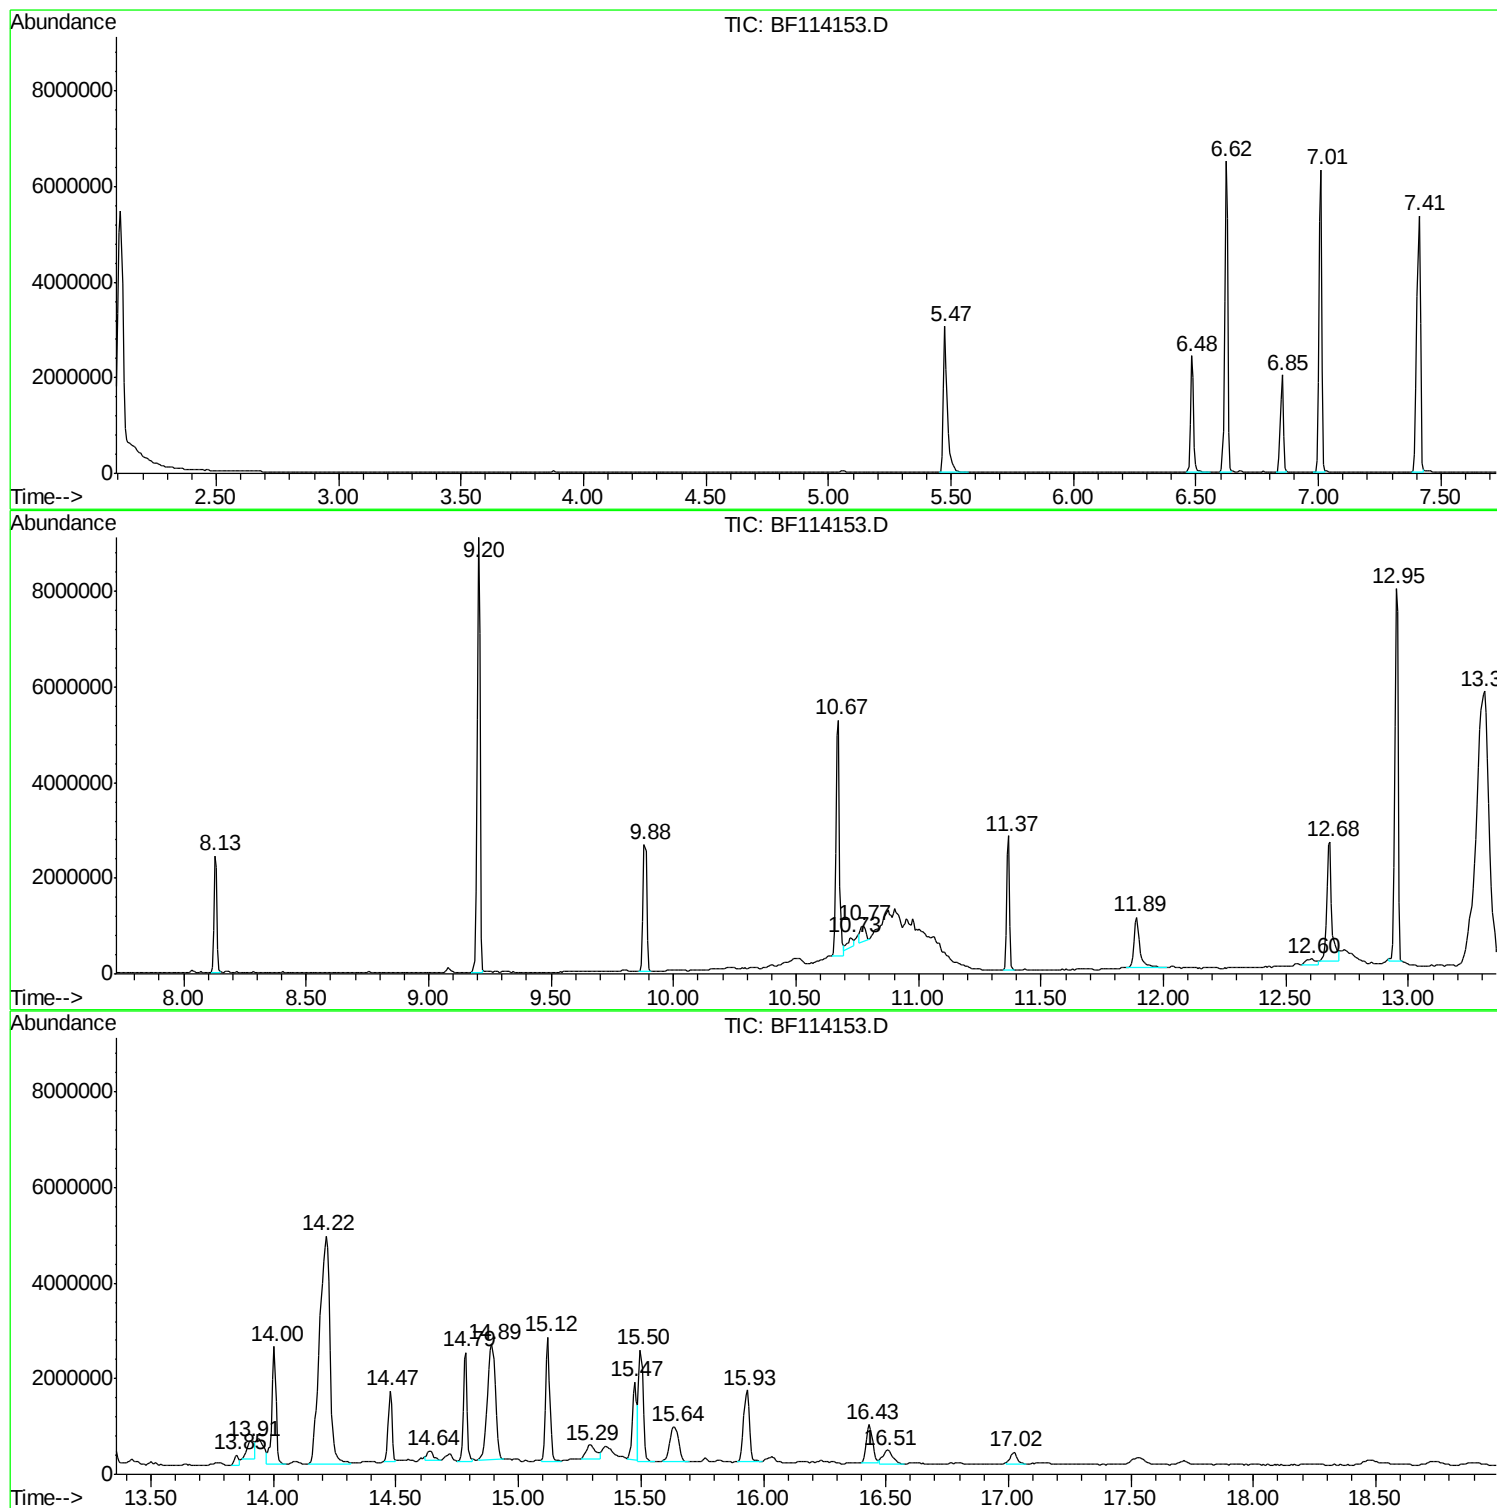

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051119\
Data File : BF114153.D
Acq On : 11 May 2019 13:34
Operator : JU/SJ
Sample : K2781-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OUTFALL001-WK-2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051119\
Data File : BF114153.D
Acq On : 11 May 2019 13:34
Operator : JU/SJ
Sample : K2781-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OUTFALL001-WK-2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc