
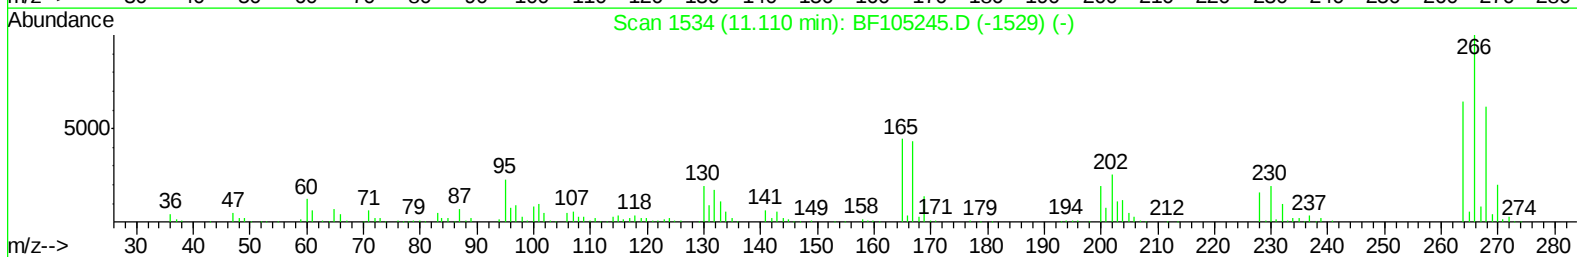
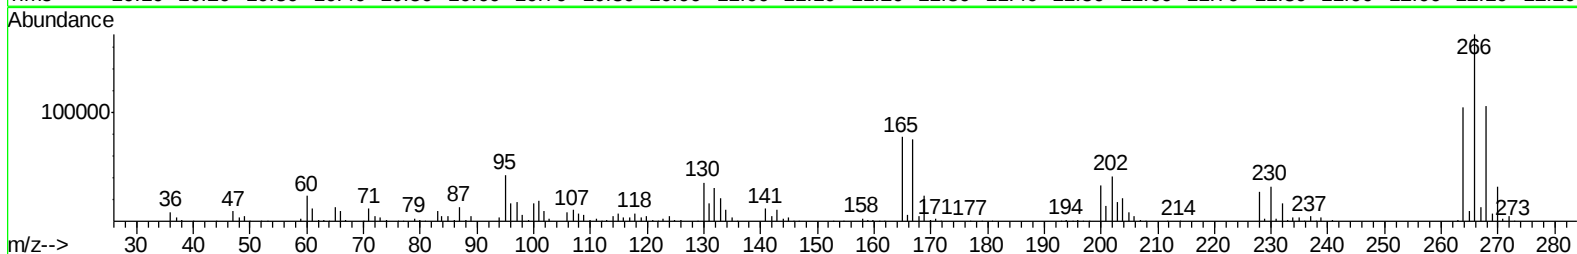


Data Path : Z:\HPCHEM1\BNA F\Data\BF051218\
Data File : BF105331.D
Acq On : 12 May 2018 12:23
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 28 05:56:31 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF051018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 17 16:15:19 2018
Response via : Initial Calibration

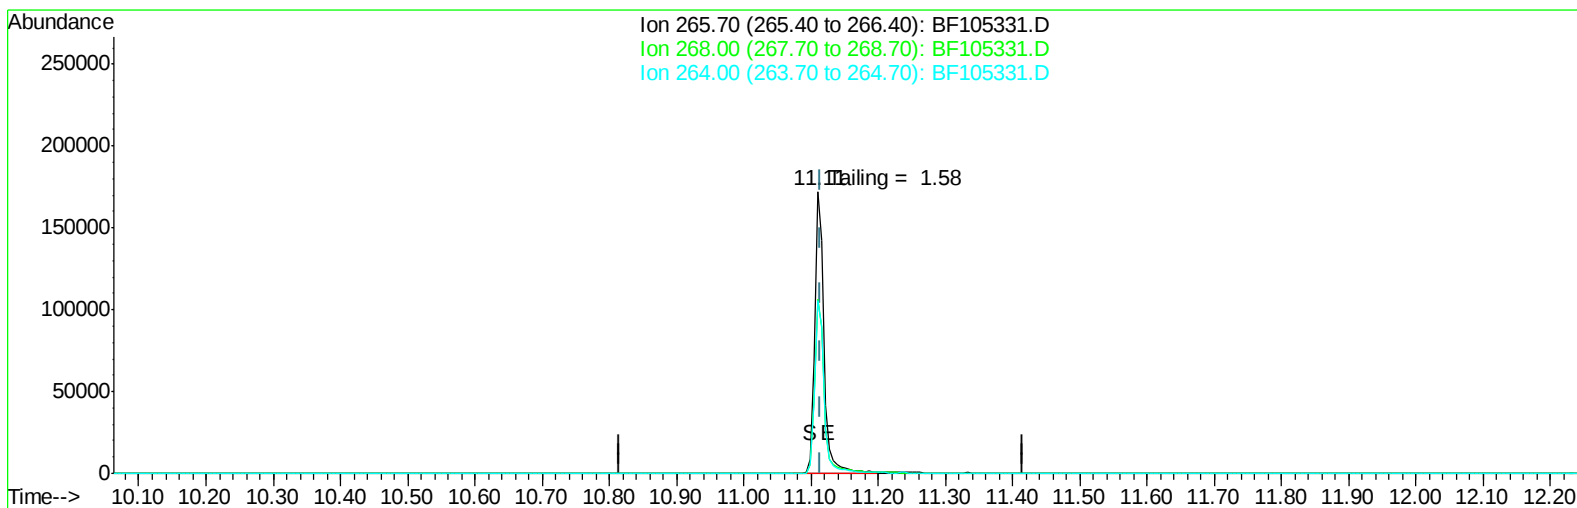

TIC: BF105331.D

(69) Pentachlorophenol (C)




11.110min (-0.006) 37845.21ng

response 171585

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	61.79
264.00	61.90	61.33
0.00	0.00	0.00

```
Data Path : Z:\HPCHEM1\BNA F\Data\BF051218\  
Data File : BF105331.D  
Acq On    : 12 May 2018  12:23  
Operator  : JU/SJ  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1      Sample Multiplier: 1
```

Quant Time: May 28 05:56:31 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF051018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 17 16:15:19 2018
Response via : Initial Calibration

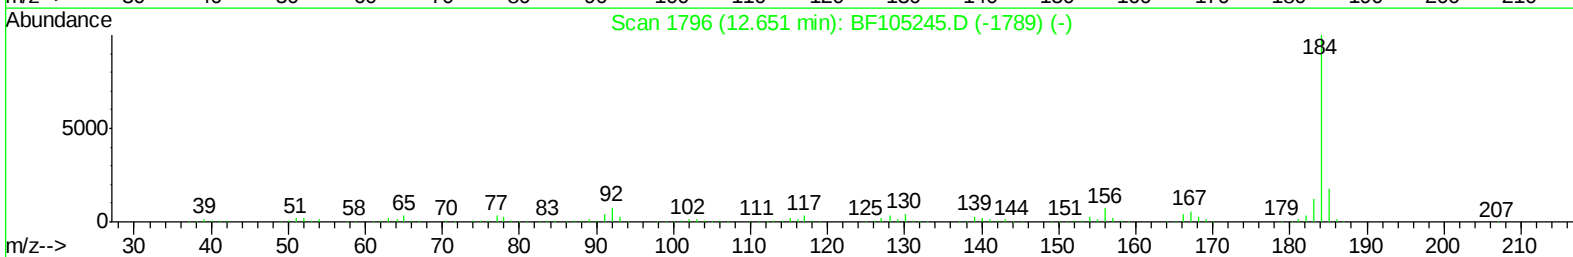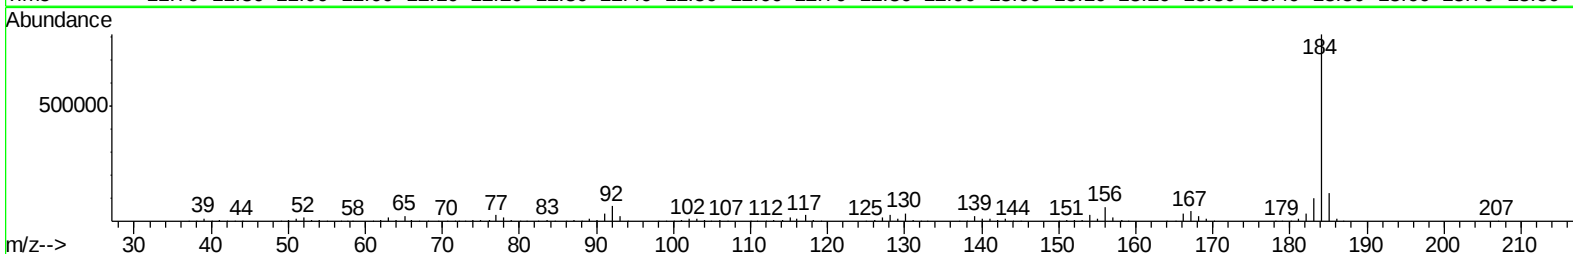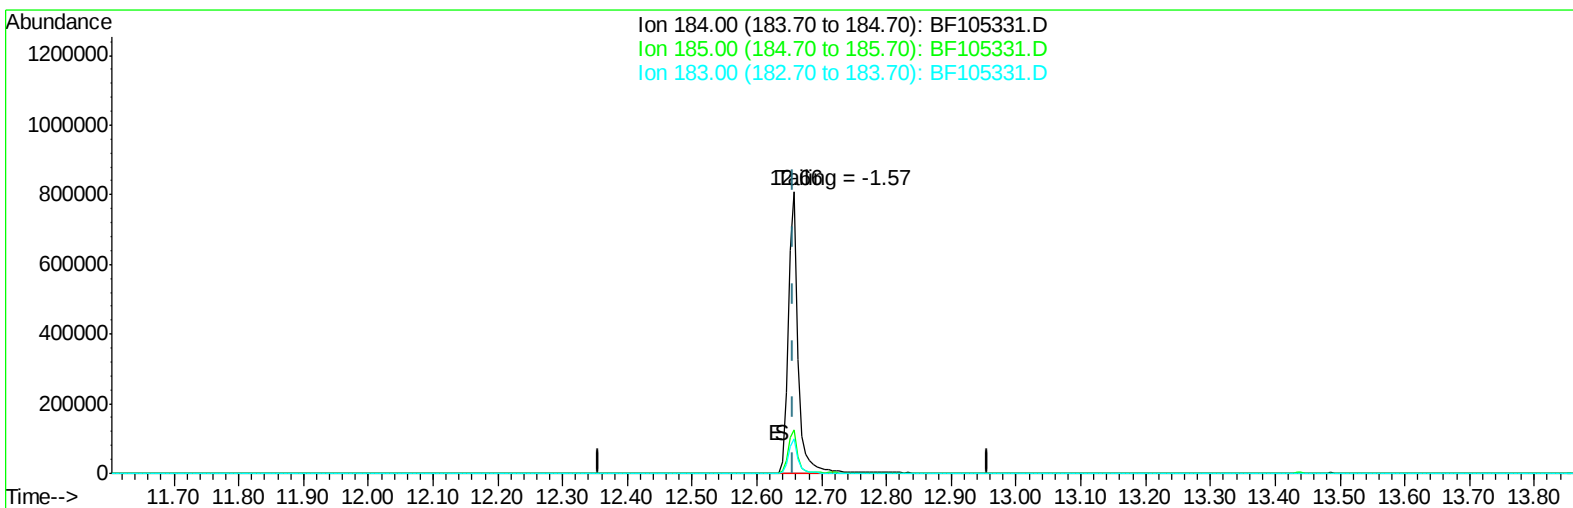

TIC: BF105331.D

(76) Benzidine

12.657min (+0.000) 0.00ng m

response 822135

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	15.38
183.00	11.60	12.32
0.00	0.00	0.00