

Data Path : Z:\HPCHEM1\BNA F\DATA\BF051218\
 Data File : BF105348.D
 Acq On : 12 May 2018 19:58
 Operator : JU/SJ
 Sample : J2834-09
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 050918-SIDI-E-D-S

Quant Time: May 14 09:18:10 2018
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF051018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 11 17:15:19 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.79	152	170364	20.00	ng	0.00
21) Naphthalene-d8	8.07	136	717241	20.00	ng	0.00
38) Acenaphthene-d10	9.82	164	314368	20.00	ng	0.00
63) Phenanthrene-d10	11.31	188	556850	20.00	ng	0.00
75) Chrysene-d12	13.99	240	338640	20.00	ng	-0.02
86) Perylene-d12	15.53	264	390281	20.00	ng	-0.04
System Monitoring Compounds						
5) 2-Fluorophenol	5.40	112	406825	35.92	ng	0.00
7) Phenol-d6	6.42	99	307706	22.86	ng	0.00
23) Nitrobenzene-d5	7.36	82	1111873	90.22	ng	0.00
41) 2,4,6-Tribromophenol	10.62	330	332185	81.79	ng	0.00
44) 2-Fluorobiphenyl	9.15	172	1753156	80.38	ng	0.00
78) Terphenyl-d14	12.90	244	1563297	99.24	ng	0.00
Target Compounds						Qvalue
49) Dimethylphthalate	9.54	163	129036	5.347	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF051218\
Data File : BF105348.D
Acq On : 12 May 2018 19:58
Operator : JU/SJ
Sample : J2834-09
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
050918-SIDI-E-D-S

Quant Time: May 14 09:18:10 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF051018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 11 17:15:19 2018
Response via : Initial Calibration

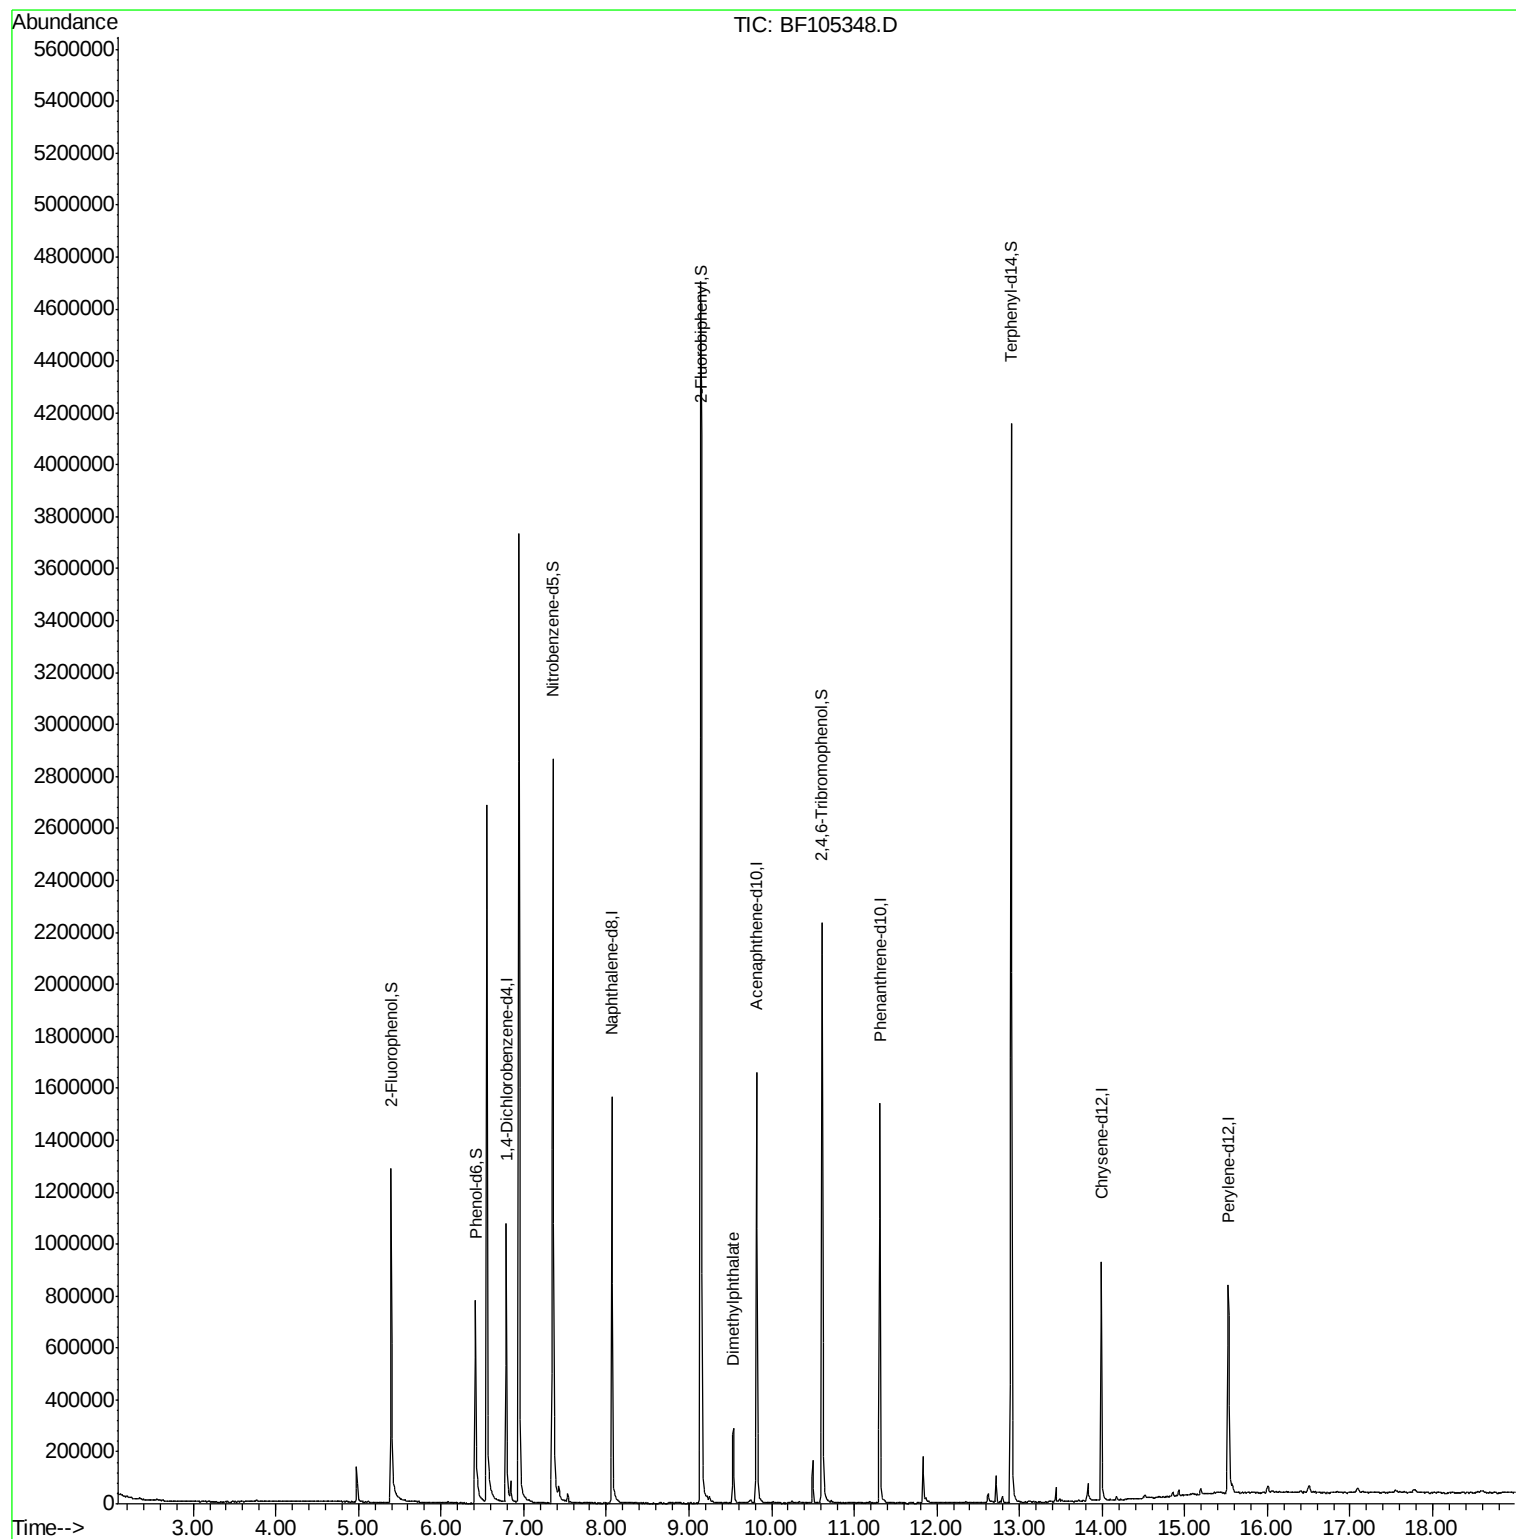

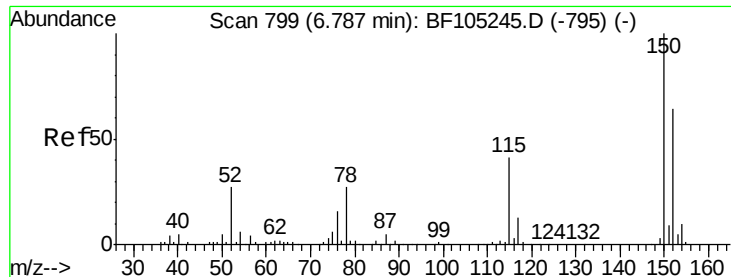


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.79 min Scan# 799
Delta R.T. -0.01 min
Lab File: BF105348.D
Acq: 12 May 2018 19:58

Instrument :
BNA_F
ClientSampleId :
050918-SIDI-E-D-S

Tot Ion:152 Resp: 170364
Ion Ratio Lower Upper
152 100
150 159.2 124.6 186.8
115 63.7 50.1 75.1

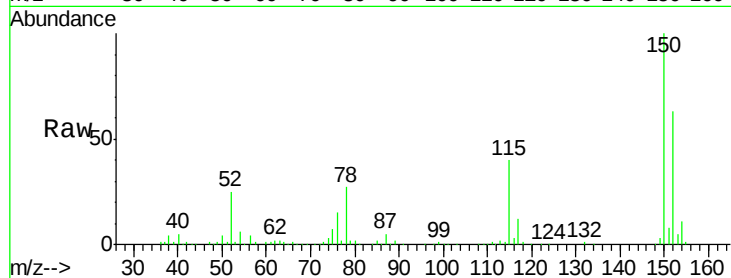


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

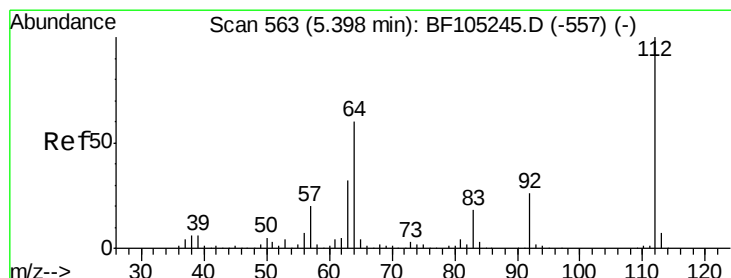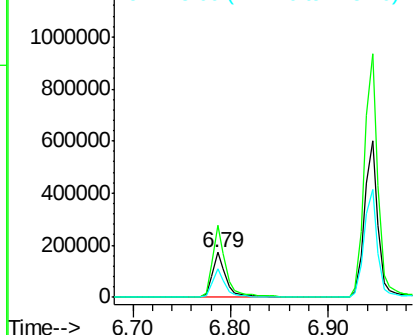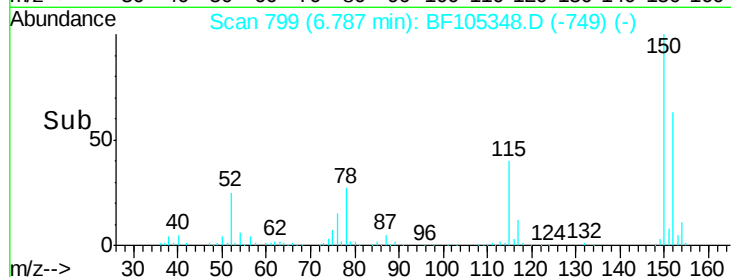



#5


2-Fluorophenol
Concen: 35.916 ng
RT: 5.40 min Scan# 563
Delta R.T. 0.00 min
Lab File: BF105348.D
Acq: 12 May 2018 19:58

Tgt Ion:112 Resp: 406825
Ion Ratio Lower Upper
112 100
64 60.9 47.9 71.9
63 31.6 23.7 35.5

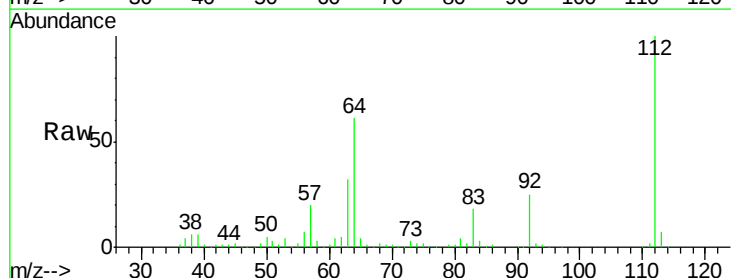

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

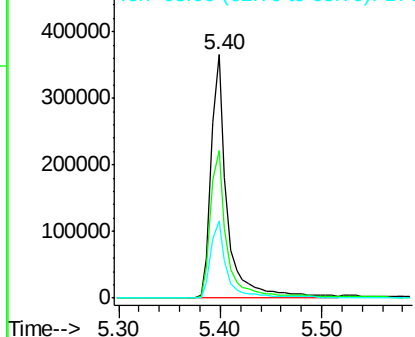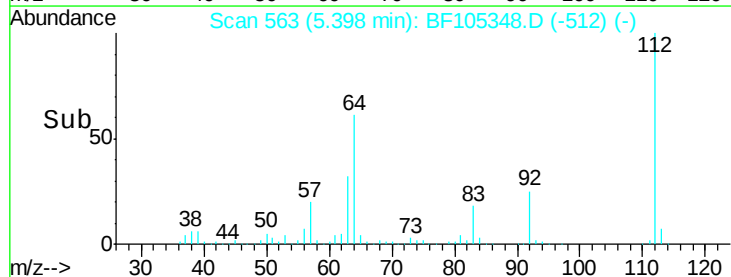

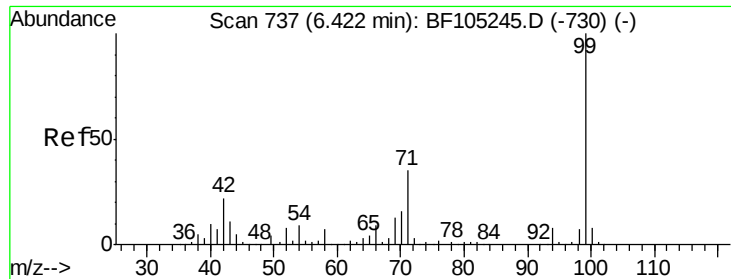

#7

Phenol-d6

Concen: 22.861 ng

RT: 6.42 min Scan# 736

Delta R.T. -0.01 min

Lab File: BF105348.D

Acq: 12 May 2018 19:58

Instrument :

BNA_F

ClientSampleId :

050918-SIDI-E-D-S


Tot Ion: 99 Resp: 307706

Ion Ratio Lower Upper

99 100

42 20.0 14.5 21.7




71 33.0 25.4 38.0

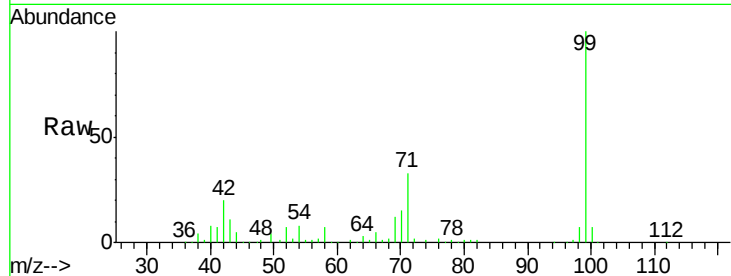

Abundance Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

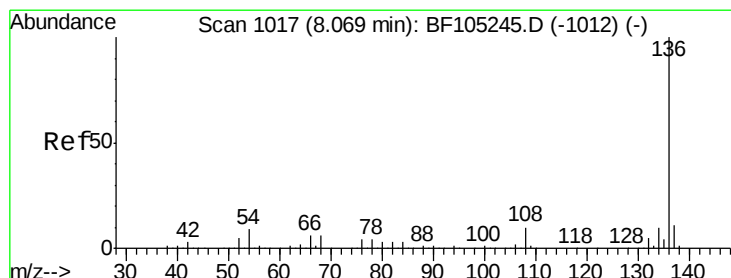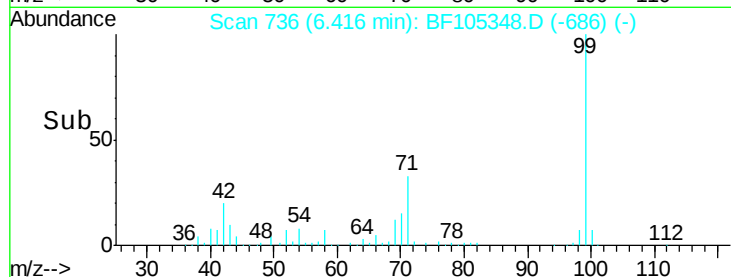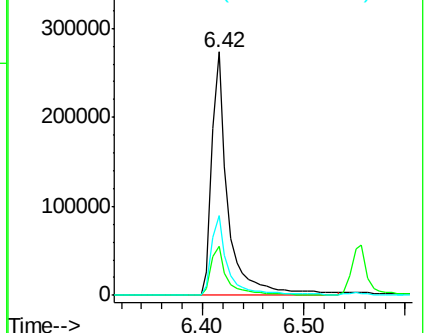

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.07 min Scan# 1017

Delta R.T. -0.01 min

Lab File: BF105348.D

Acq: 12 May 2018 19:58

Tgt Ion: 136 Resp: 717241


Ion Ratio Lower Upper

136 100

137 11.5 8.9 13.3

54 9.4 6.6 9.8

68 6.3 5.0 7.4


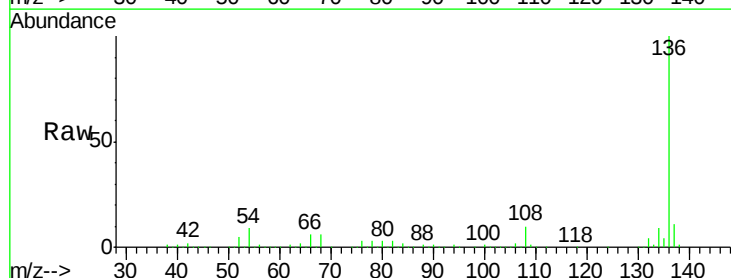



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1

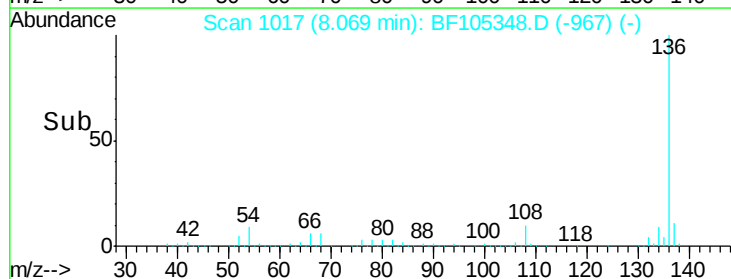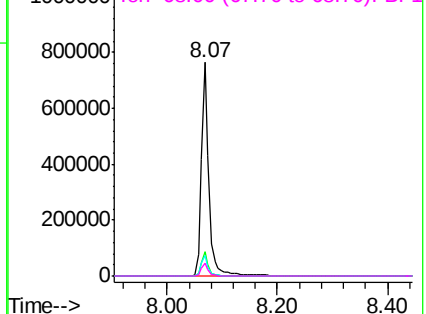

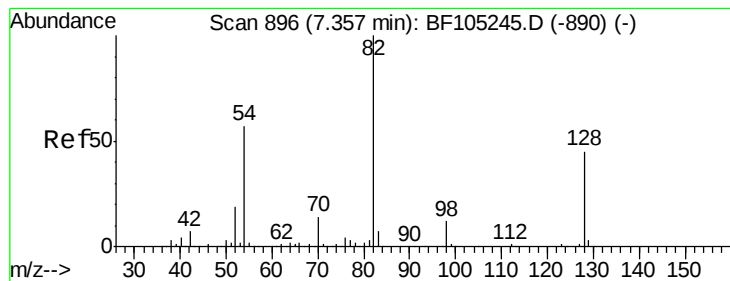

#23

Nitrobenzene-d5

Concen: 90.225 ng

RT: 7.36 min Scan# 896

Delta R.T. 0.00 min

Lab File: BF105348.D

Acq: 12 May 2018 19:58

Instrument :

BNA_F

ClientSampleId :

050918-SIDI-E-D-S


Tot Ion: 82 Resp: 1111873

Ion Ratio Lower Upper

82 100

128 45.3 36.1 54.1




54 57.4 41.4 62.2

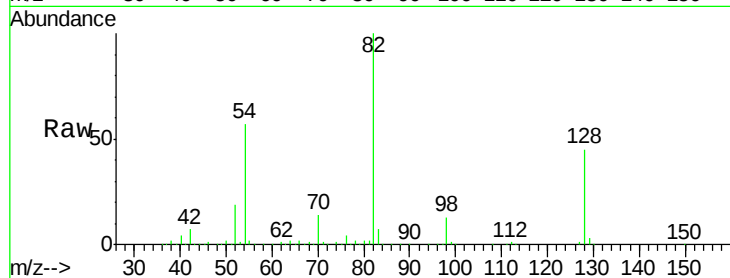

Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 128.00 (127.70 to 128.70): BF1

Ion 54.00 (53.70 to 54.70): BF1

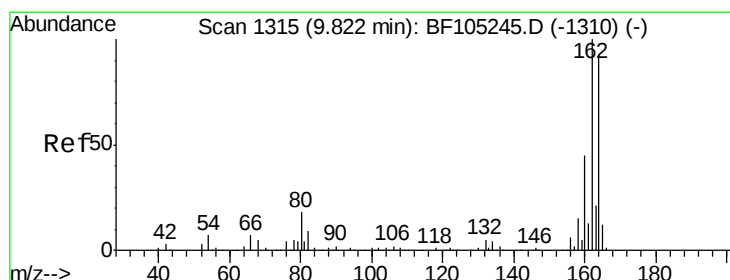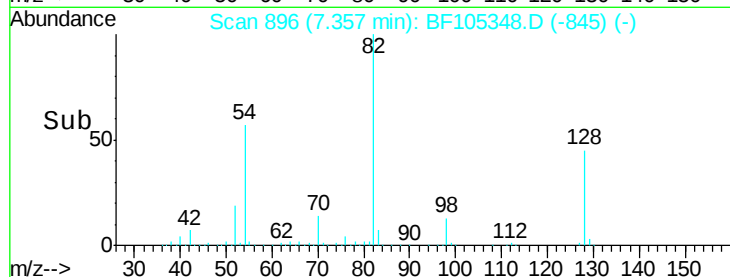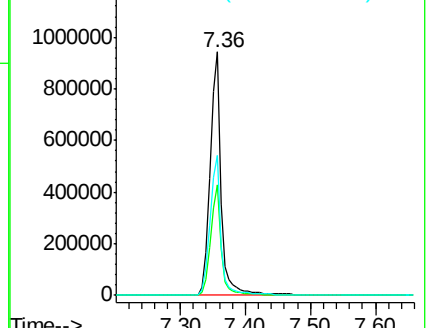

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.82 min Scan# 1315

Delta R.T. -0.01 min

Lab File: BF105348.D

Acq: 12 May 2018 19:58


Tgt Ion:164 Resp: 314368

Ion Ratio Lower Upper

164 100

162 105.7 86.1 129.1



160 47.1 38.3 57.5

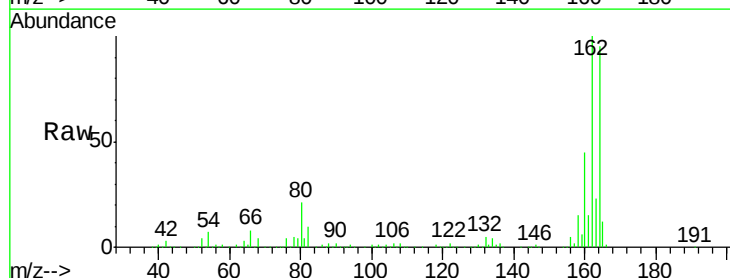


Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E



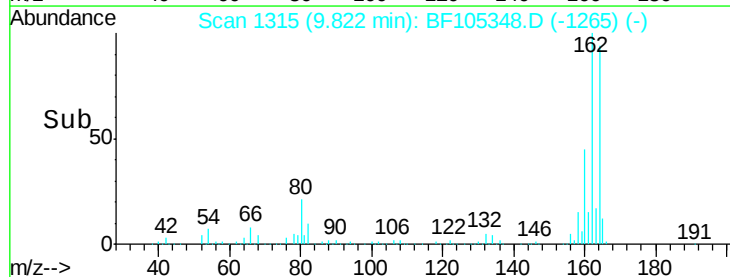
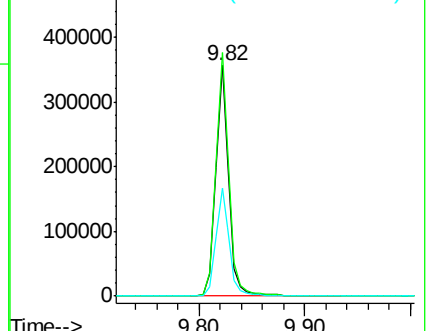


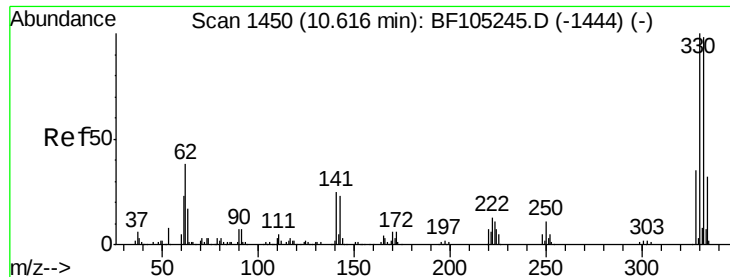

#41
 2,4,6-Tribromophenol
 Concen: 81.788 ng
 RT: 10.62 min Scan# 1450
 Delta R.T. 0.00 min
 Lab File: BF105348.D
 Acq: 12 May 2018 19:58




Instrument :
 BNA_F
 ClientSampleId :
 050918-SIDI-E-D-S


Tot Ion	Ratio	Lower	Upper
330	100		
332	96.1	77.0	115.6
141	30.2	29.9	44.9

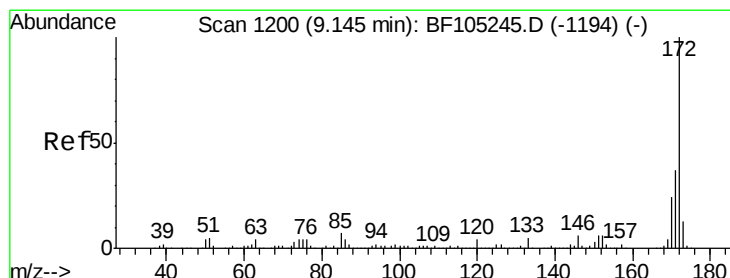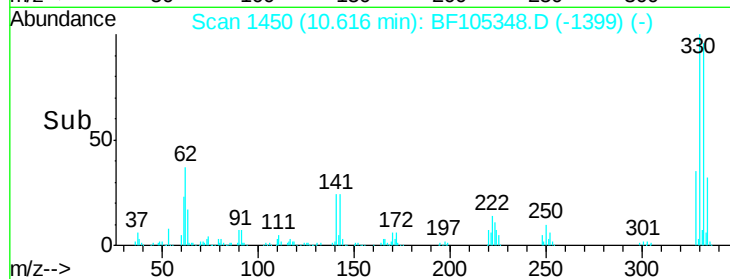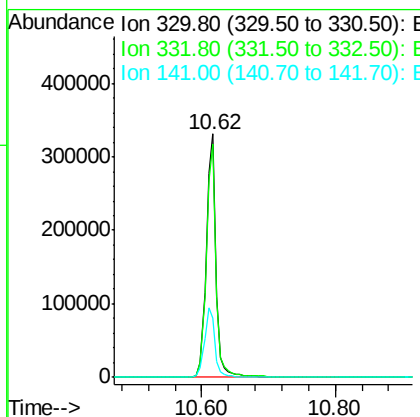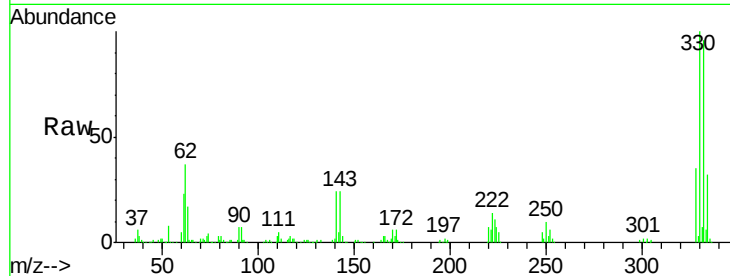

#44
 2-Fluorobiphenyl
 Concen: 80.378 ng
 RT: 9.15 min Scan# 1200
 Delta R.T. -0.01 min
 Lab File: BF105348.D
 Acq: 12 May 2018 19:58

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.3	29.7	44.5
170	24.3	19.6	29.4

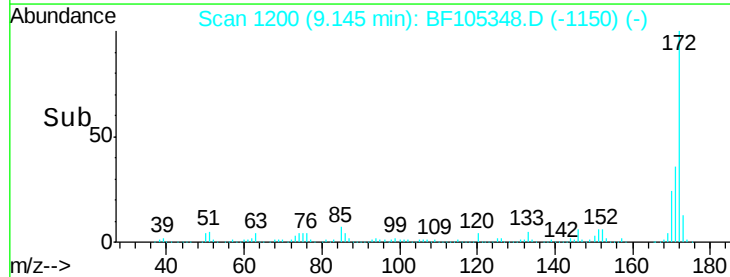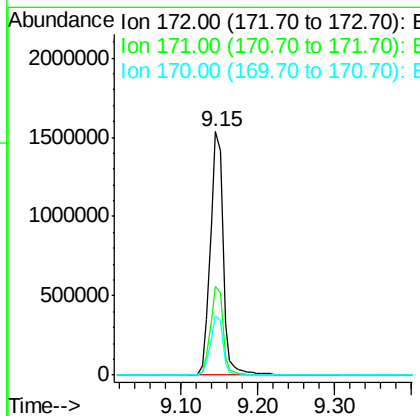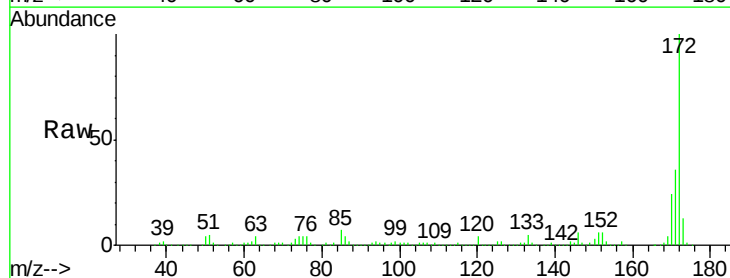

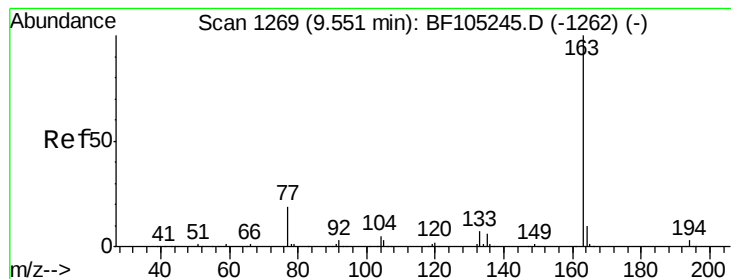

#49

Dimethylphthalate

Concen: 5.347 ng

RT: 9.54 min Scan# 1267

Delta R.T. -0.01 min

Lab File: BF105348.D

Acq: 12 May 2018 19:58

Instrument :

BNA_F

ClientSampleId :

050918-SIDI-E-D-S


Tot Ion:163 Resp: 129036

Ion Ratio Lower Upper

163 100

194 3.9 2.7 4.1




164 9.7 8.2 12.2

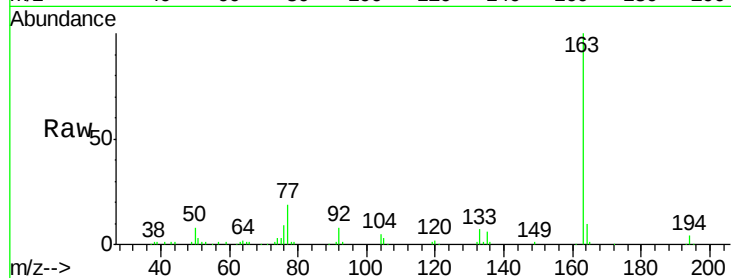

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

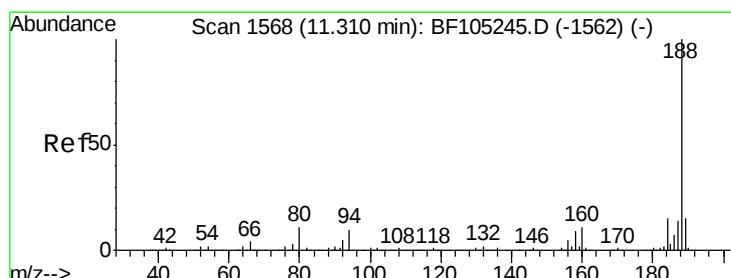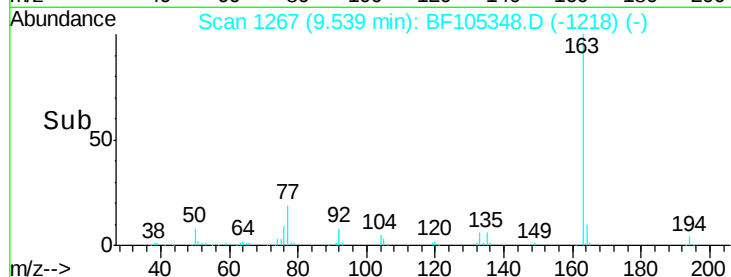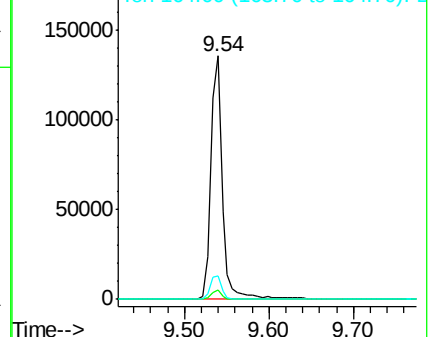

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.31 min Scan# 1568

Delta R.T. 0.00 min

Lab File: BF105348.D

Acq: 12 May 2018 19:58


Tgt Ion:188 Resp: 556850

Ion Ratio Lower Upper

188 100

94 10.2 8.5 12.7



80 11.1 9.2 13.8

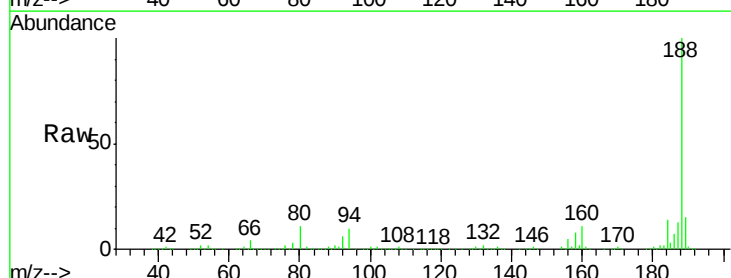


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

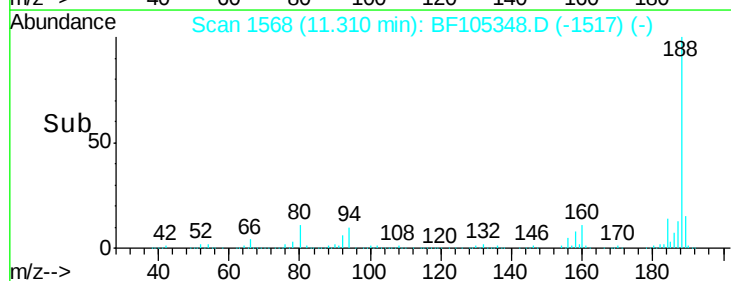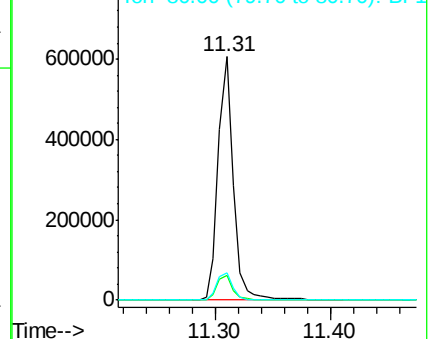

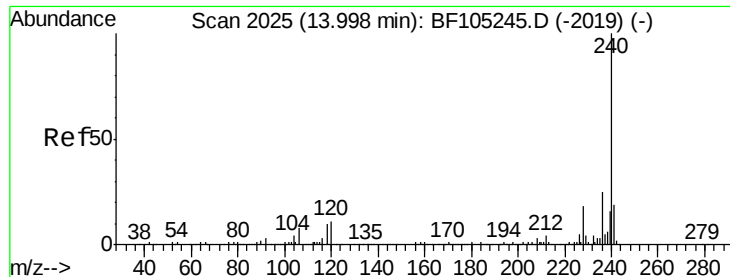

#75

Chrvsene-d12

Concen: 20.000 ng

RT: 13.99 min Scan# 2024

Delta R.T. -0.02 min

Lab File: BF105348.D

Acq: 12 May 2018 19:58

Instrument :

BNA_F

ClientSampleId :

050918-SIDI-E-D-S


Tot Ion:240 Resp: 338640

Ion Ratio Lower Upper

240 100

120 12.5 9.5 14.3




236 24.3 20.7 31.1

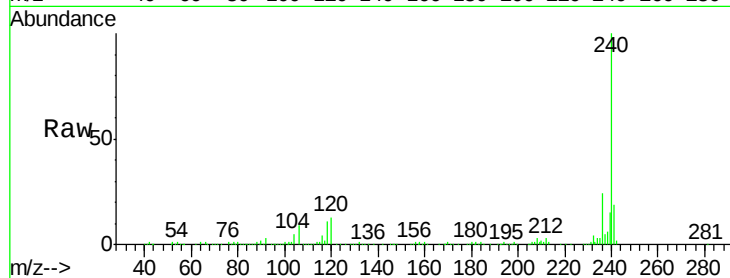

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

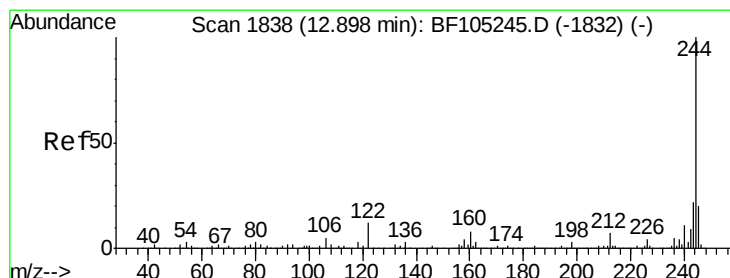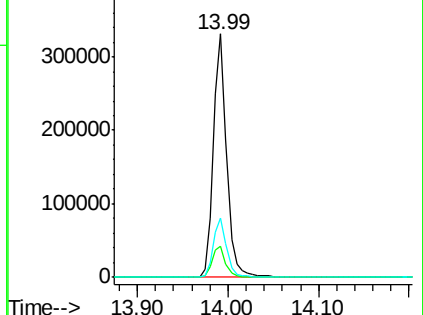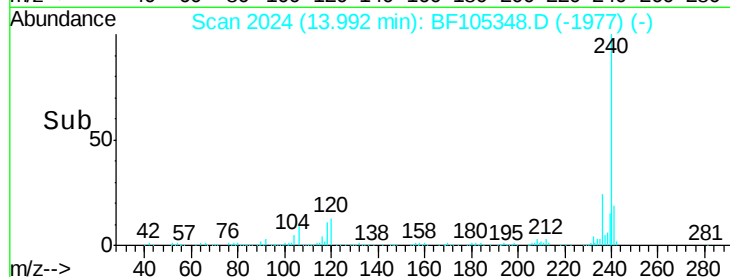

#78

Terphenyl-d14

Concen: 99.237 ng

RT: 12.90 min Scan# 1839

Delta R.T. 0.00 min

Lab File: BF105348.D

Acq: 12 May 2018 19:58


Tgt Ion:244 Resp: 1563297

Ion Ratio Lower Upper

244 100

212 6.6 5.4 8.0



122 11.9 11.0 16.4



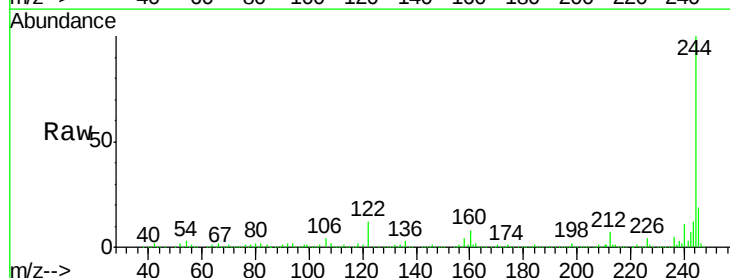


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

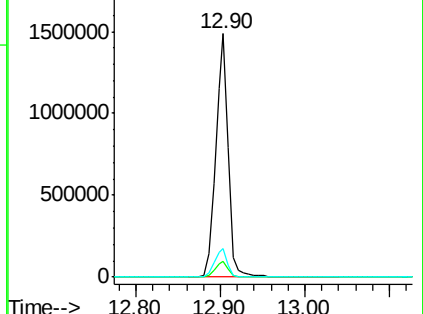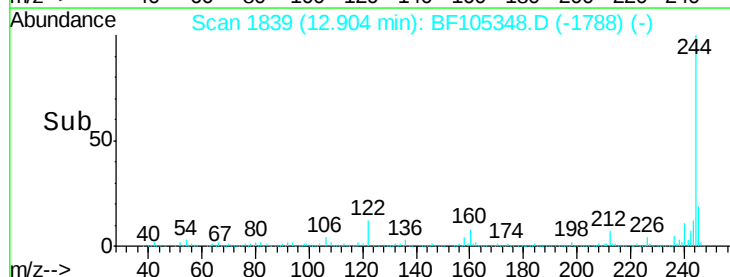

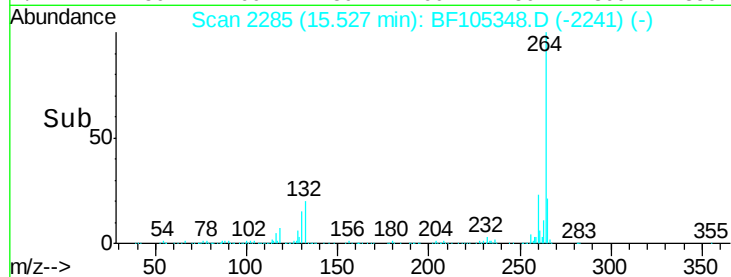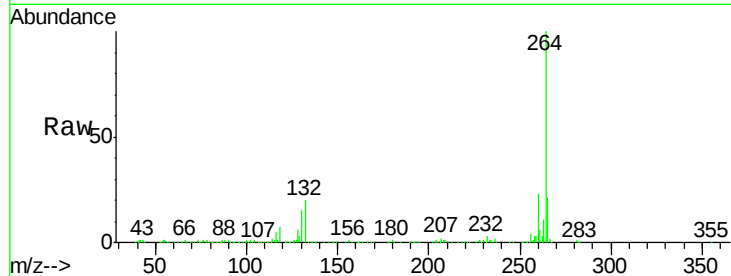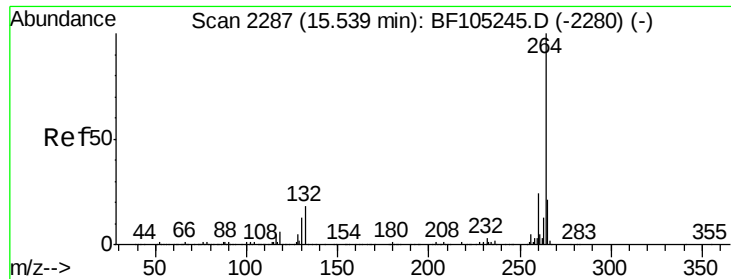

#86

Pervlene-d12

Concen: 20.000 ng

RT: 15.53 min Scan# 2285

Delta R.T. -0.04 min

Lab File: BF105348.D

Acq: 12 May 2018 19:58

Instrument :

BNA_F

ClientSampleId :

050918-SIDI-E-D-S

Tot Ion:264 Resp: 390281

Ion Ratio Lower Upper

264 100

260 23.3 19.2 28.8

265 20.7 17.5 26.3

