


Data Path : Z:\HPCHEM1\BNA F\Data\BF051218\
 Data File : BF105326.D
 Acq On : 12 May 2018 10:14
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF051018.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon May 14 13:23:31 2018

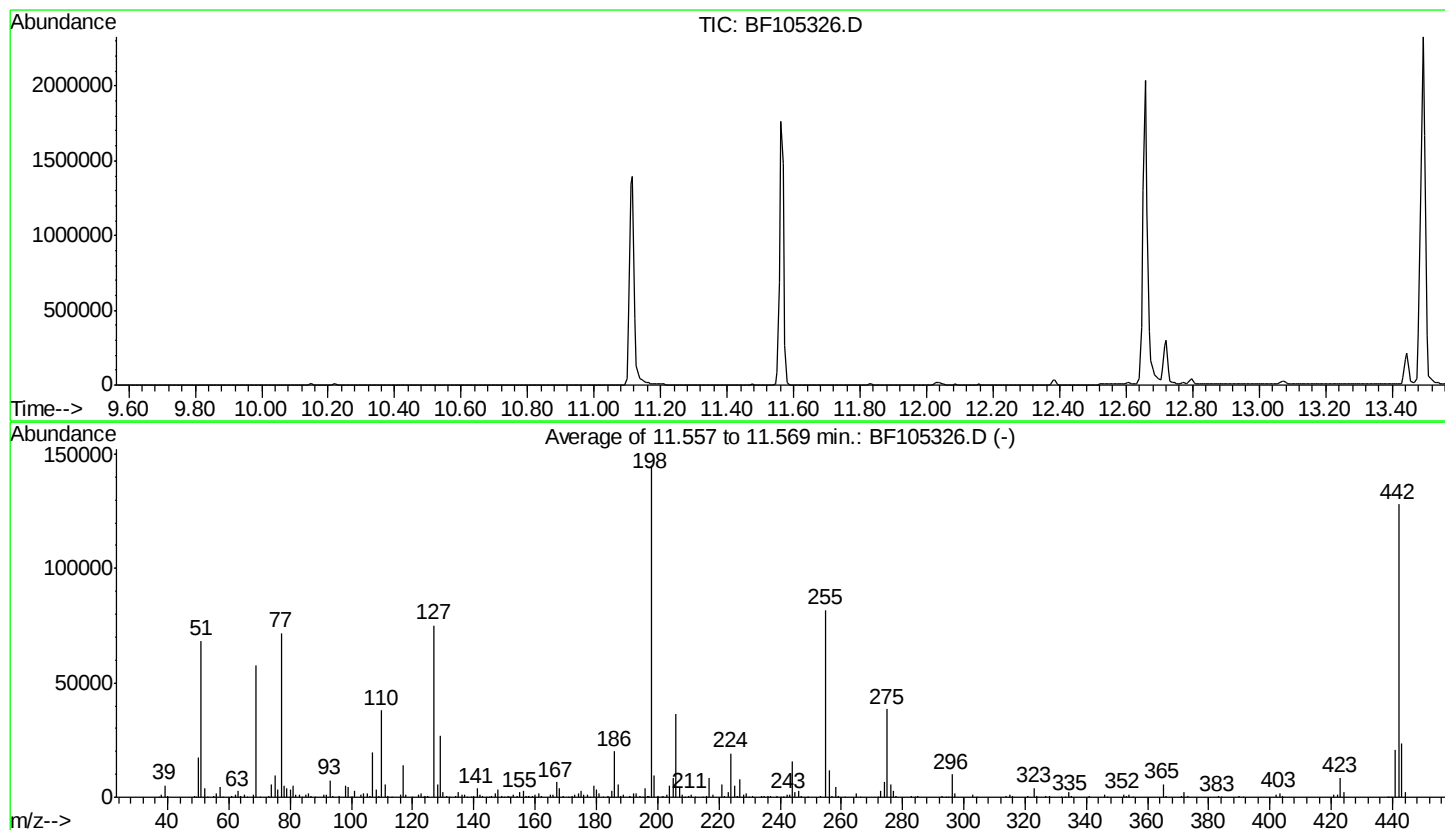

AutoFind: Scans 1610, 1611, 1612; Background Corrected with Scan 1605

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.2	68362	PASS
68	69	0.00	2	1.8	1061	PASS
69	198	0.00	100	39.6	57408	PASS
70	69	0.00	2	0.3	159	PASS
127	198	10	80	51.8	75040	PASS
197	198	0.00	2	0.4	509	PASS
198	198	100	100	100.0	144981	PASS
199	198	5	9	6.6	9587	PASS
275	198	10	60	26.5	38431	PASS
365	198	1	100	4.0	5769	PASS
441	443	0.01	100	88.3	20963	PASS
442	198	50	100	88.3	128090	PASS
443	442	15	24	18.5	23740	PASS