


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF051219\
 Data File : BF114210.D
 Acq On : 12 May 2019 23:54
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 10 15:56:46 2019

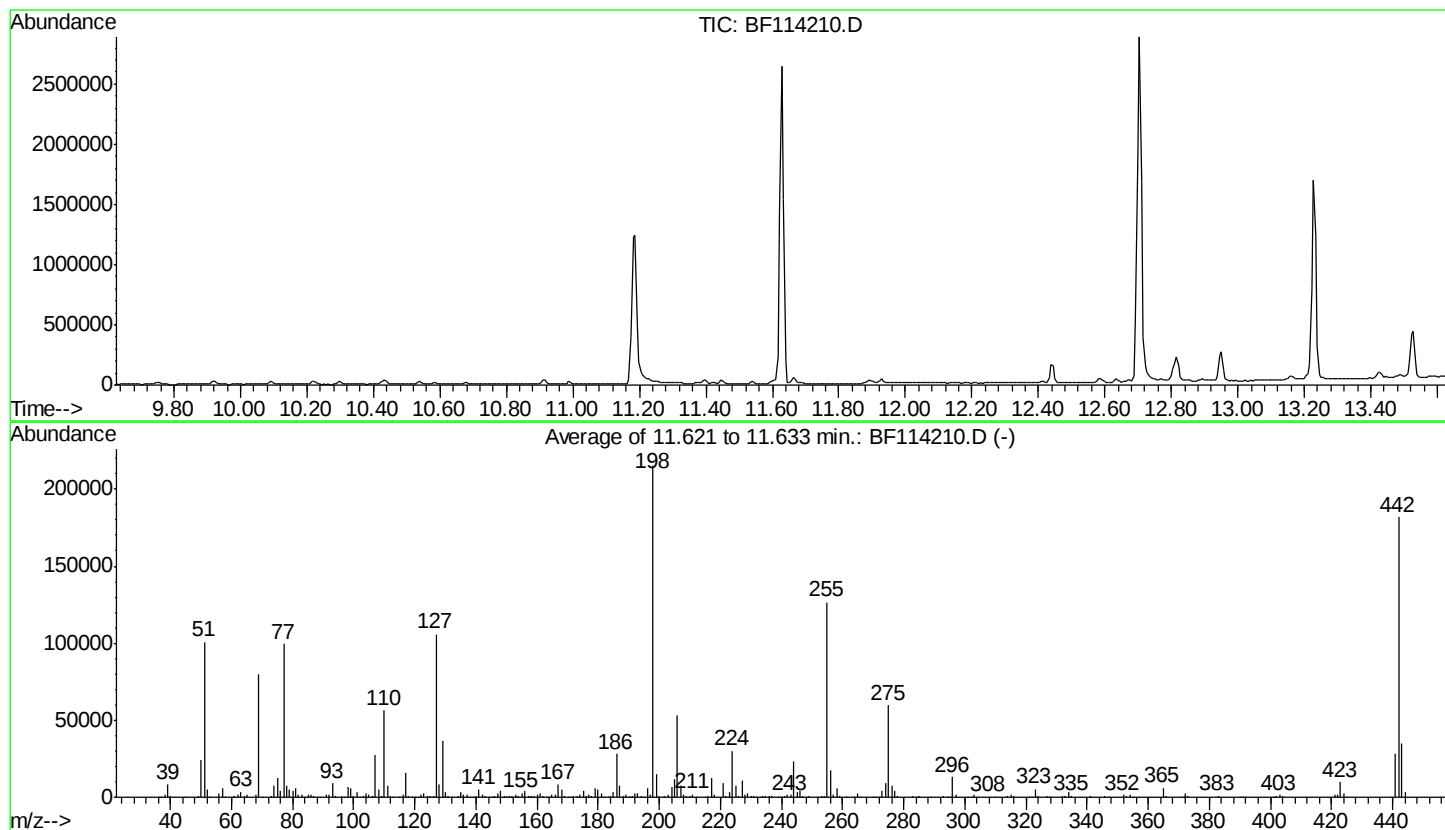

AutoFind: Scans 1621, 1622, 1623; Background Corrected with Scan 1616

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.8	100734	PASS
68	69	0.00	2	1.9	1540	PASS
69	198	0.00	100	37.2	80111	PASS
70	69	0.00	2	0.4	319	PASS
127	198	10	80	49.2	105850	PASS
197	198	0.00	2	0.7	1489	PASS
198	198	100	100	100.0	215253	PASS
199	198	5	9	7.0	15039	PASS
275	198	10	60	27.7	59610	PASS
365	198	1	100	2.8	5997	PASS
441	198	0.01	100	13.3	28653	PASS
442	198	50	100	84.5	181784	PASS
443	442	15	24	19.1	34704	PASS