


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051419\
 Data File : BF114255.D
 Acq On : 14 May 2019 14:59
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 10 15:56:46 2019

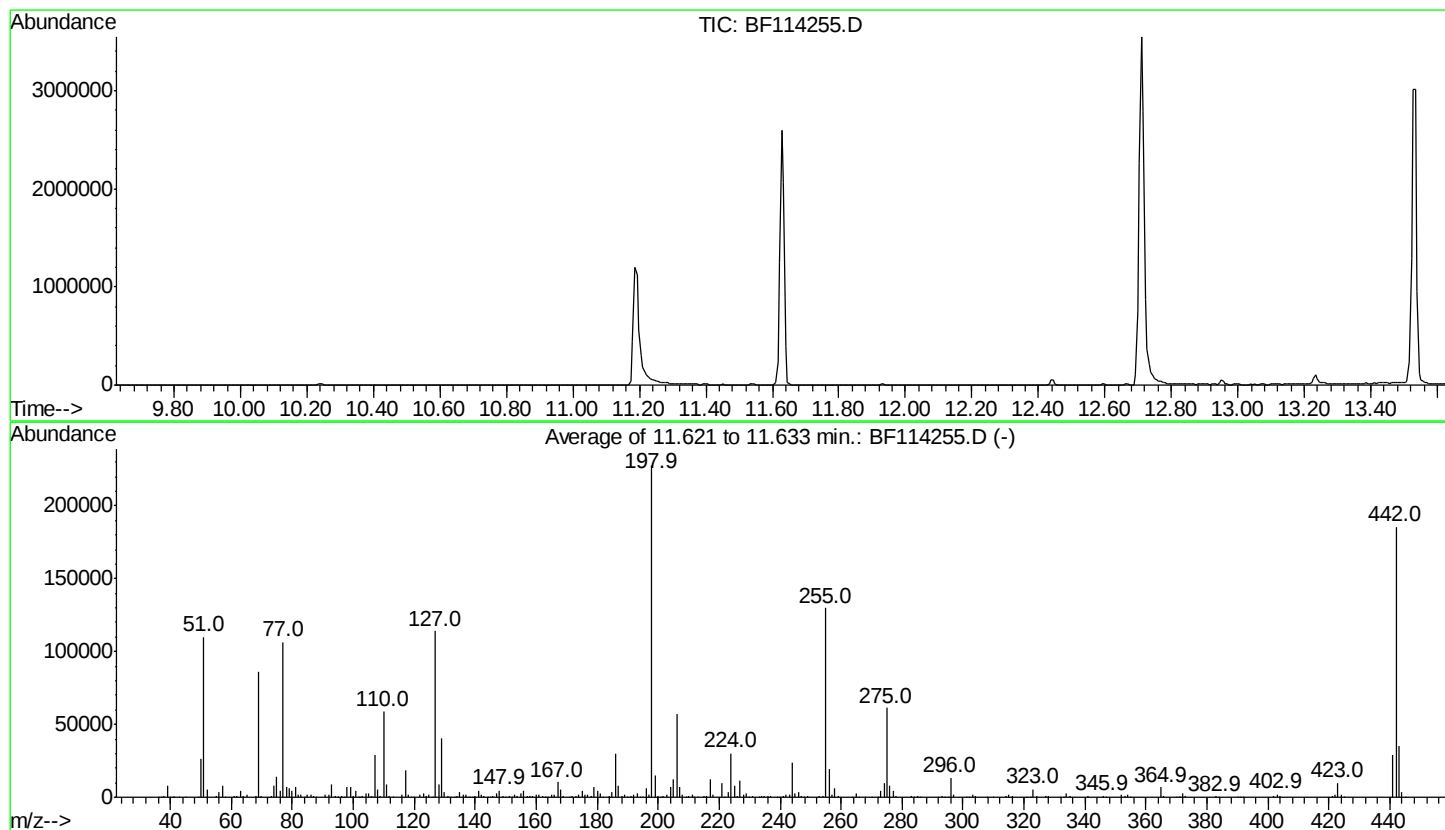

AutoFind: Scans 1621, 1622, 1623; Background Corrected with Scan 1616

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.3	109826	PASS
68	69	0.00	2	1.5	1327	PASS
69	198	0.00	100	37.9	86282	PASS
70	69	0.00	2	0.6	542	PASS
127	198	10	80	50.0	113802	PASS
197	198	0.00	2	0.7	1652	PASS
198	198	100	100	100.0	227584	PASS
199	198	5	9	6.6	14965	PASS
275	198	10	60	26.9	61301	PASS
365	198	1	100	2.9	6648	PASS
441	198	0.01	100	12.9	29248	PASS
442	198	50	100	81.6	185698	PASS
443	442	15	24	19.0	35302	PASS