


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF051519\
 Data File : BF114277.D
 Acq On : 15 May 2019 11:34
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 10 15:56:46 2019

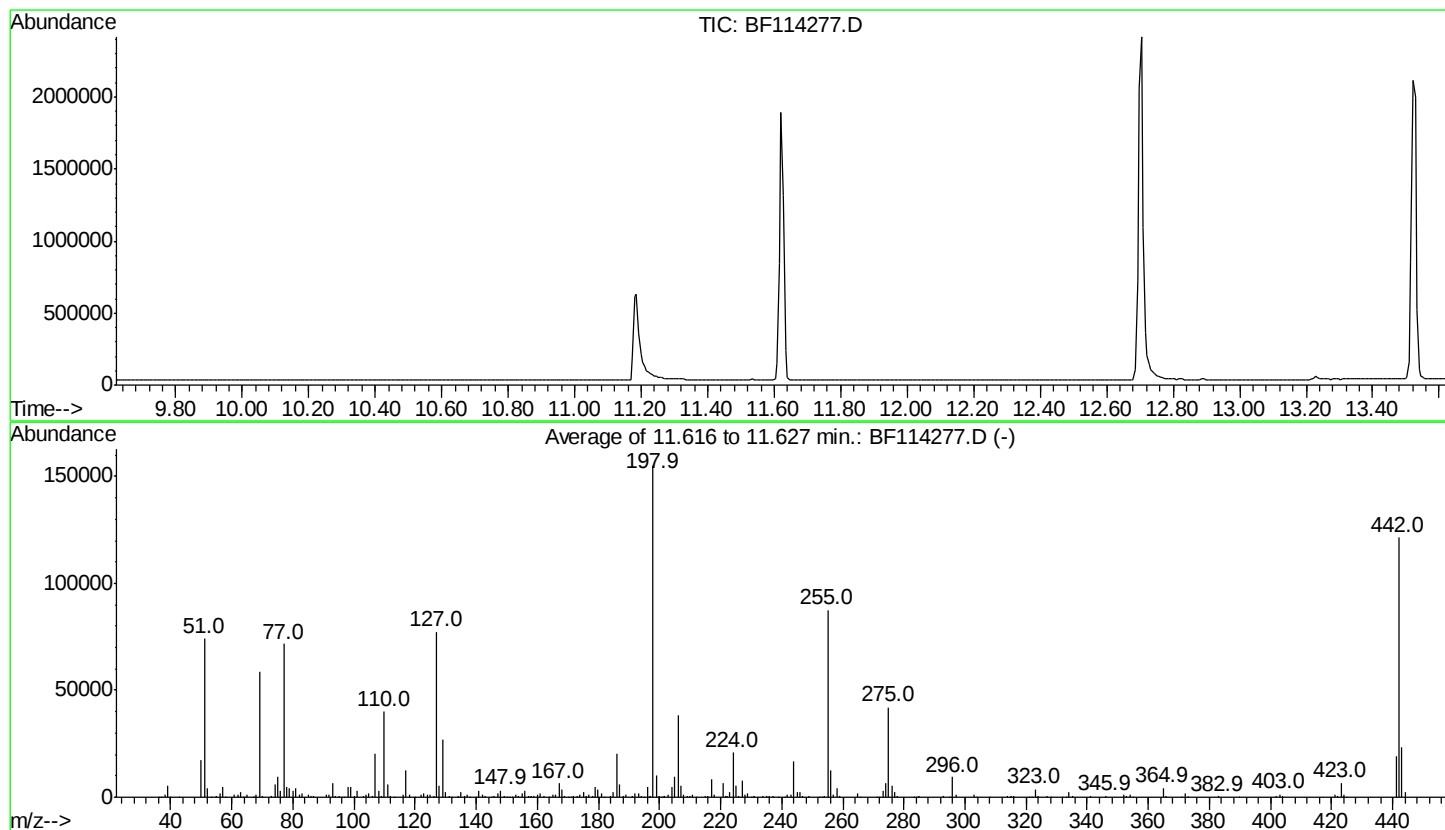

AutoFind: Scans 1620, 1621, 1622; Background Corrected with Scan 1615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.7	73982	PASS
68	69	0.00	2	1.8	1048	PASS
69	198	0.00	100	37.7	58389	PASS
70	69	0.00	2	0.8	452	PASS
127	198	10	80	50.0	77469	PASS
197	198	0.00	2	0.5	771	PASS
198	198	100	100	100.0	155045	PASS
199	198	5	9	6.7	10414	PASS
275	198	10	60	27.0	41909	PASS
365	198	1	100	2.7	4193	PASS
441	198	0.01	100	12.4	19216	PASS
442	198	50	100	78.3	121360	PASS
443	442	15	24	19.0	23108	PASS