
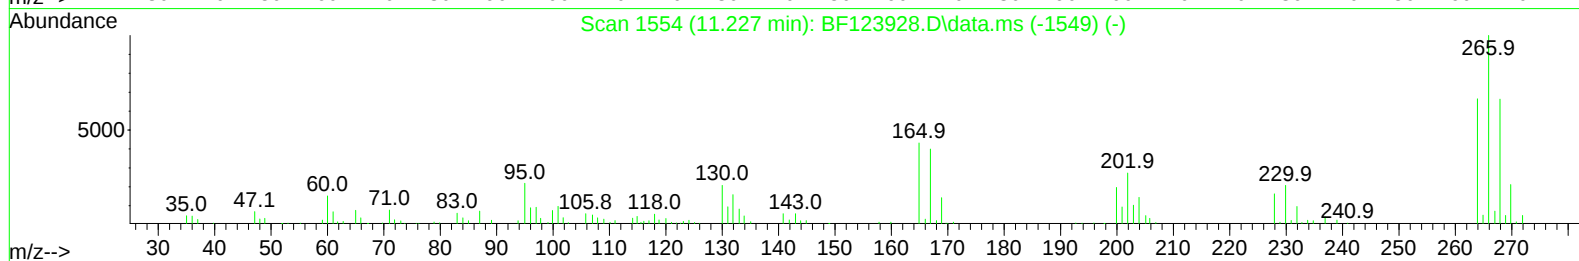
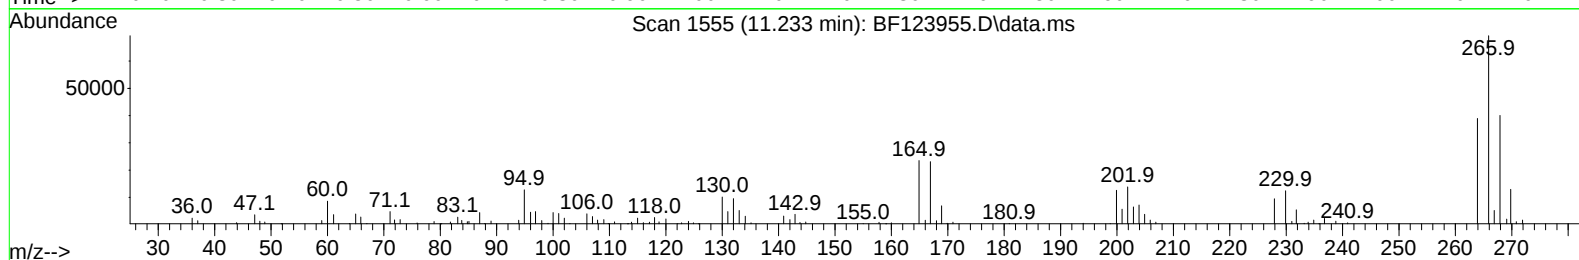


```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051721\  
Data File : BF123955.D  
Acq On    : 17 May 2021    9:06  
Operator  : JU/CG  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: May 17 13:53:22 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 14 19:05:57 2021
Response via : Initial Calibration

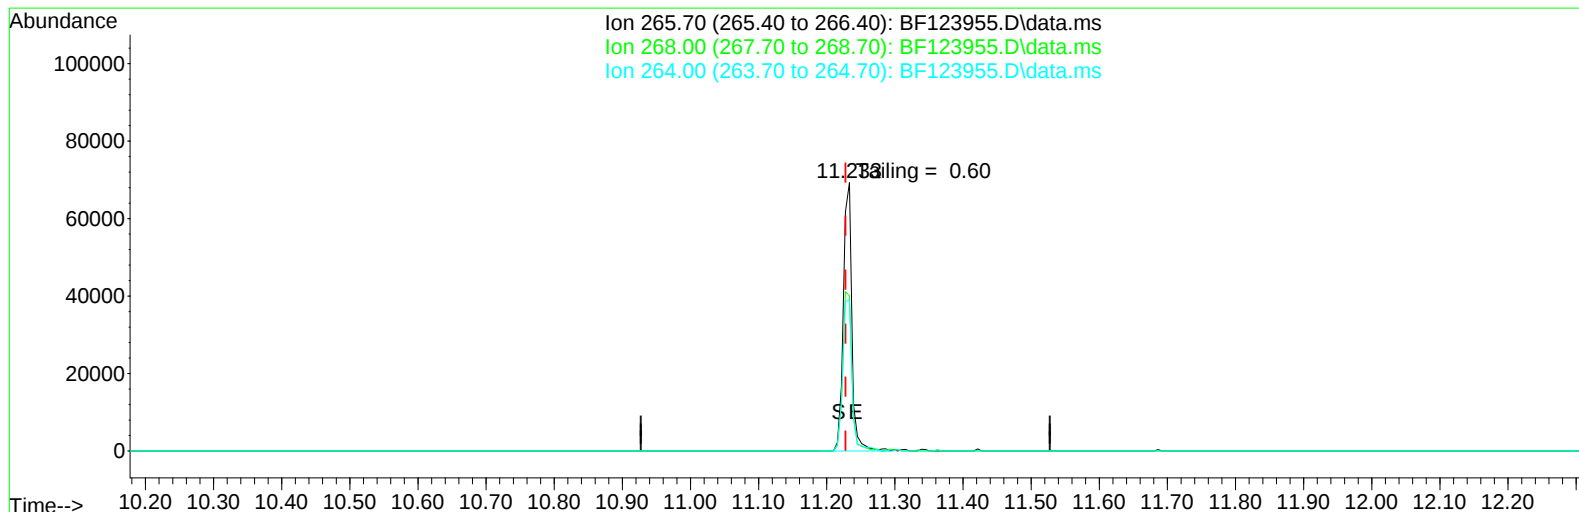

TIC: BF123955.D\data.ms

(70) Pentachlorophenol (C)




11.233min (+ 0.006) 14415.52 ng

response 60812

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	57.83
264.00	65.70	56.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051721\
Data File : BF123955.D
Acq On : 17 May 2021 9:06
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 17 13:53:22 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 14 19:05:57 2021
Response via : Initial Calibration

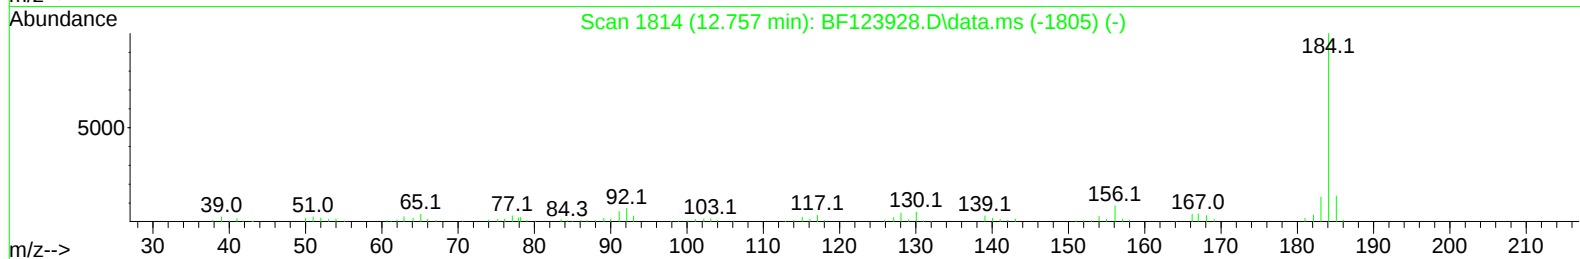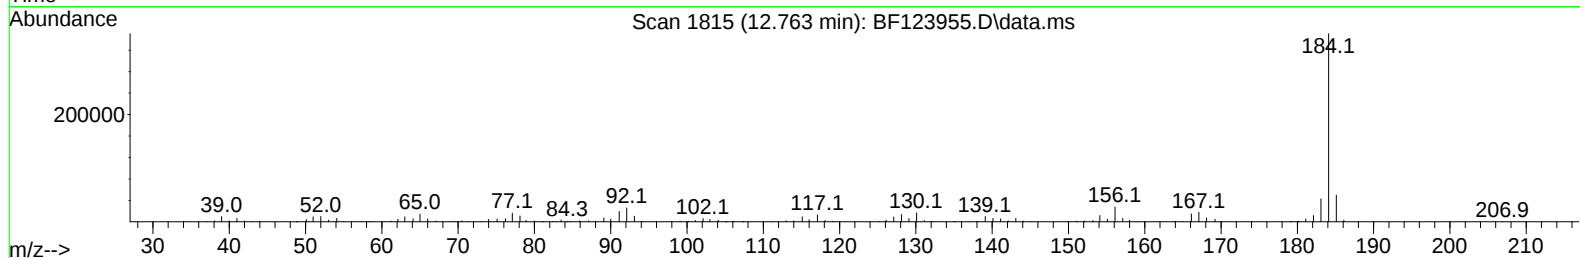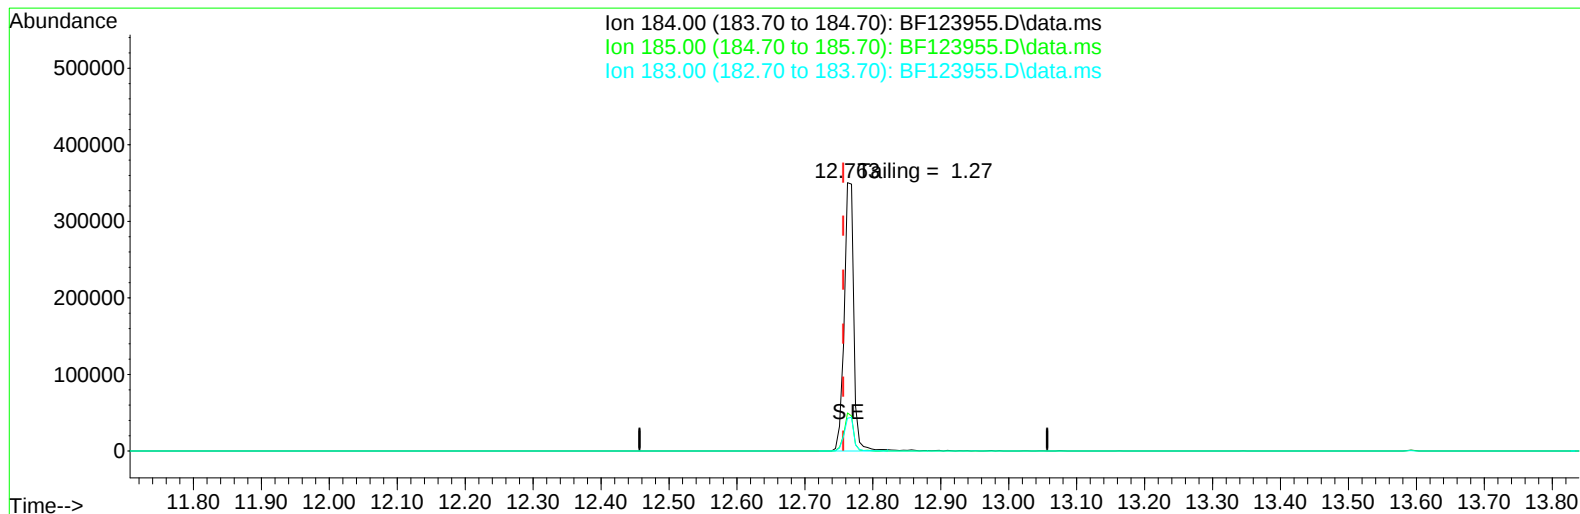

TIC: BF123955.D\data.ms

(77) Benzidine

12.763min (+ 0.006) 0.00 ng

response 341590

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.18
183.00	9.80	12.26#
0.00	0.00	0.00