
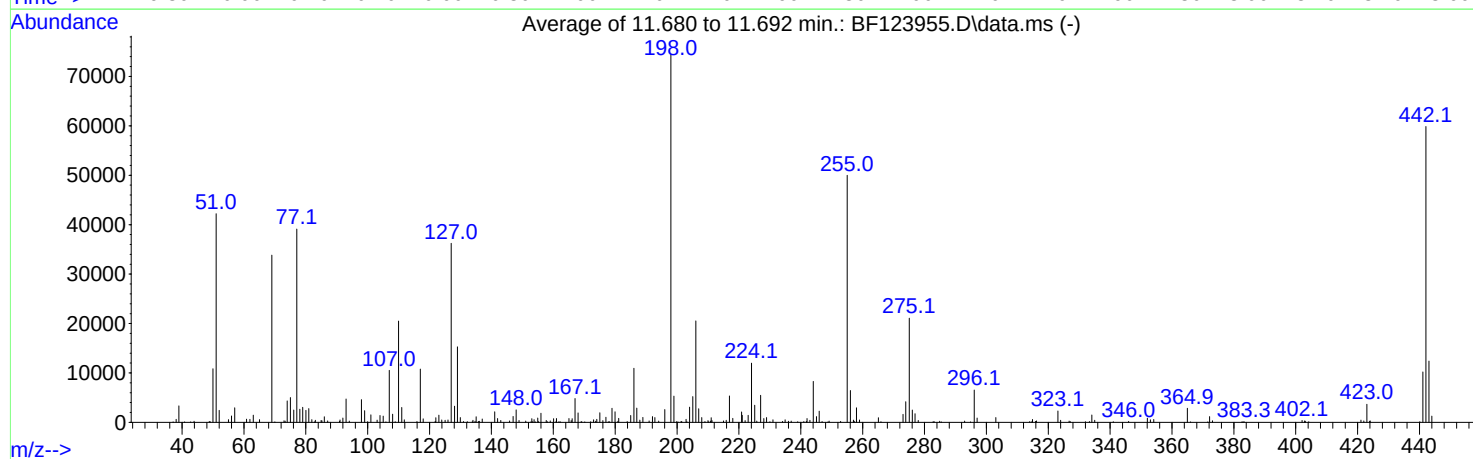


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051721\
 Data File : BF123955.D
 Acq On : 17 May 2021 9:06
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 14 19:05:57 2021

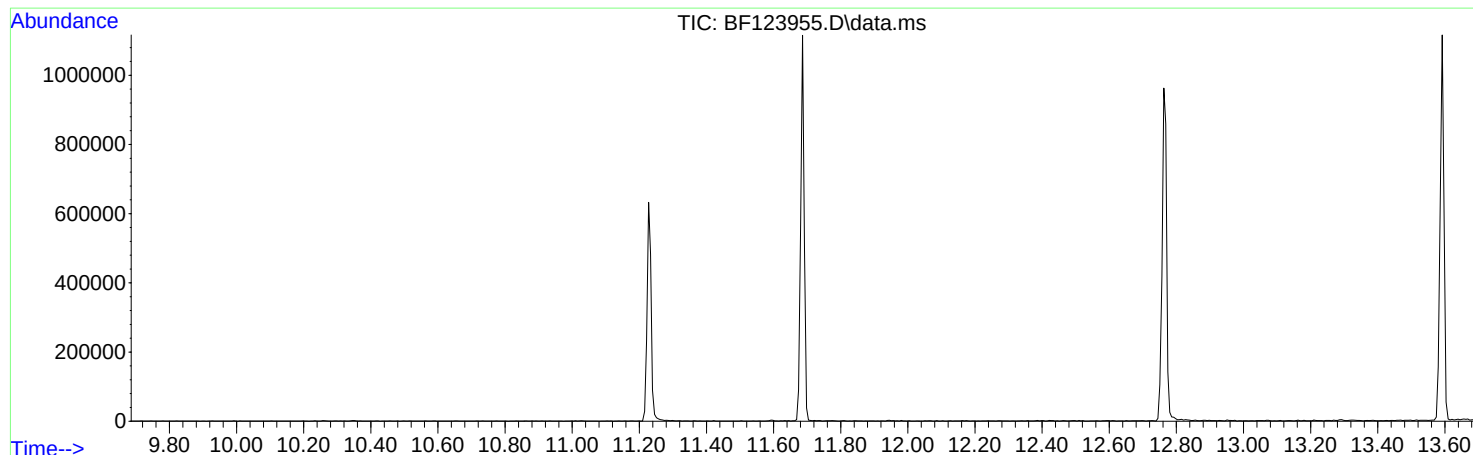




AutoFind: Scans 1631, 1632, 1633; Background Corrected with Scan 1627

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	56.7	42205	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	45.5	33842	PASS
70	69	0.00	2	0.3	114	PASS
127	198	10	80	48.7	36216	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	74435	PASS
199	198	5	9	7.1	5316	PASS
275	198	10	60	28.3	21095	PASS
365	198	1	100	3.8	2851	PASS
441	198	0.01	100	13.7	10196	PASS
442	442	50	100	100.0	59875	PASS
443	442	15	24	20.7	12402	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051721\
Data File : BF123955.D
Acq On : 17 May 2021 9:06
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 17 13:53:22 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 14 19:05:57 2021
Response via : Initial Calibration

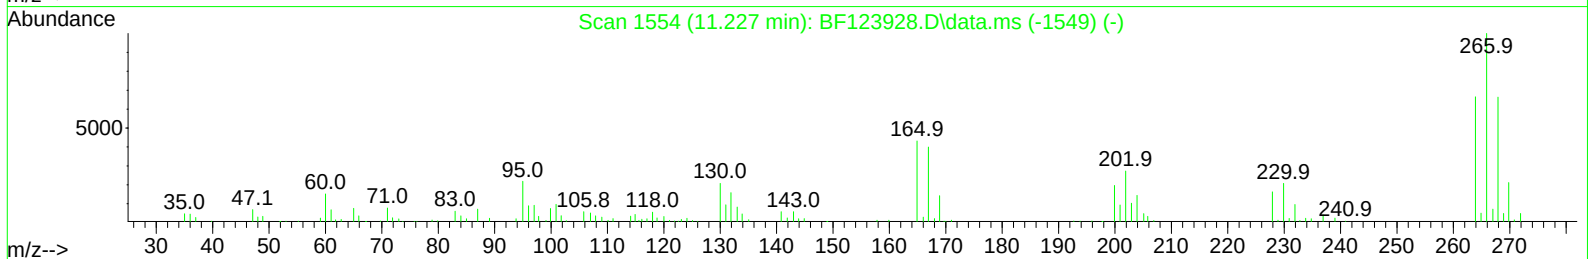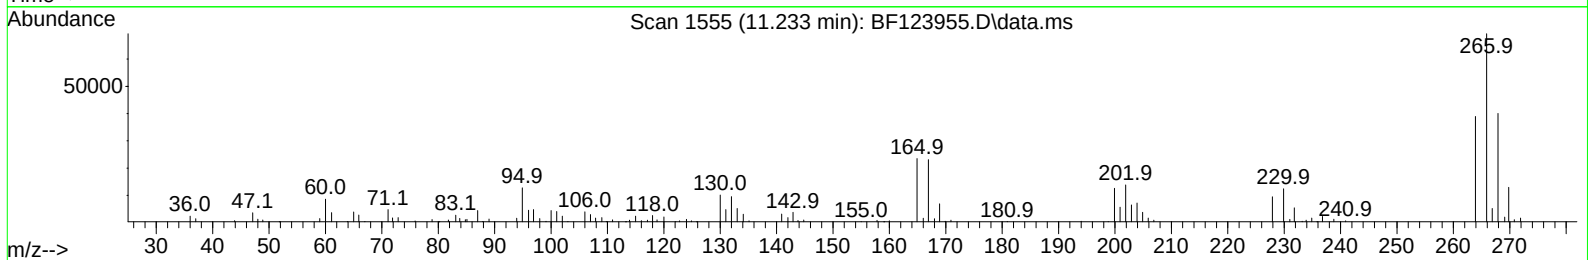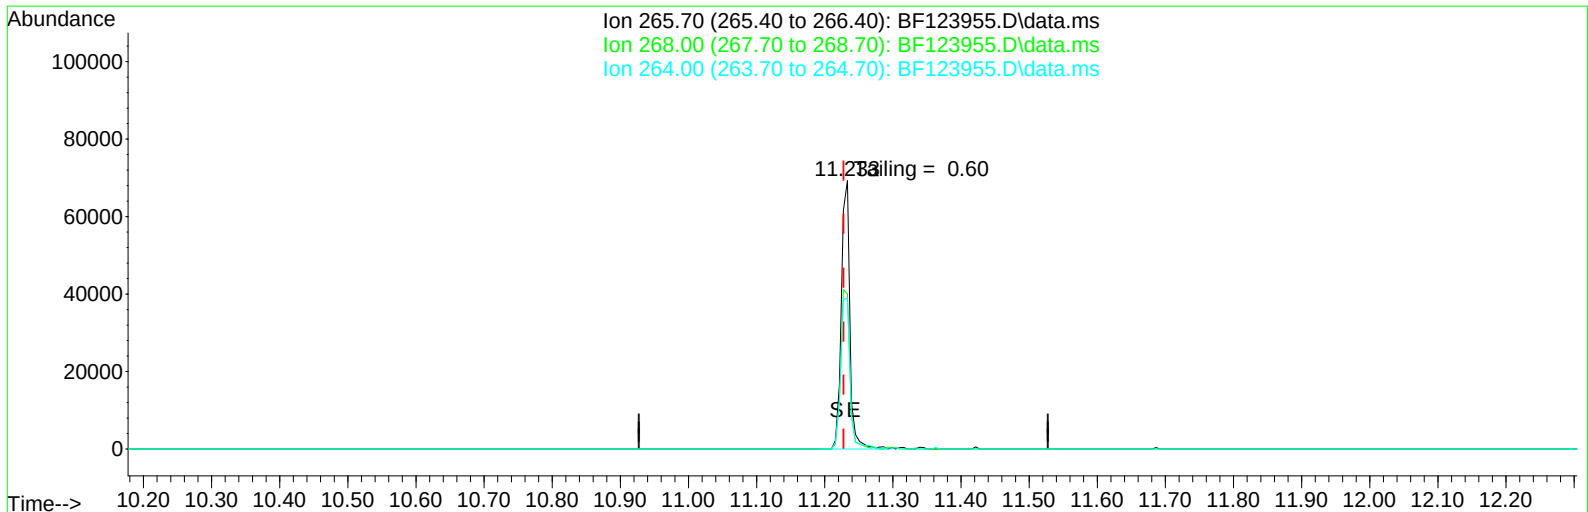

TIC: BF123955.D\data.ms

(70) Pentachlorophenol (C)

11.233min (+ 0.006) 14415.52 ng




response 60812

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	57.83
264.00	65.70	56.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051721\
 Data File : BF123955.D
 Acq On : 17 May 2021 9:06
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: May 17 13:53:22 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 14 19:05:57 2021
 Response via : Initial Calibration

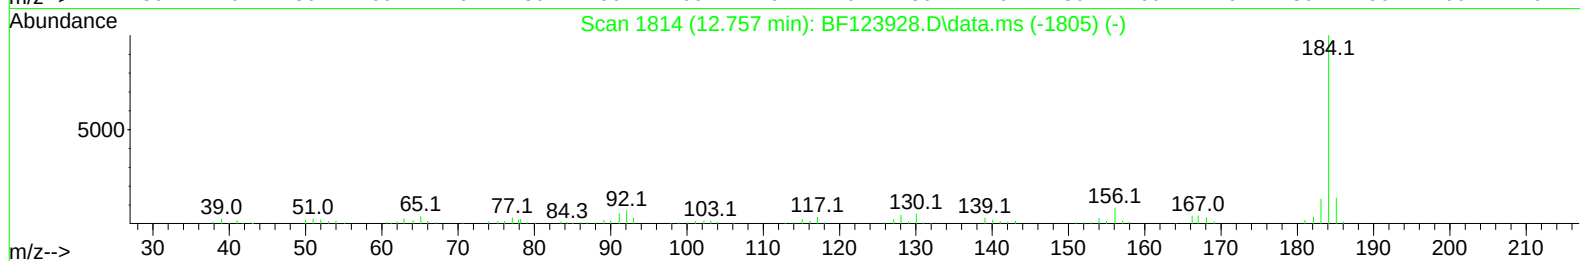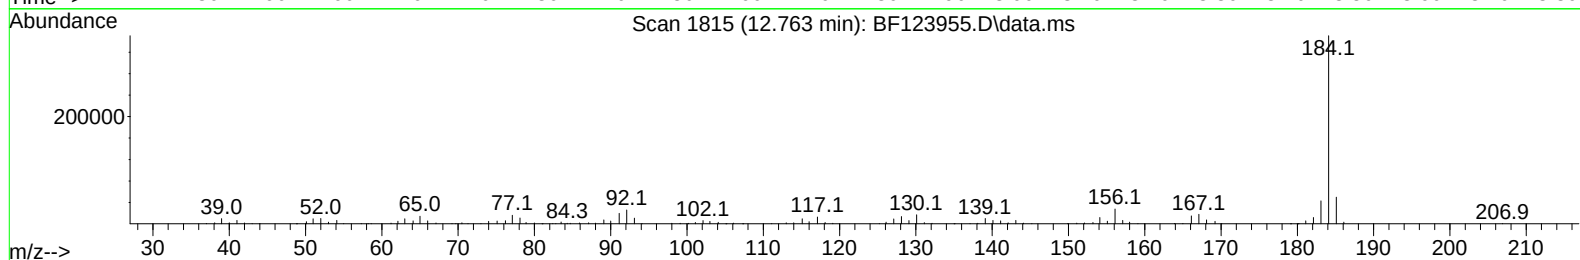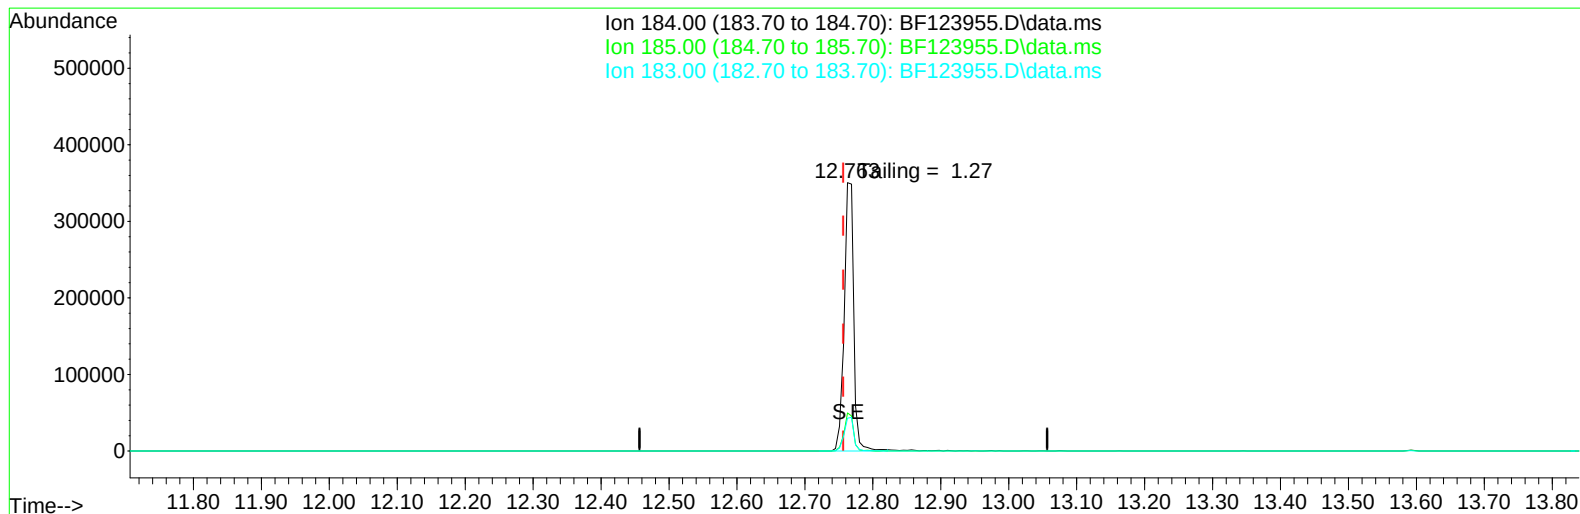

TIC: BF123955.D\data.ms

(77) Benzidine

12.763min (+ 0.006) 0.00 ng

response 341590

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.18
183.00	9.80	12.26#
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/17/2021	BNA_F	<u>BF123955.D</u>
Compound Name	Response	Retention Time
DDT	158820	13.59
DDD	1092	13.29
DDE	413	12.95
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1505	160325	0.94