
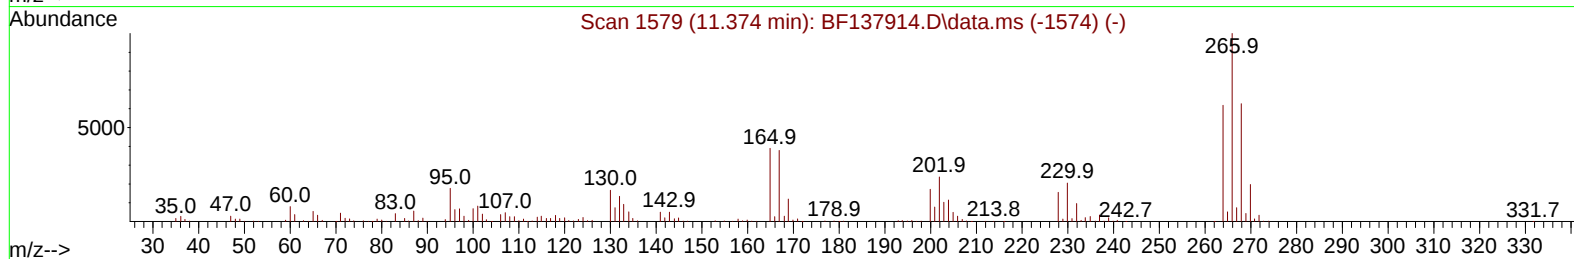
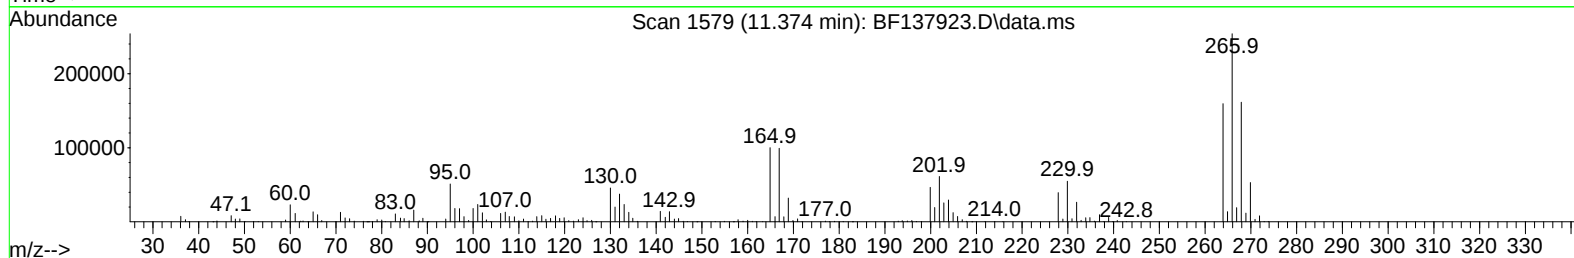


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051724\
Data File : BF137923.D
Acq On : 17 May 2024 10:53
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 17 12:08:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF051424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 15 04:12:16 2024
Response via : Initial Calibration

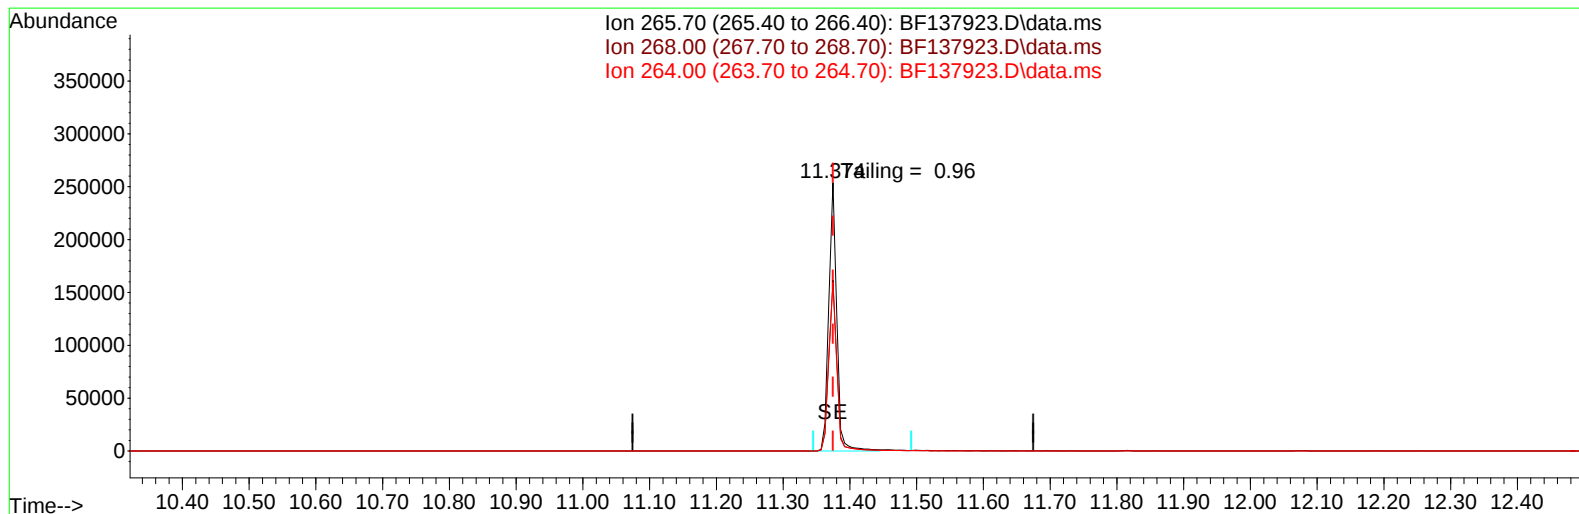

TIC: BF137923.D\data.ms

(70) Pentachlorophenol (C)




11.374min (+ 0.000) 203410.32 ng

response 215140

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	63.62
264.00	61.80	62.84
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051724\
Data File : BF137923.D
Acq On : 17 May 2024 10:53
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 17 12:08:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF051424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 15 04:12:16 2024
Response via : Initial Calibration

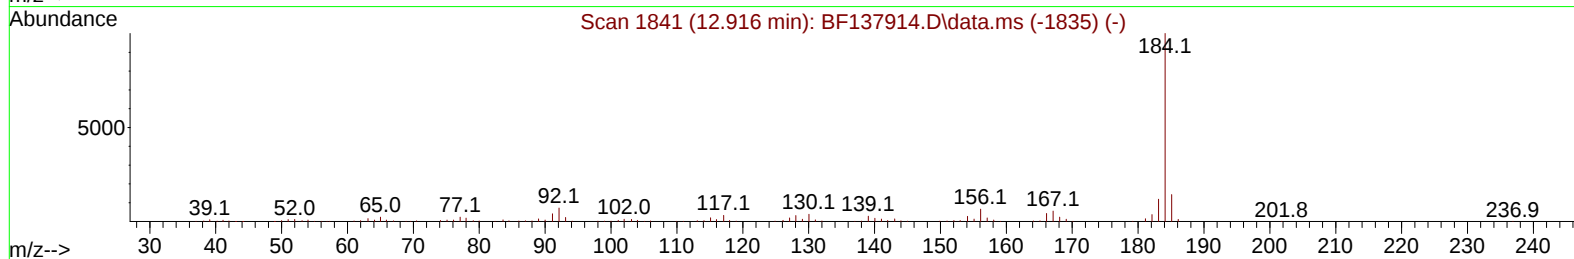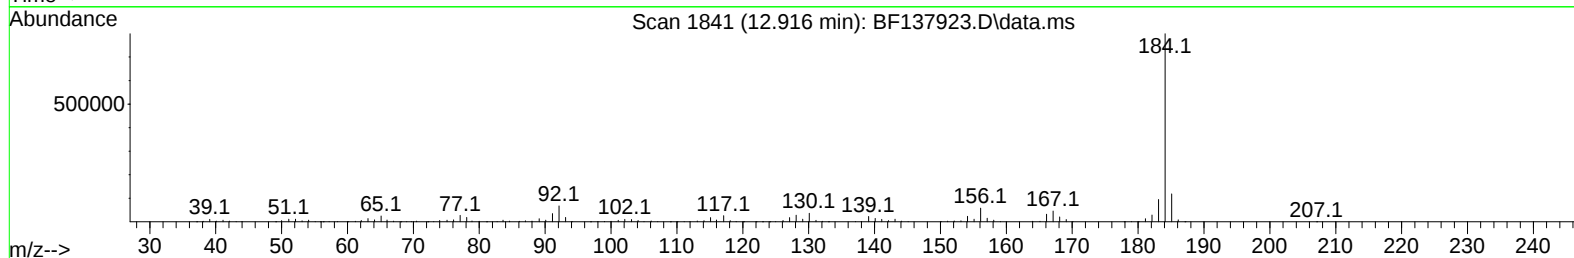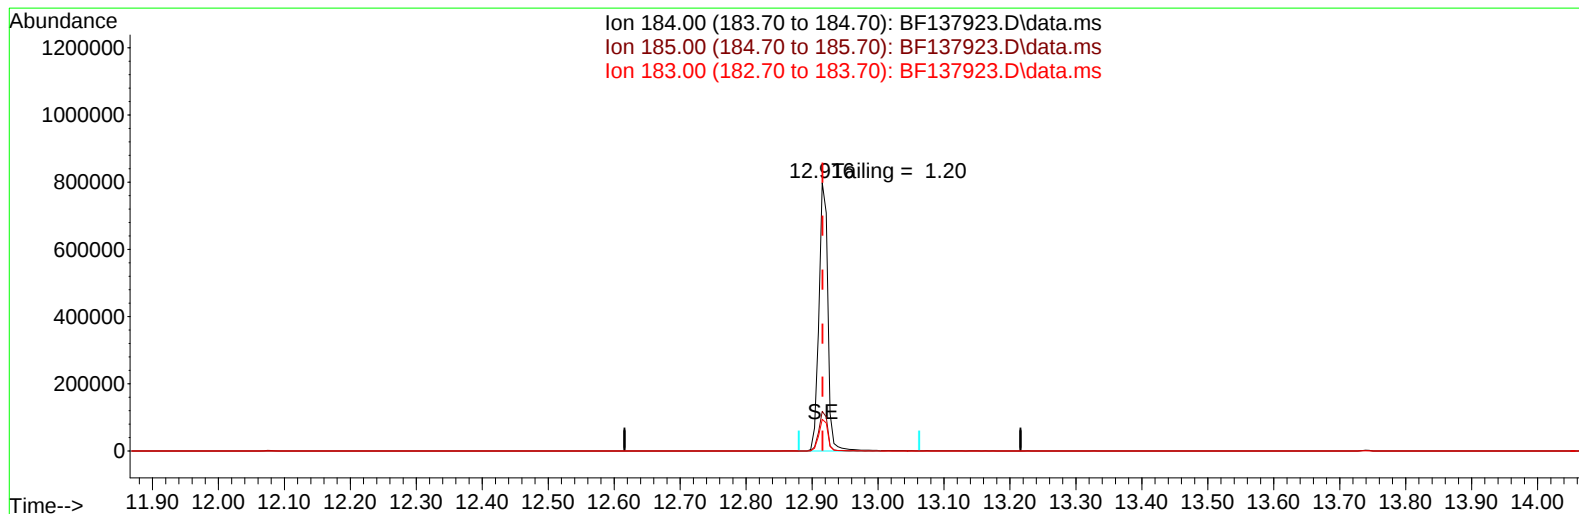

TIC: BF137923.D\data.ms

(77) Benzidine

12.916min (-0.000) 14920.66 ng

response 752882

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.81
183.00	11.90	11.81
0.00	0.00	0.00