


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051724\
Data File : BF137923.D
Acq On : 17 May 2024 10:53
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF051424.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed May 15 04:12:16 2024

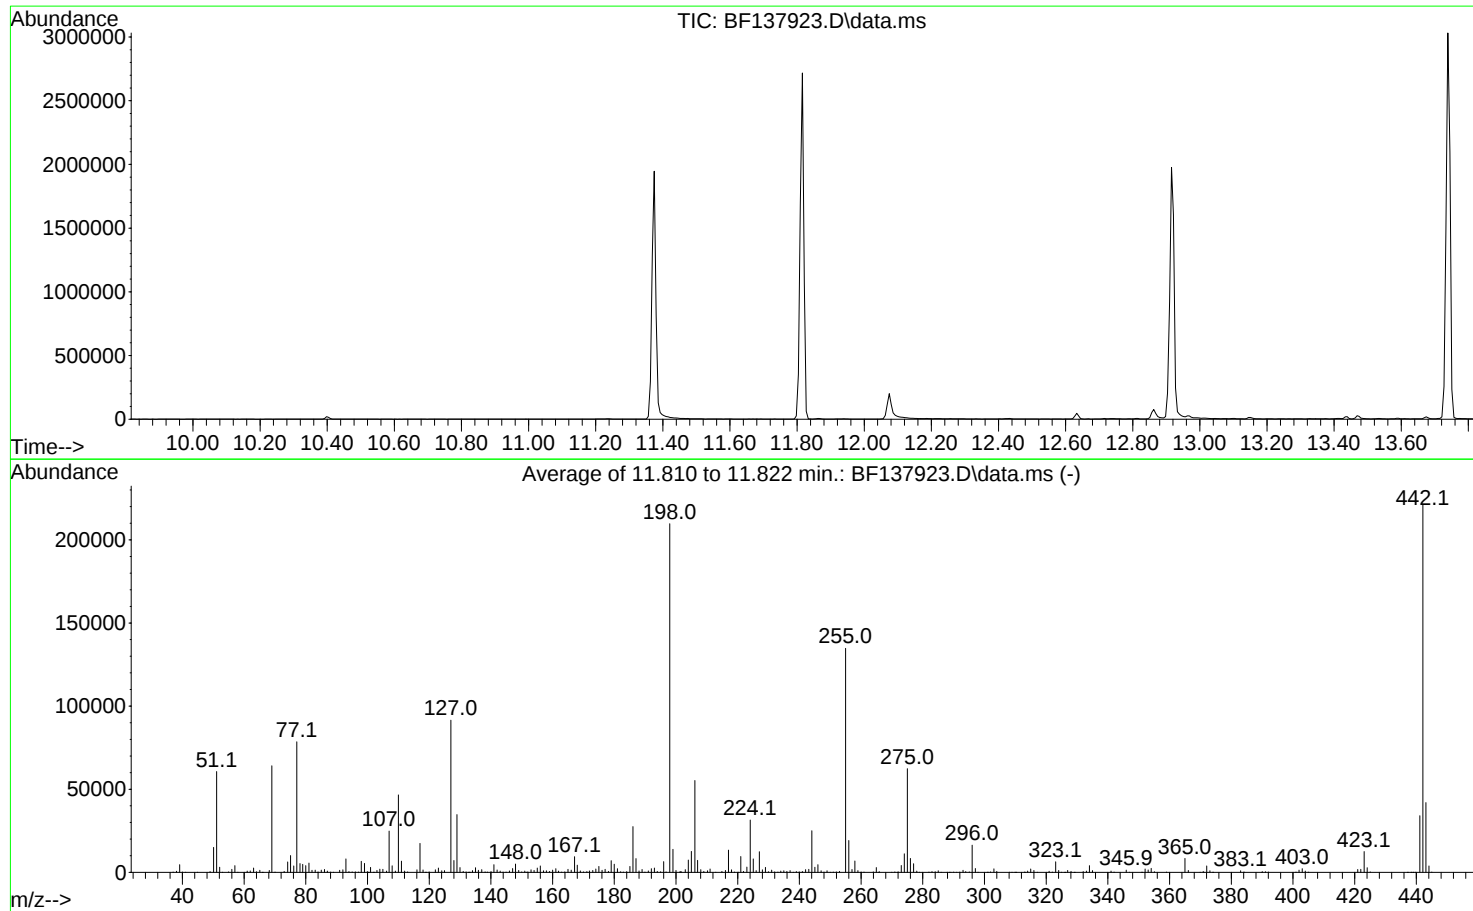

AutoFind: Scans 1653, 1654, 1655; Background Corrected with Scan 1647

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.9	60667	PASS
68	69	0.00	2	1.8	1182	PASS
69	198	0.00	100	30.6	64139	PASS
70	69	0.00	2	0.4	245	PASS
127	198	10	80	43.7	91560	PASS
197	198	0.00	2	0.1	301	PASS
198	198	100	100	100.0	209701	PASS
199	198	5	9	6.6	13870	PASS
275	198	10	60	29.7	62357	PASS
365	198	1	100	4.0	8373	PASS
441	198	0.01	100	16.3	34096	PASS
442	442	50	100	100.0	221277	PASS
443	442	15	24	18.9	41931	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/17/2024	BNA_F	<u>BF137923.D</u>
Compound Name	Response	Retention Time
DDT	521051	13.739
DDD	7993	13.474
DDE	529	13.098
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8522	529573	1.61

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051724\
Data File : BF137923.D
Acq On : 17 May 2024 10:53
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 17 12:08:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF051424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 15 04:12:16 2024
Response via : Initial Calibration

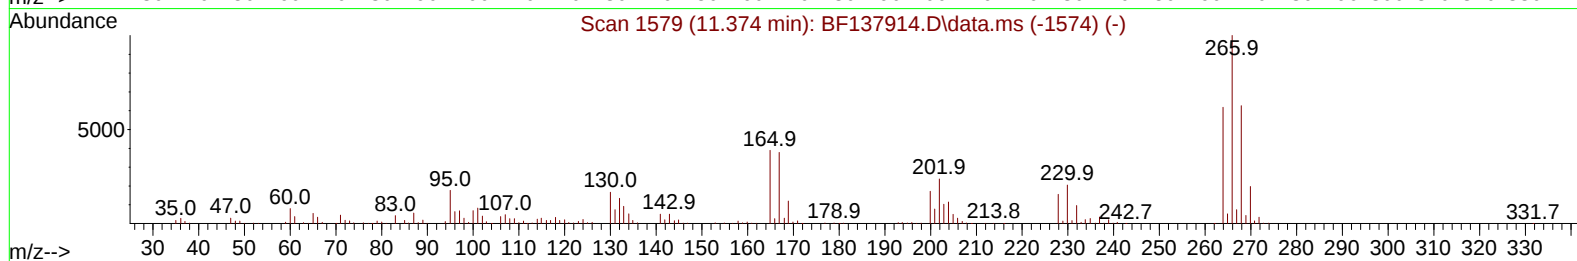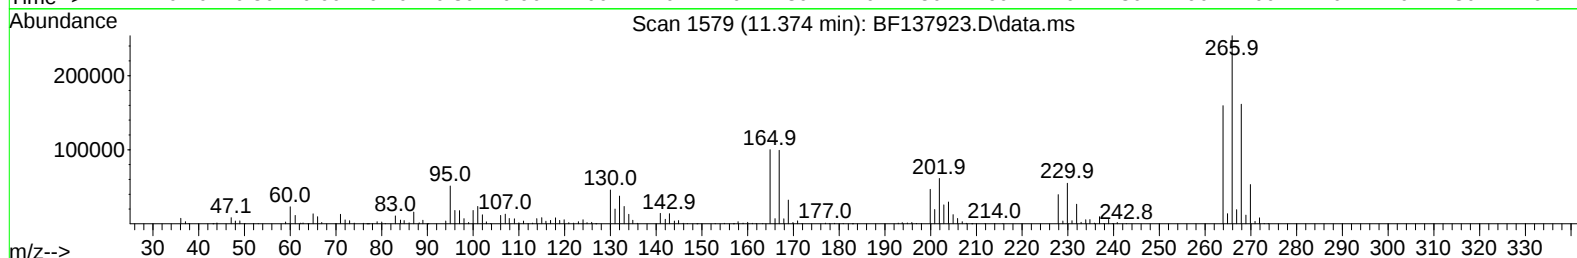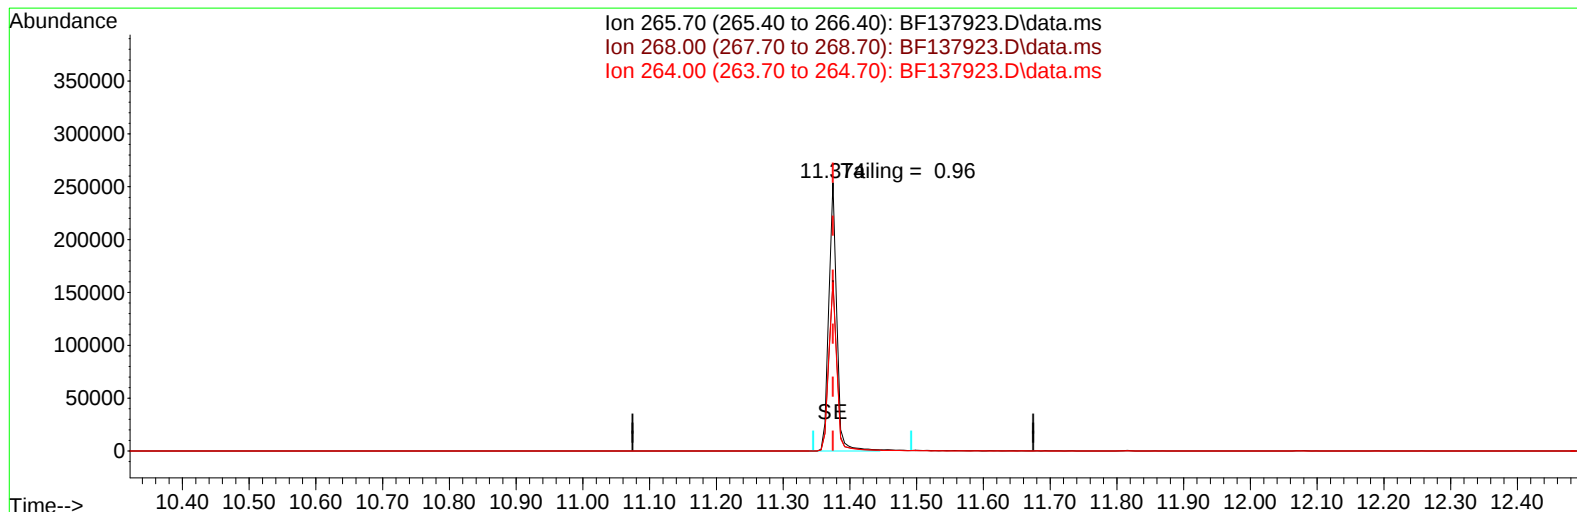

TIC: BF137923.D\data.ms

(70) Pentachlorophenol (C)

11.374min (+ 0.000) 203410.32 ng




response 215140

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	63.62
264.00	61.80	62.84
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051724\
Data File : BF137923.D
Acq On : 17 May 2024 10:53
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 17 12:08:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF051424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 15 04:12:16 2024
Response via : Initial Calibration

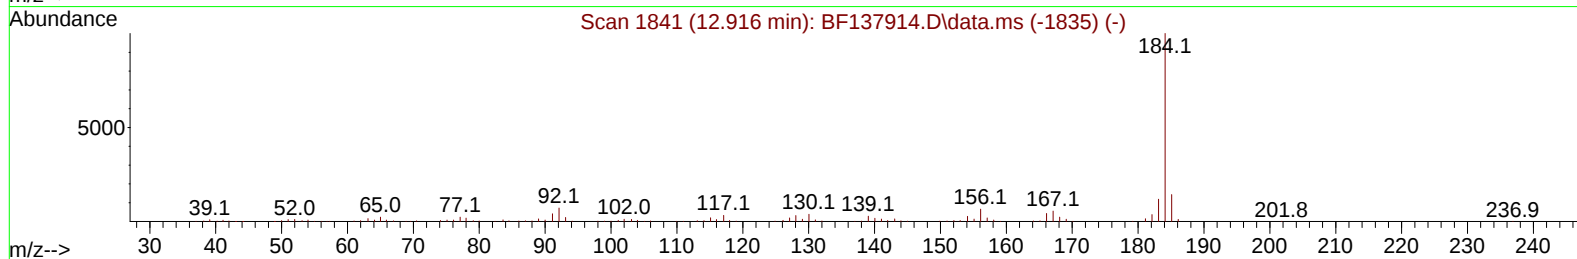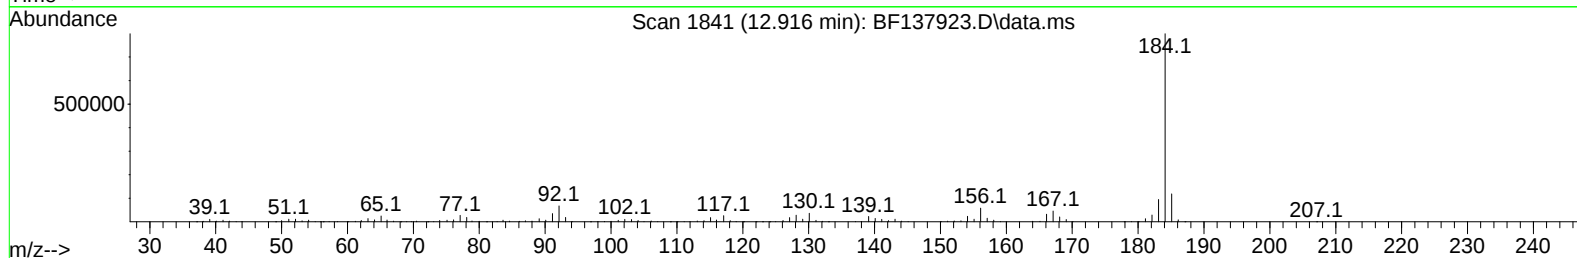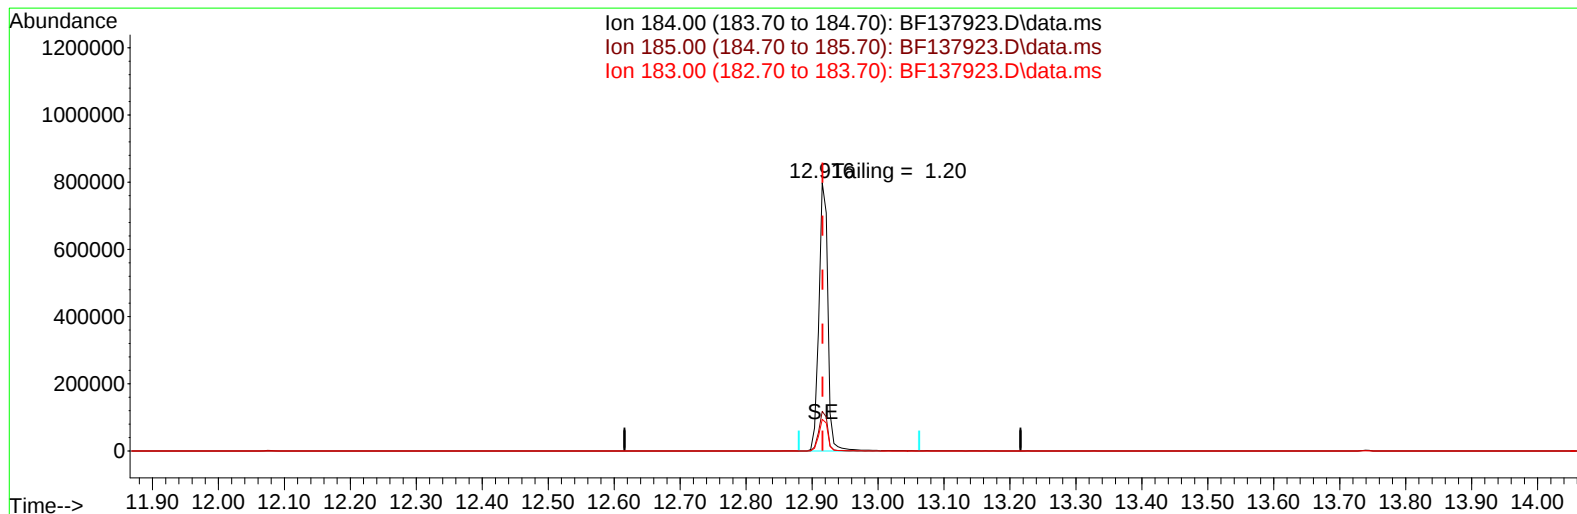

TIC: BF137923.D\data.ms

(77) Benzidine

12.916min (-0.000) 14920.66 ng

response 752882

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.81
183.00	11.90	11.81
0.00	0.00	0.00