

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051821\
 Data File : BF123976.D
 Acq On : 18 May 2021 13:40
 Operator : JU/CG
 Sample : PB136493BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB136493BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF123976.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.304	26	37	41	rBB	64713	88958	3.65%	0.608%
2	5.533	581	586	589	rBV	1948697	2025072	83.08%	13.840%
3	6.528	749	755	758	rBV	1748977	2002491	82.15%	13.686%
4	6.904	815	819	822	rBV	490167	380000	15.59%	2.597%
5	7.469	908	915	918	rBV	1218296	1350765	55.41%	9.232%
6	8.186	1032	1037	1041	rBV	557772	493798	20.26%	3.375%
7	9.269	1215	1221	1223	rBV	2469043	2388490	97.99%	16.324%
8	9.945	1328	1336	1339	rBV	681421	568102	23.31%	3.883%
9	10.733	1465	1470	1473	rBV	1824602	1535416	62.99%	10.494%
10	11.427	1584	1588	1592	rBV	622376	573460	23.53%	3.919%
11	13.021	1854	1859	1862	rBV	2789006	2437584	100.00%	16.659%
12	14.068	2033	2037	2041	rBV	468142	435206	17.85%	2.974%
13	15.562	2286	2291	2296	rBV	241318	310917	12.76%	2.125%
14	17.268	2574	2581	2583	rBV4	20744	41668	1.71%	0.285%




Sum of corrected areas: 14631927

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051821\
Data File : BF123976.D
Acq On : 18 May 2021 13:40
Operator : JU/CG
Sample : PB136493BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB136493BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

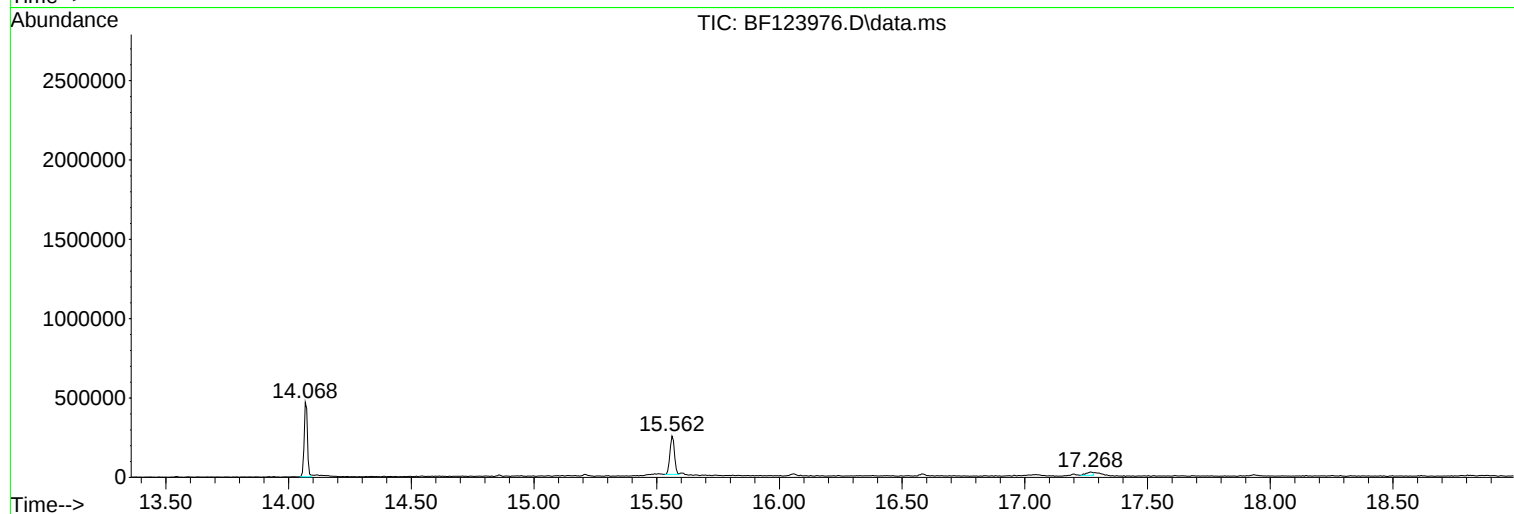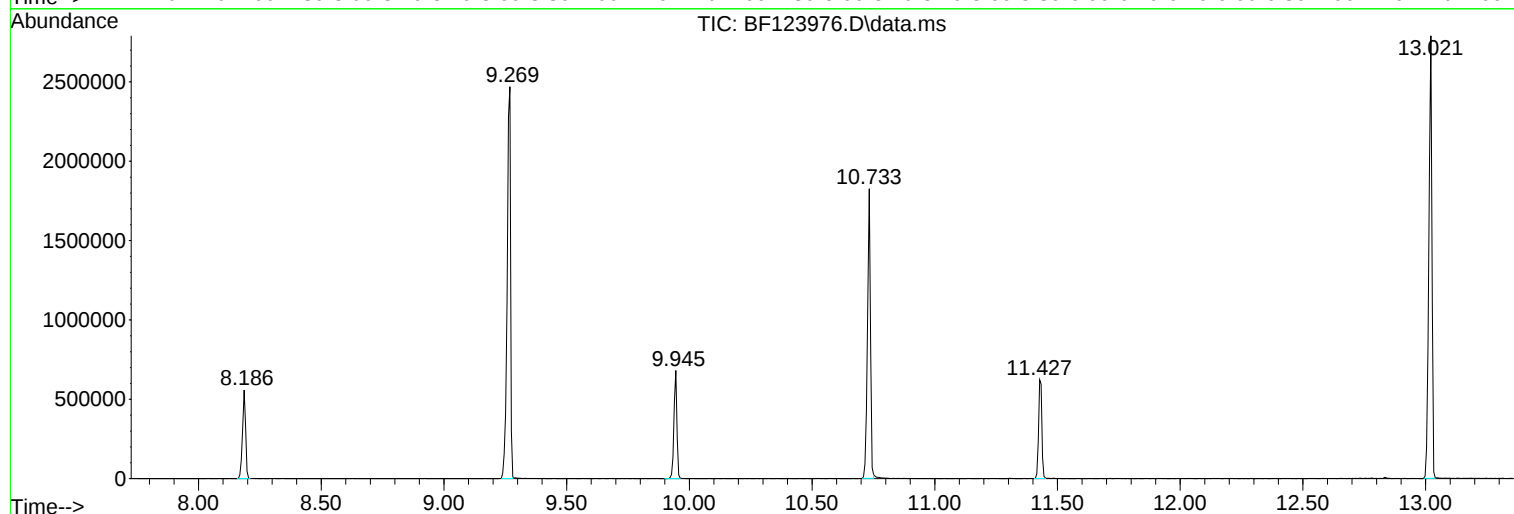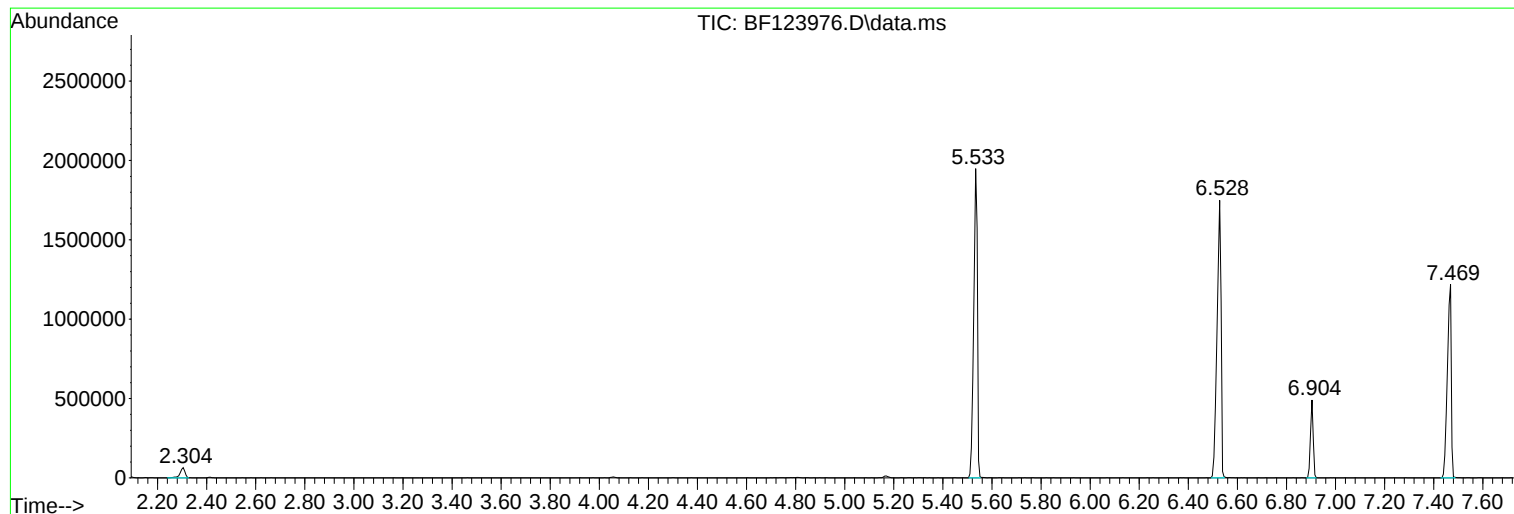

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051821\
Data File : BF123976.D
Acq On : 18 May 2021 13:40
Operator : JU/CG
Sample : PB136493BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB136493BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.304	4.68 ng	88958	1,4-Dichlorobenzene-d4	6.904

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	72
2			1,3-Dioxolane, 2-methyl-	88	C4H8O2	000497-26-7	47
3			(R)-3-Pyrrolidinol	87	C4H9NO	002799-21-5	9
4			1-Propanol, 2-methyl-	74	C4H10O	000078-83-1	9
5			Propane, 2-methoxy-2-methyl-	88	C5H12O	001634-04-4	9

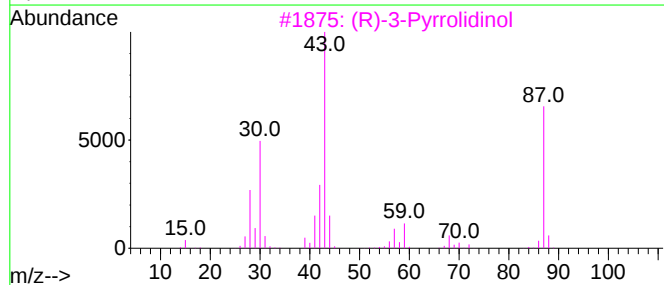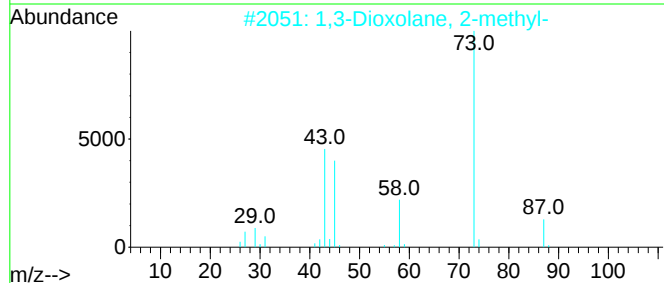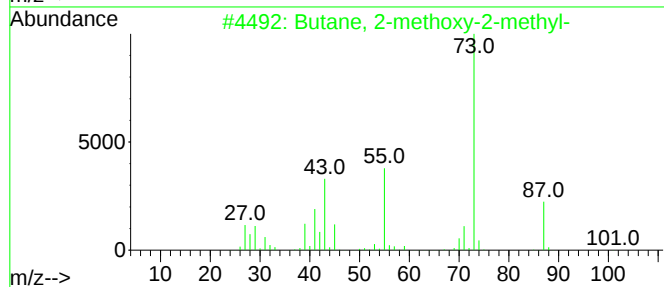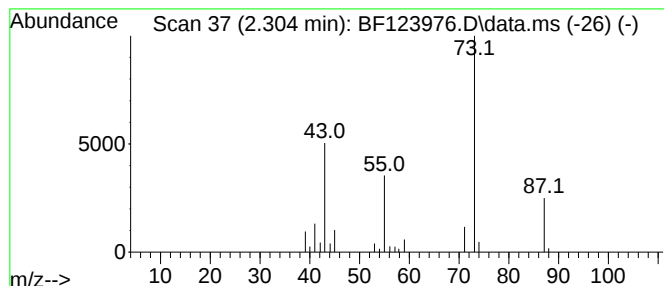

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051821\
Data File : BF123976.D
Acq On : 18 May 2021 13:40
Operator : JU/CG
Sample : PB136493BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB136493BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown17.26 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
17.268	2.68 ng	41668	Perylene-d12	15.562

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	1,10-Phenanthroline, 2,9-dimethy...	360	C26H20N2	004733-39-5	43		
2	Cholan-12-one, 3-hydroxy-, (3.alpha...	360	C24H40O2	054411-58-4	9		
3	Pentacyclo[18.4.1.1(2,7).1(8,13)...	360	C28H24	101077-60-5	5		
4	2-Cyclohexylamino-3-methyl(pheny...	360	C23H24N2O2	134614-17-8	5		
5	[.mu.-Fulvalene]bis(cyclopentadi...	360	C20H18V2	1000163-45-2	5		

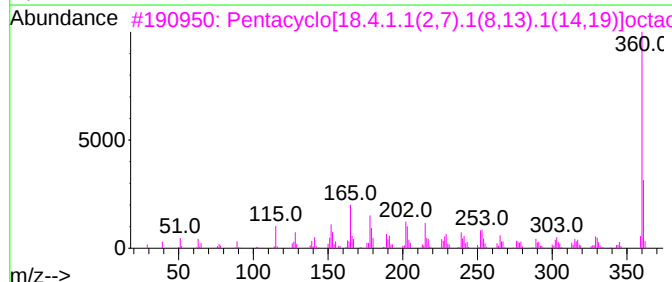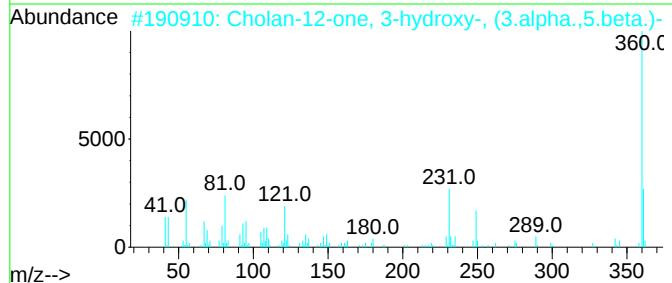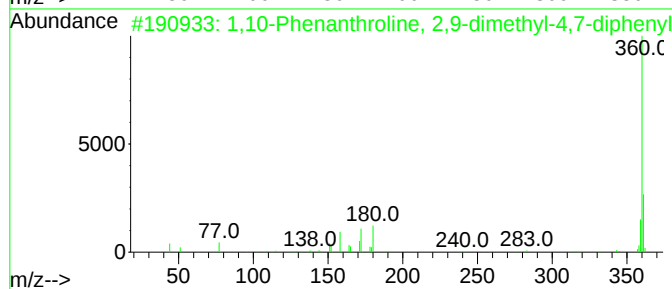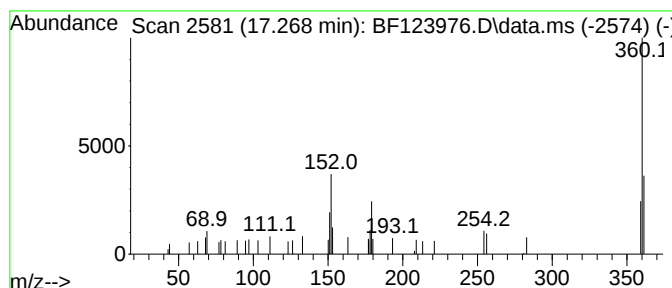

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051821\
Data File : BF123976.D
Acq On : 18 May 2021 13:40
Operator : JU/CG
Sample : PB136493BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB136493BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.304	4.7	ng	88958	1	6.904	380000	20.0
unknown17.26	17.268	2.7	ng	41668	6	15.562	310917	20.0