
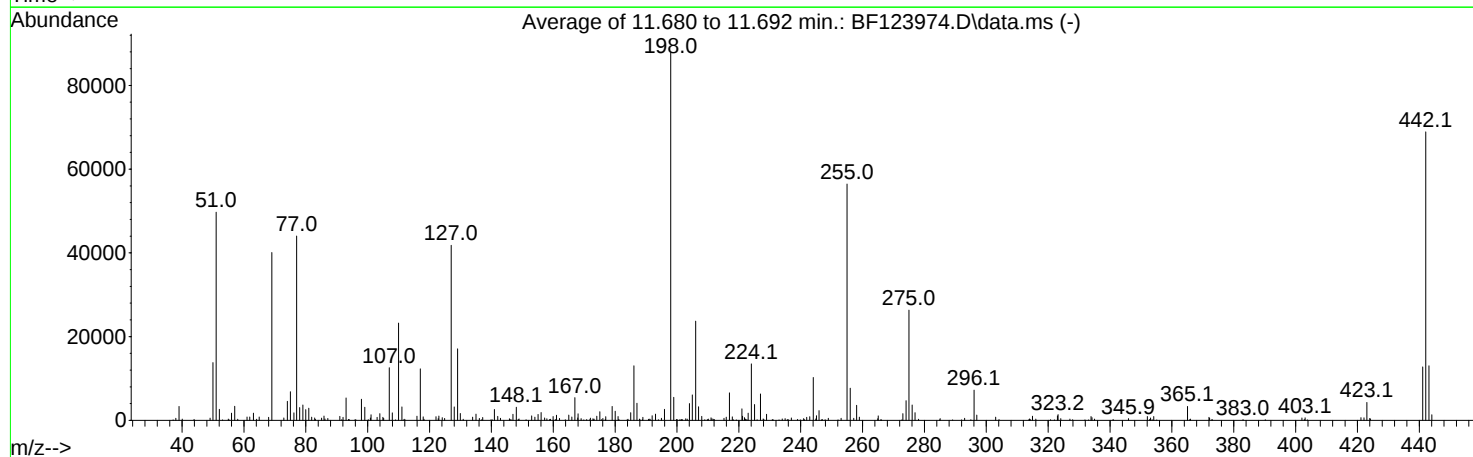


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051821\
 Data File : BF123974.D
 Acq On : 18 May 2021 12:06
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 14 19:05:57 2021

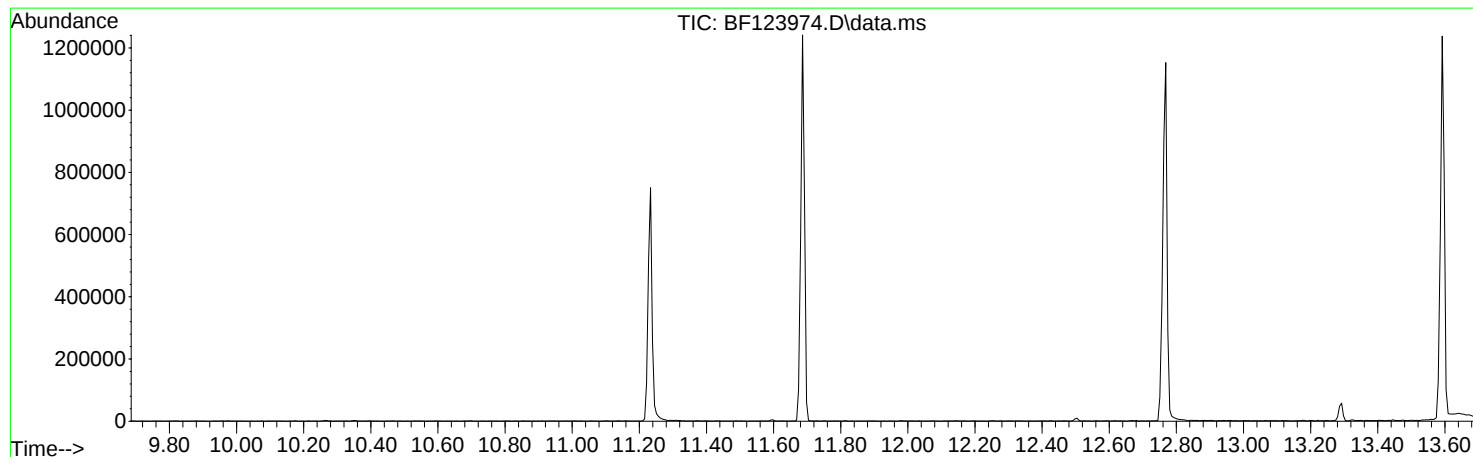

AutoFind: Scans 1631, 1632, 1633; Background Corrected with Scan 1626

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	56.6	49733	PASS
68	69	0.00	2	1.8	715	PASS
69	198	0.00	100	45.6	40085	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.6	41824	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	87869	PASS
199	198	5	9	6.3	5508	PASS
275	198	10	60	30.0	26354	PASS
365	198	1	100	3.8	3334	PASS
441	198	0.01	100	14.5	12763	PASS
442	442	50	100	100.0	68901	PASS
443	442	15	24	18.9	13025	PASS




DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/18/2021	BNA_F	<u>BF123974.D</u>
Compound Name	Response	Retention Time
DDT	178535	13.59
DDD	9593	13.29
DDE	474	12.95
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10067	188602	5.34

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051821\
Data File : BF123974.D
Acq On : 18 May 2021 12:06
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 18 15:03:36 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 14 19:05:57 2021
Response via : Initial Calibration

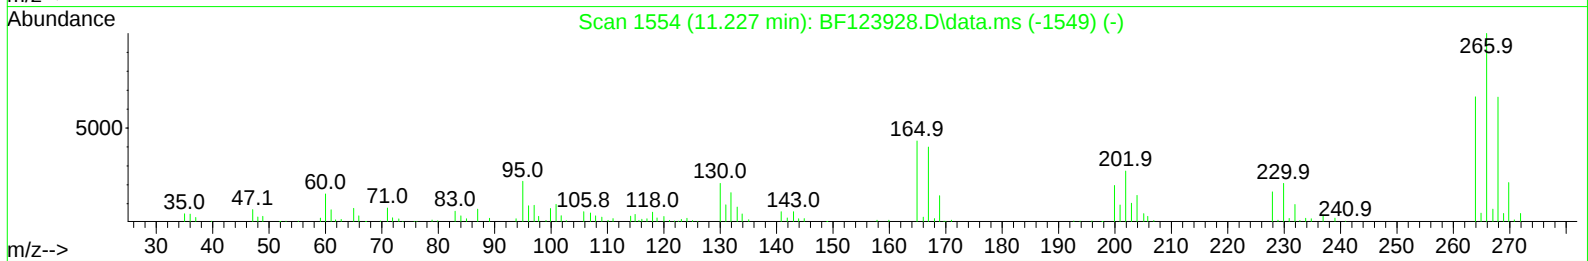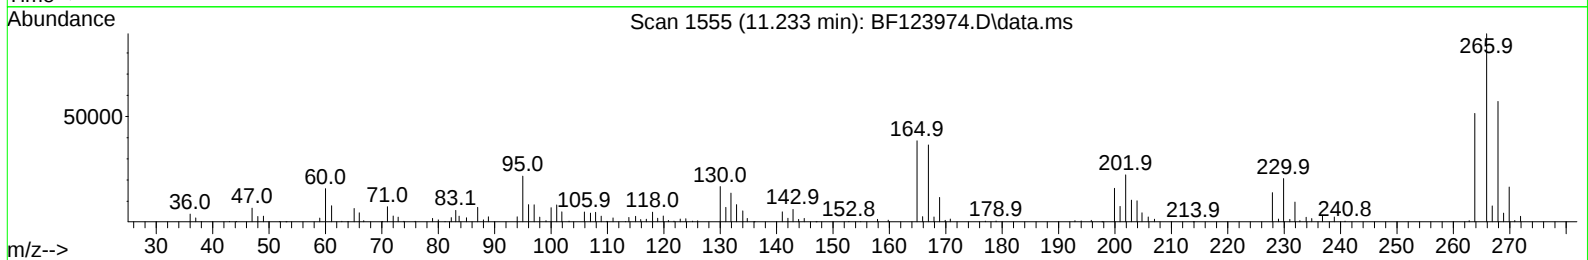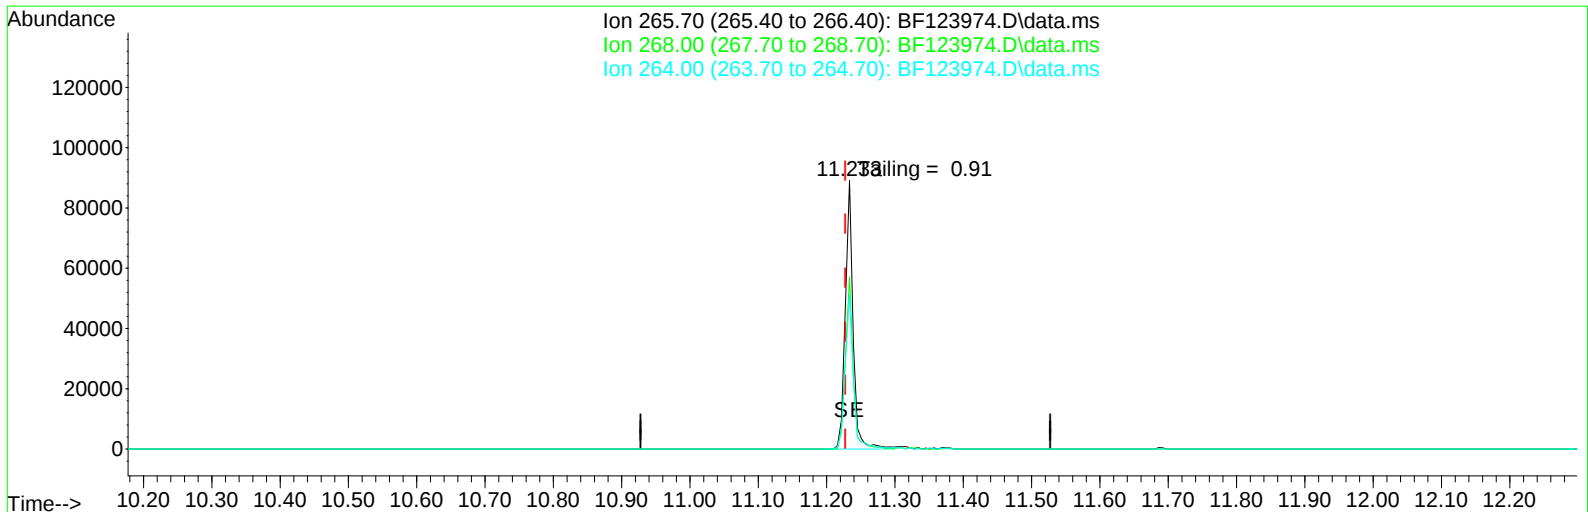

TIC: BF123974.D\data.ms

(70) Pentachlorophenol (C)

11.233min (+ 0.006) 18586.14 ng




response 71131

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	64.11
264.00	65.70	57.79
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051821\
Data File : BF123974.D
Acq On : 18 May 2021 12:06
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 18 15:03:36 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 14 19:05:57 2021
Response via : Initial Calibration

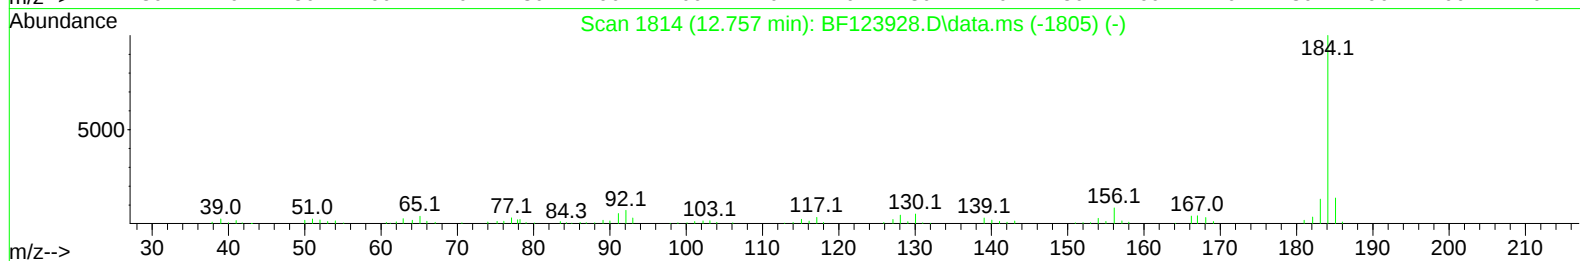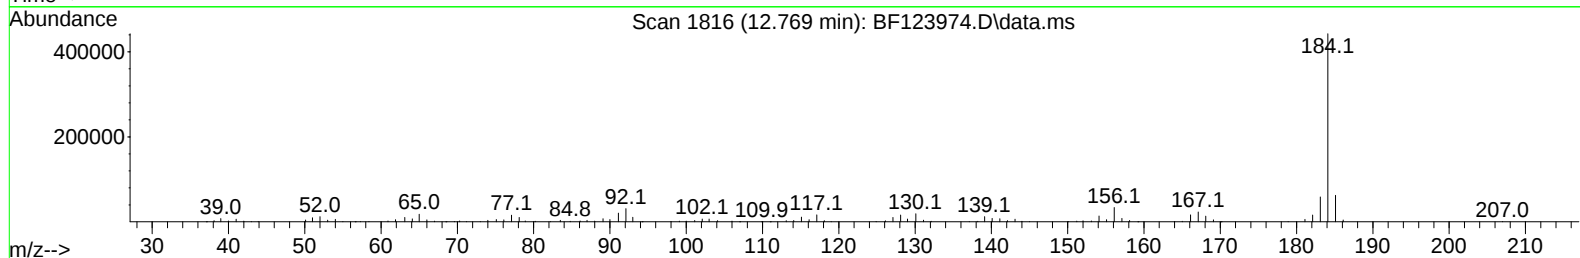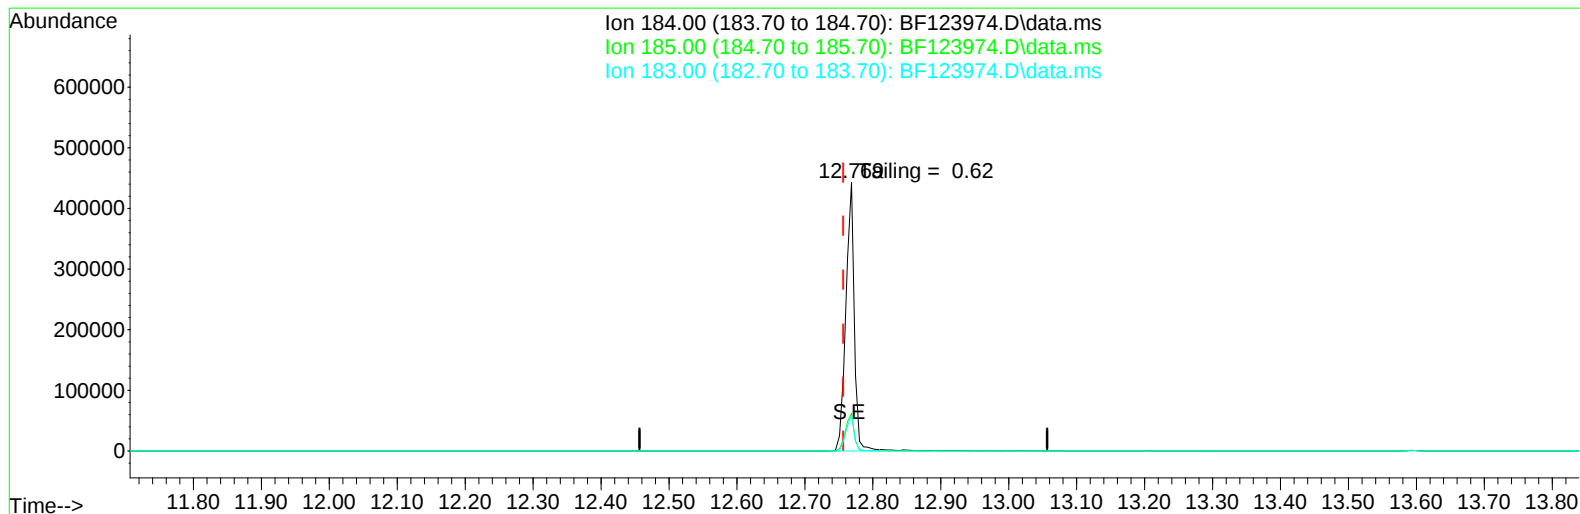

TIC: BF123974.D\data.ms

(77) Benzidine

12.769min (+ 0.012) 0.00 ng

response 382528

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.10
183.00	9.80	13.23#
0.00	0.00	0.00