

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF052019\
 Data File : BF114446.D
 Acq On : 21 May 2019 3:09
 Operator : JU/SJ
 Sample : K2943-09
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: May 21 11:14:24 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF051019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon May 20 04:47:40 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.83	152	215001	20.00	ng	-0.01
21) Naphthalene-d8	8.11	136	818365	20.00	ng	-0.01
39) Acenaphthene-d10	9.86	164	383127	20.00	ng	-0.01
64) Phenanthrene-d10	11.35	188	785943	20.00	ng	0.00
76) Chrysene-d12	13.99	240	524737	20.00	ng	-0.01
87) Perylene-d12	15.46	264	500611	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.46	112	1554001	116.32	ng	0.00
7) Phenol-d6	6.47	99	2017143	127.65	ng	-0.01
23) Nitrobenzene-d5	7.39	82	1257927	86.26	ng	-0.01
42) 2,4,6-Tribromophenol	10.66	330	492838	124.43	ng	0.00
45) 2-Fluorobiphenyl	9.19	172	2043752	80.69	ng	0.00
79) Terphenyl-d14	12.93	244	2126532	83.54	ng	0.00
Target Compounds						
19) n-Nitroso-di-n-propylamine	7.39	70	167324	16.706	ng	# 76
25) Isophorone	7.39	82	1257921	46.513	ng	# 64
50) Dimethylphthalate	9.58	163	312012	11.094	ng	99
57) 2,4-Dinitrotoluene	9.86	165	49707	5.871	ng	# 25
67) 4-Bromophenyl-phenylether	10.66	248	32333	3.736	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF052019\
Data File : BF114446.D
Acq On : 21 May 2019 3:09
Operator : JU/SJ
Sample : K2943-09
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: May 21 11:14:24 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF051019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 20 04:47:40 2019
Response via : Initial Calibration

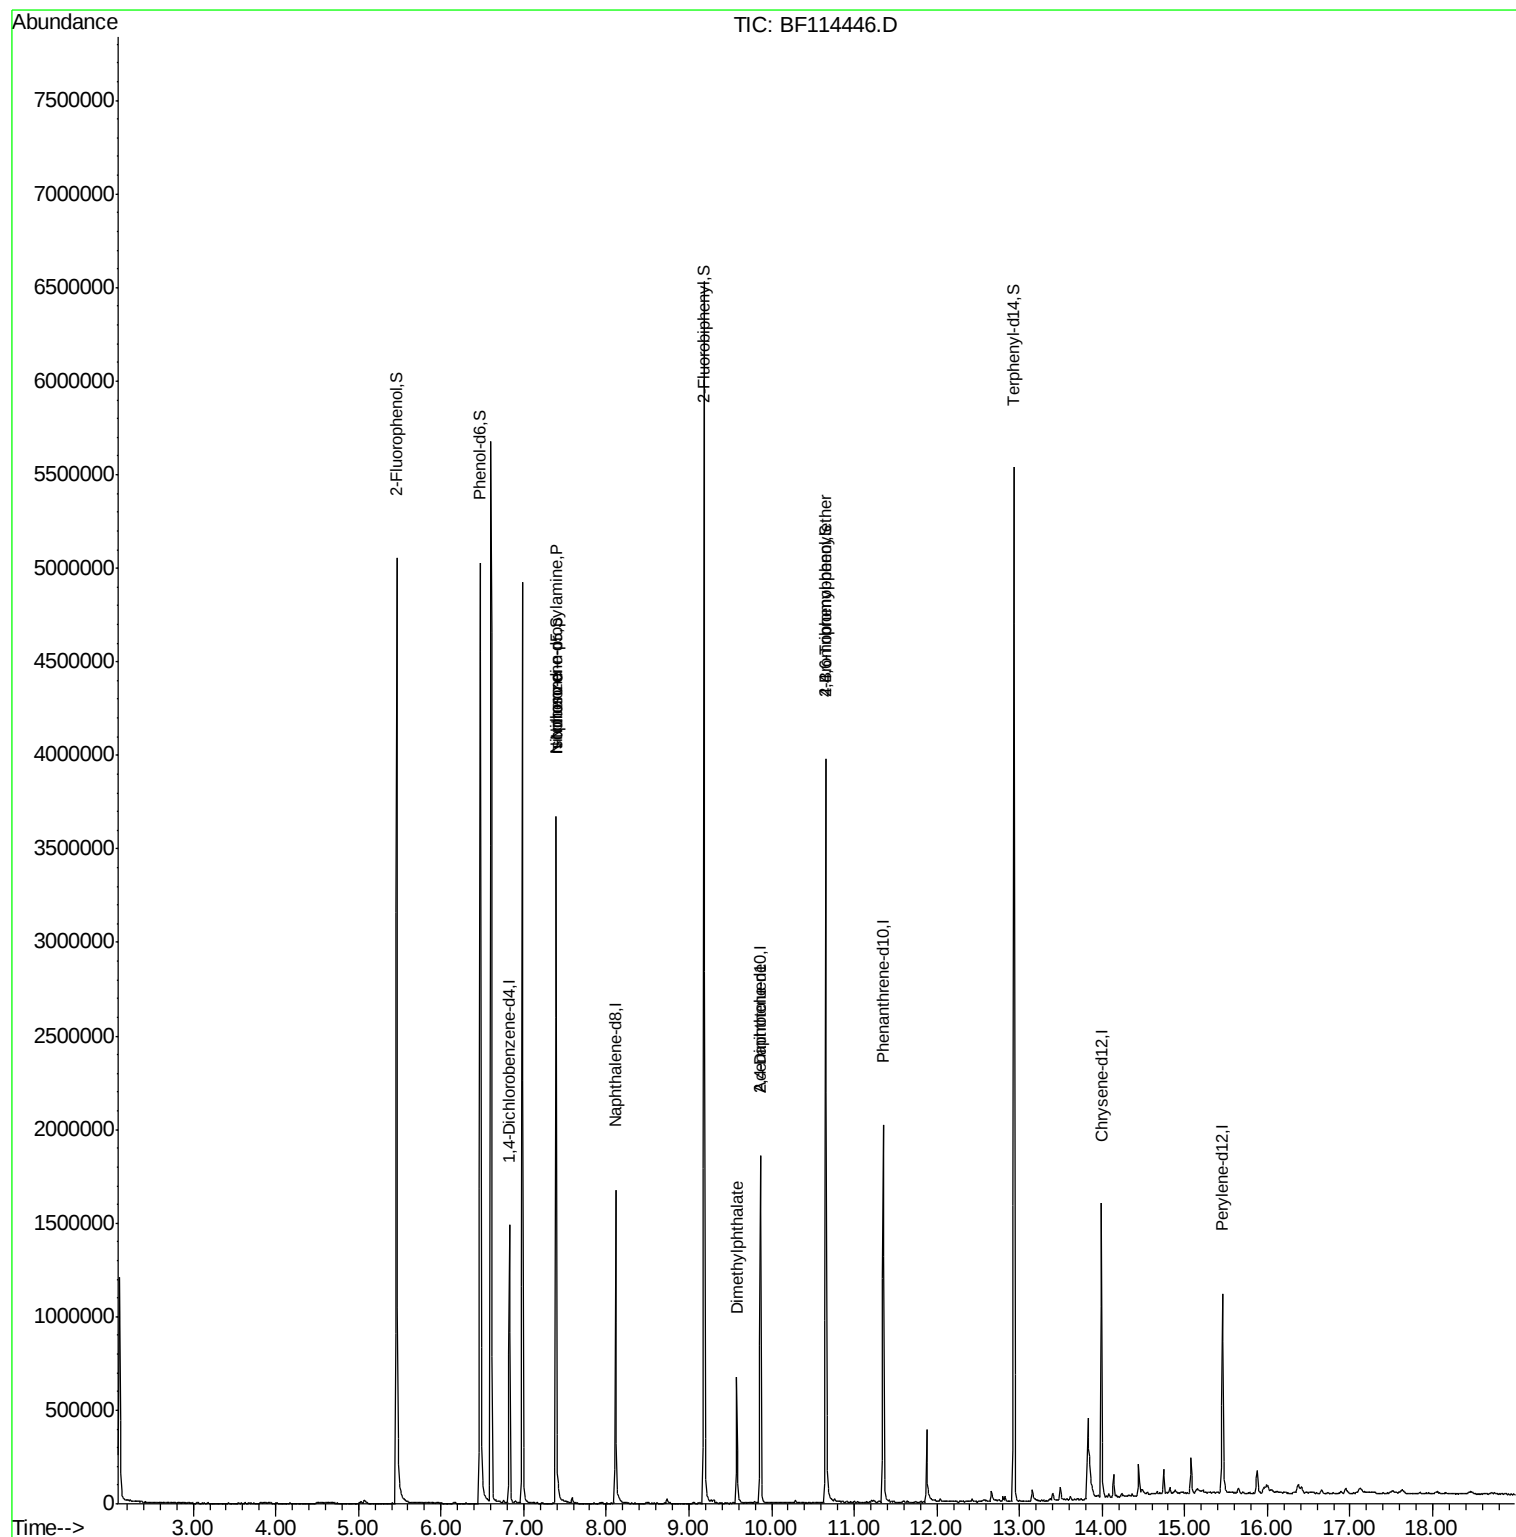




#1

1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.83 min Scan# 806
 Delta R.T. -0.01 min
 Lab File: BF114446.D
 Acq: 21 May 2019 3:09

Instrument :
 BNA_F
 ClientSampled :

Tot Ion	Ratio	Lower	Upper
152	100		
150	155.0	124.3	186.5
115	60.1	49.1	73.7



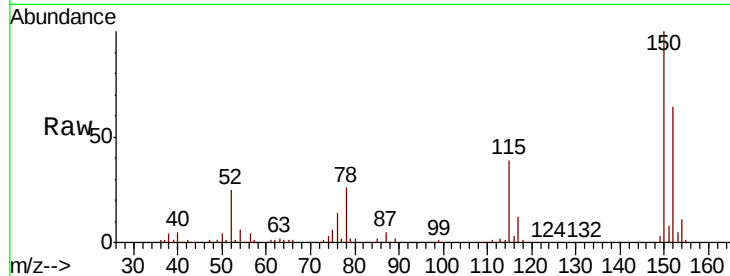


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

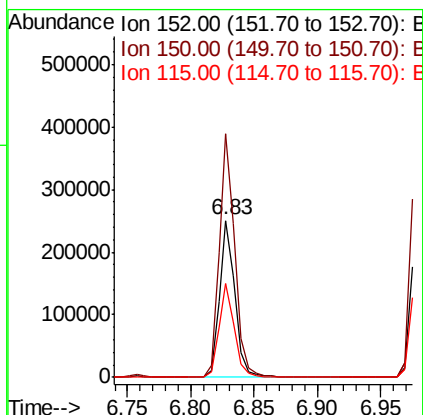

#5

2-Fluorophenol
 Concen: 116.315 ng
 RT: 5.46 min Scan# 574
 Delta R.T. -0.01 min
 Lab File: BF114446.D
 Acq: 21 May 2019 3:09

Tgt Ion	Ratio	Lower	Upper
112	100		
64	68.1	49.0	73.6
63	34.2	24.6	37.0





Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF1

Ion 63.00 (62.70 to 63.70): BF1

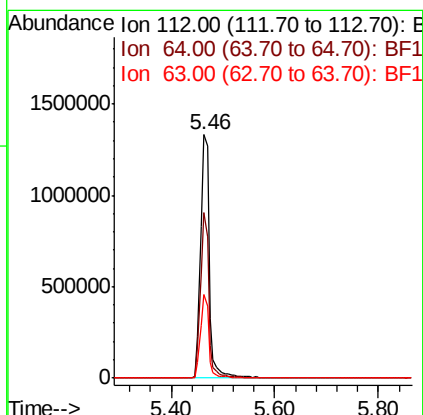



#7

Phenol-d6

Concen: 127.655 ng

RT: 6.47 min Scan# 746

Delta R.T. -0.01 min

Lab File: BF114446.D

Acq: 21 May 2019 3:09





Instrument :

BNA_F

ClientSampleId :

Tot Ion: 99 Resp: 2017143

Ion	Ratio	Lower	Upper
99	100		
42	23.6	17.9	26.9
71	34.7	26.2	39.2

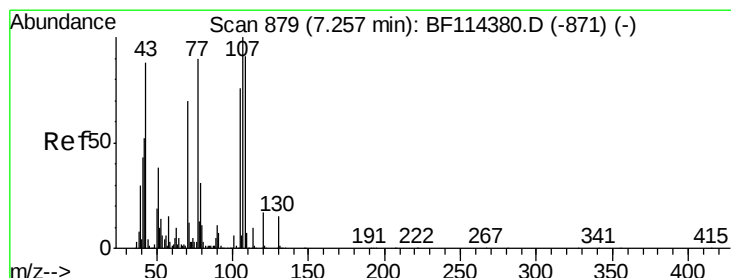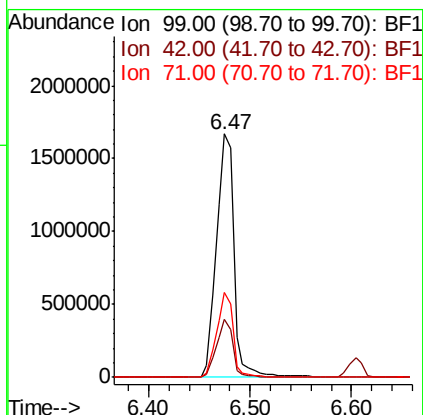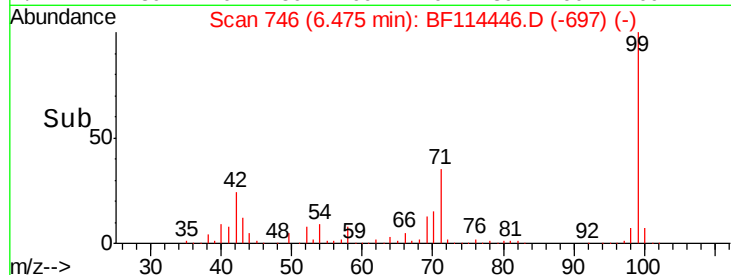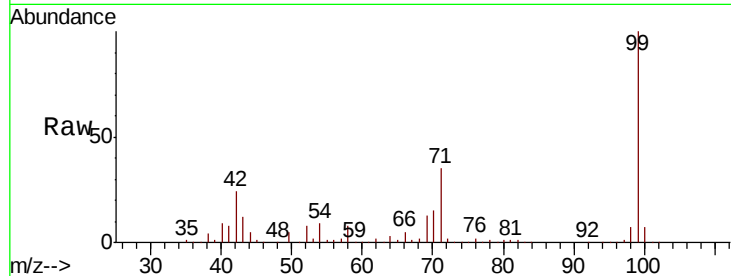

#19

n-Nitroso-di-n-propylamine

Concen: 16.706 ng

RT: 7.39 min Scan# 902




Delta R.T. 0.14 min


Lab File: BF114446.D

Acq: 21 May 2019 3:09

Tgt Ion: 70 Resp: 167324

Ion	Ratio	Lower	Upper
70	100		
42	57.6	58.6	87.8#
101	0.0	7.8	11.8#
130	2.3	17.1	25.7#


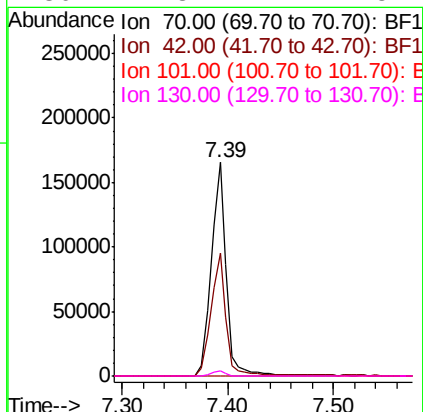
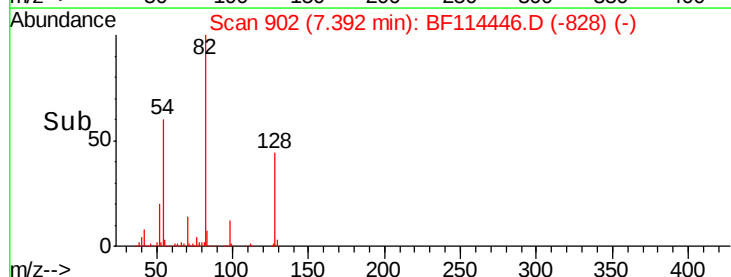
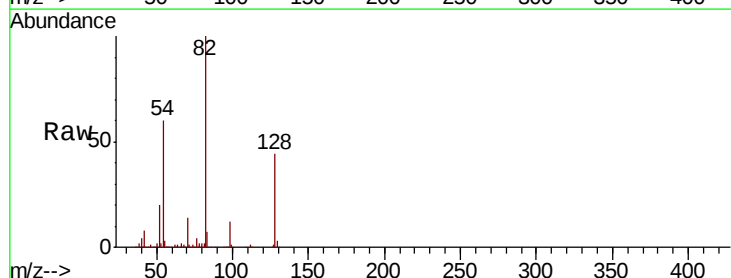


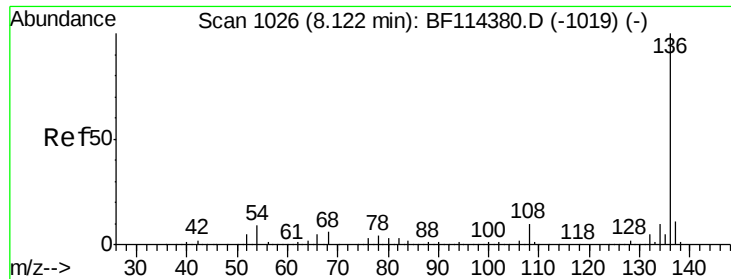

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.11 min Scan# 1024
Delta R.T. -0.01 min
Lab File: BF114446.D
Acq: 21 May 2019 3:09




Instrument :
BNA_F
ClientSampleId :


Tot Ion:136	Resp:	818365
Ion Ratio	Lower	Upper
136	100	
137	11.1	8.8 13.2
54	9.3	7.8 11.8
68	6.3	5.1 7.7

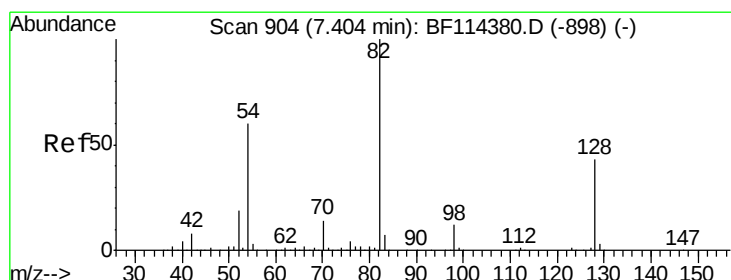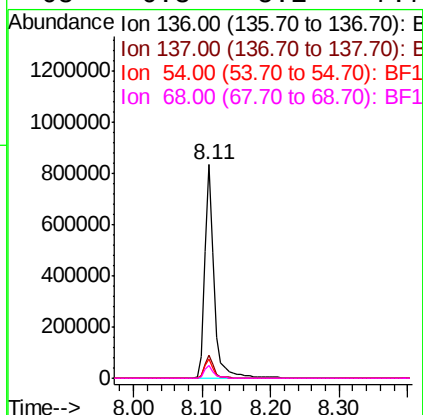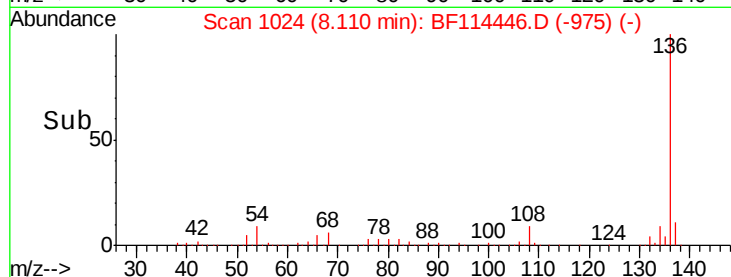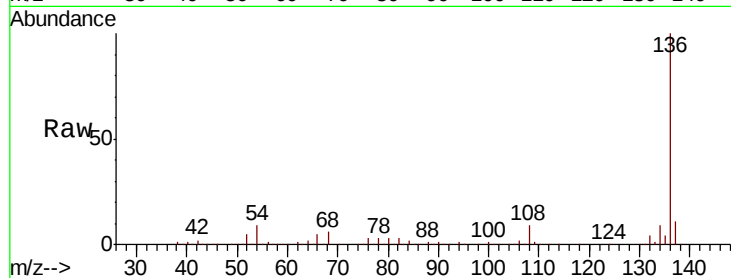

#23
Nitrobenzene-d5
Concen: 86.263 ng
RT: 7.39 min Scan# 902
Delta R.T. -0.01 min
Lab File: BF114446.D
Acq: 21 May 2019 3:09

Tgt Ion: 82	Resp:	1257927
Ion Ratio	Lower	Upper
82	100	
128	43.9	35.5 53.3
54	60.1	48.5 72.7

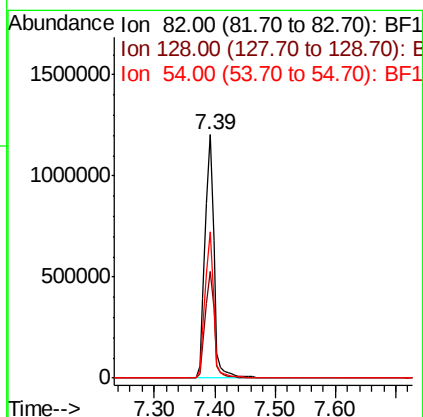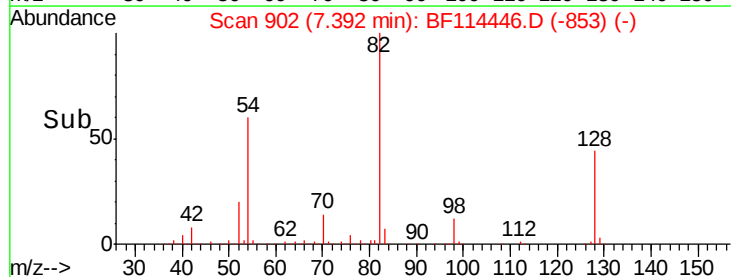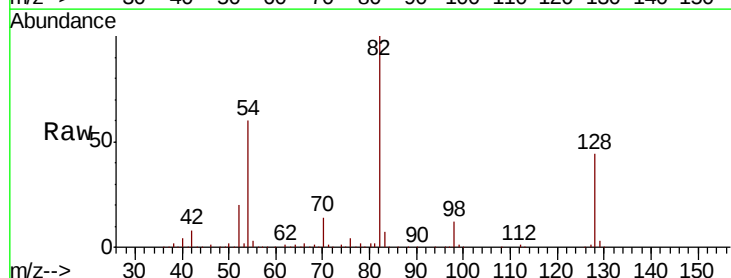

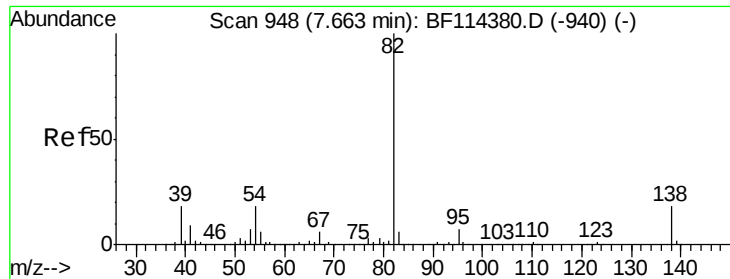

#25

Isophorone

Concen: 46.513 ng

RT: 7.39 min Scan# 902

Delta R.T. -0.27 min

Lab File: BF114446.D

Acq: 21 May 2019 3:09

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 82 Resp: 1257921

Ion Ratio Lower Upper

82 100

95 0.0 5.6 8.4#




138 0.0 14.8 22.2#

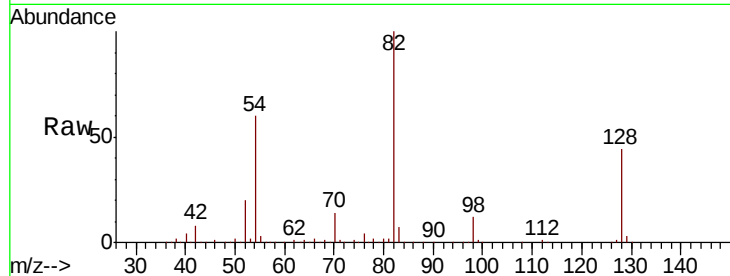

Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 95.00 (94.70 to 95.70): BF1

Ion 138.00 (137.70 to 138.70): BF1

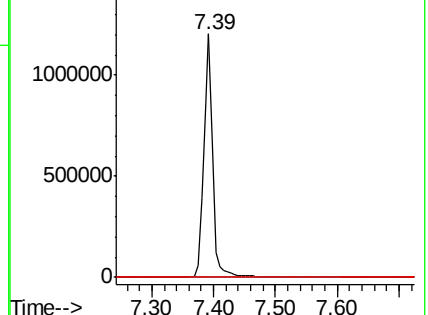

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.86 min Scan# 1322

Delta R.T. -0.01 min

Lab File: BF114446.D

Acq: 21 May 2019 3:09


Tgt Ion: 164 Resp: 383127

Ion Ratio Lower Upper

164 100

162 101.8 80.6 120.8



160 44.9 36.5 54.7




Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

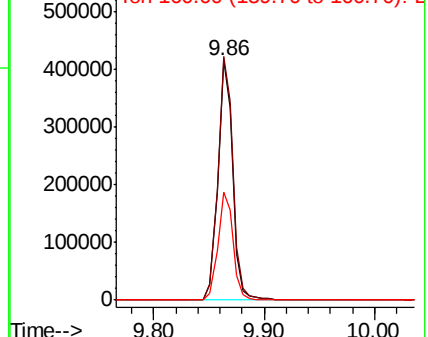




#42
 2,4,6-Tribromophenol
 Concen: 124.426 ng
 RT: 10.66 min Scan# 1457
 Delta R.T. -0.01 min
 Lab File: BF114446.D
 Acq: 21 May 2019 3:09

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
330	100		
332	102.4	81.4	122.2
141	32.6	26.6	40.0



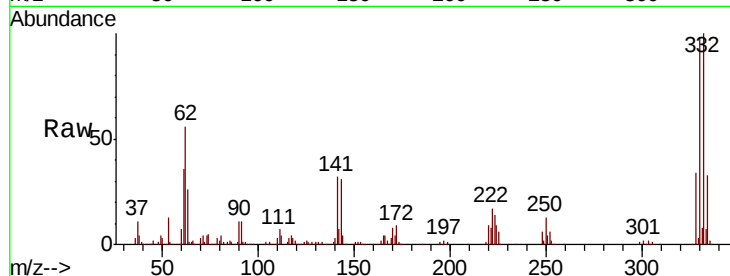


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

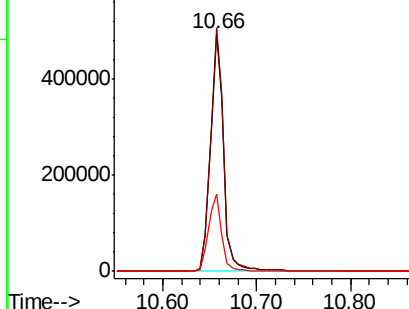

#45
 2-Fluorobiphenyl
 Concen: 80.692 ng
 RT: 9.19 min Scan# 1207
 Delta R.T. -0.01 min
 Lab File: BF114446.D
 Acq: 21 May 2019 3:09

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.8	30.7	46.1
170	24.6	20.5	30.7






Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

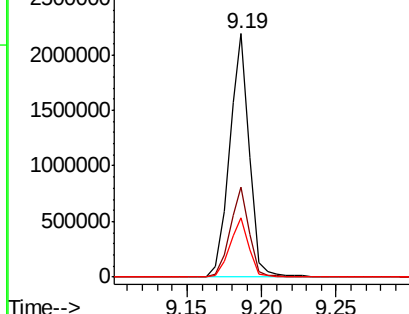


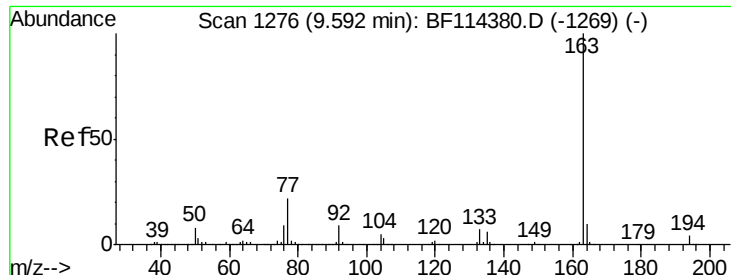




#50
Dimethylphthalate
Concen: 11.094 ng
RT: 9.58 min Scan# 1274
Delta R.T. -0.01 min
Lab File: BF114446.D
Acq: 21 May 2019 3:09

Instrument :
BNA_F
ClientSampleId :

Tot Ion:163 Resp: 312012
Ion Ratio Lower Upper
163 100
194 4.0 3.4 5.0
164 10.4 8.2 12.2

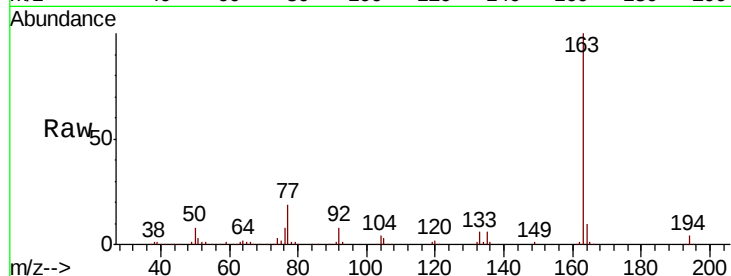


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

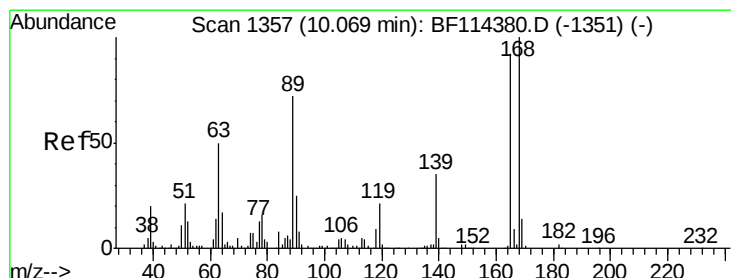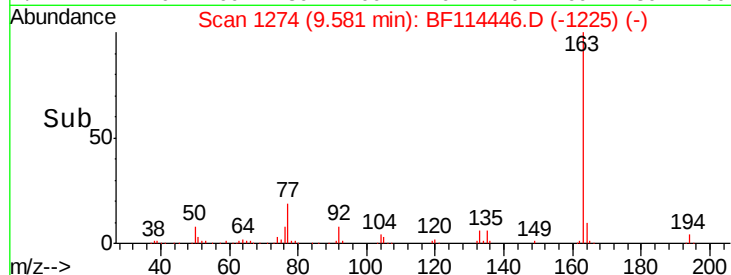
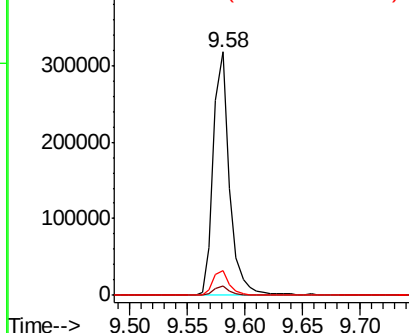



#57
2,4-Dinitrotoluene
Concen: 5.871 ng
RT: 9.86 min Scan# 1322
Delta R.T. -0.21 min
Lab File: BF114446.D
Acq: 21 May 2019 3:09

Tgt Ion:165 Resp: 49707
Ion Ratio Lower Upper
165 100
63 1.1 35.5 53.3#
89 1.1 55.2 82.8#
182 0.0 2.2 3.2#

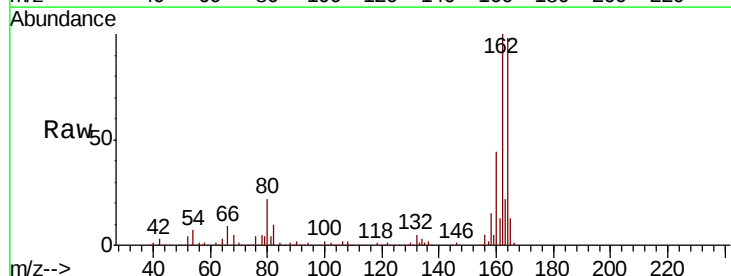

Abundance Ion 165.00 (164.70 to 165.70): E
Ion 63.00 (62.70 to 63.70): BF1
Ion 89.00 (88.70 to 89.70): BF1
Ion 182.00 (181.70 to 182.70): E

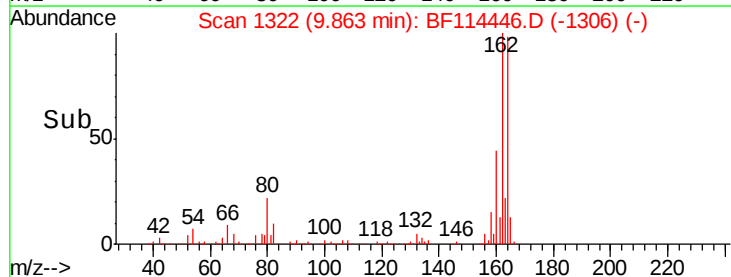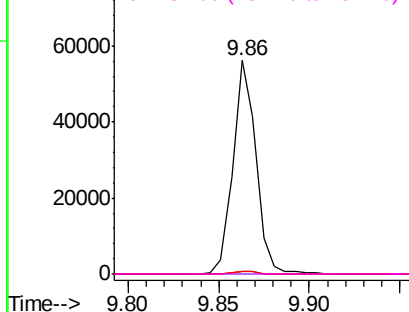



#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.35 min Scan# 1575

Delta R.T. -0.01 min

Lab File: BF114446.D

Acq: 21 May 2019 3:09

Instrument :

BNA_F

ClientSampled :



Tot Ion:188 Resp: 785943

Ion Ratio Lower Upper

188 100

94 9.7 8.4 12.6



80 10.6 9.2 13.8



Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

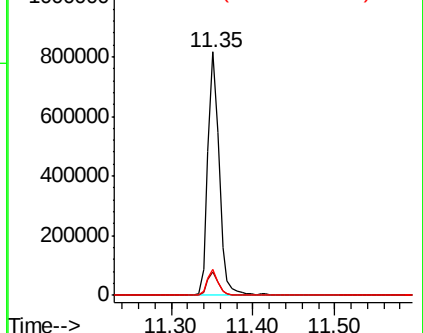

#67

4-Bromophenyl-phenylether

Concen: 3.736 ng

RT: 10.66 min Scan# 1457

Delta R.T. -0.24 min

Lab File: BF114446.D

Acq: 21 May 2019 3:09



Tgt Ion:248 Resp: 32333

Ion Ratio Lower Upper

248 100

250 198.9 77.4 116.2#


141 490.3 55.6 83.4#




Abundance Ion 248.00 (247.70 to 248.70): E

Ion 250.00 (249.70 to 250.70): E

Ion 141.00 (140.70 to 141.70): E

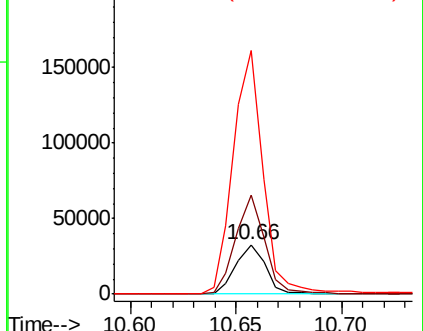



#76

Chrysene-d12

Concen: 20.000 ng

RT: 13.99 min Scan# 2024

Delta R.T. -0.01 min

Lab File: BF114446.D

Acq: 21 May 2019 3:09

Instrument :

BNA_F

ClientSampleId :


Tot Ion:240 Resp: 524737

Ion Ratio Lower Upper

240 100

120 11.8 8.3 12.5




236 26.7 20.8 31.2



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

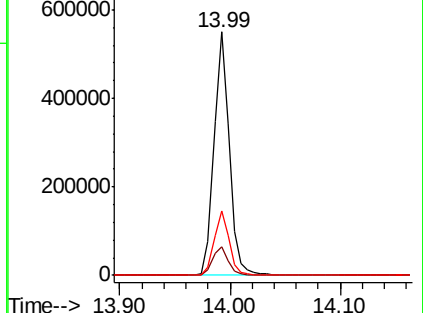

#79

Terphenyl-d14

Concen: 83.541 ng

RT: 12.93 min Scan# 1844

Delta R.T. -0.01 min

Lab File: BF114446.D

Acq: 21 May 2019 3:09


Tgt Ion:244 Resp: 2126532

Ion Ratio Lower Upper

244 100

212 7.1 5.8 8.6



122 13.7 9.4 14.2




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

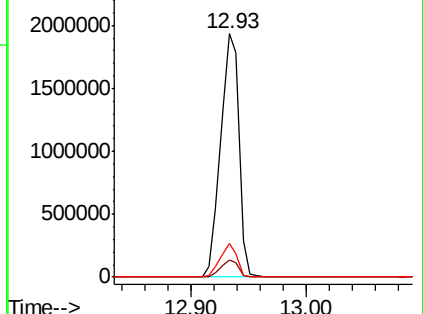

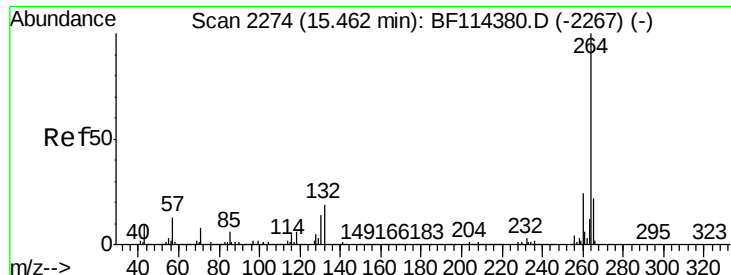

#87
Pervlene-d12
Concen: 20.000 ng
RT: 15.46 min Scan# 2273
Delta R.T. -0.01 min
Lab File: BF114446.D
Acq: 21 May 2019 3:09

Instrument :
BNA_F
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.4	19.4	29.0
265	20.9	16.9	25.3

