


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF052019\
 Data File : BF114440.D
 Acq On : 20 May 2019 15:56
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon May 20 04:47:40 2019

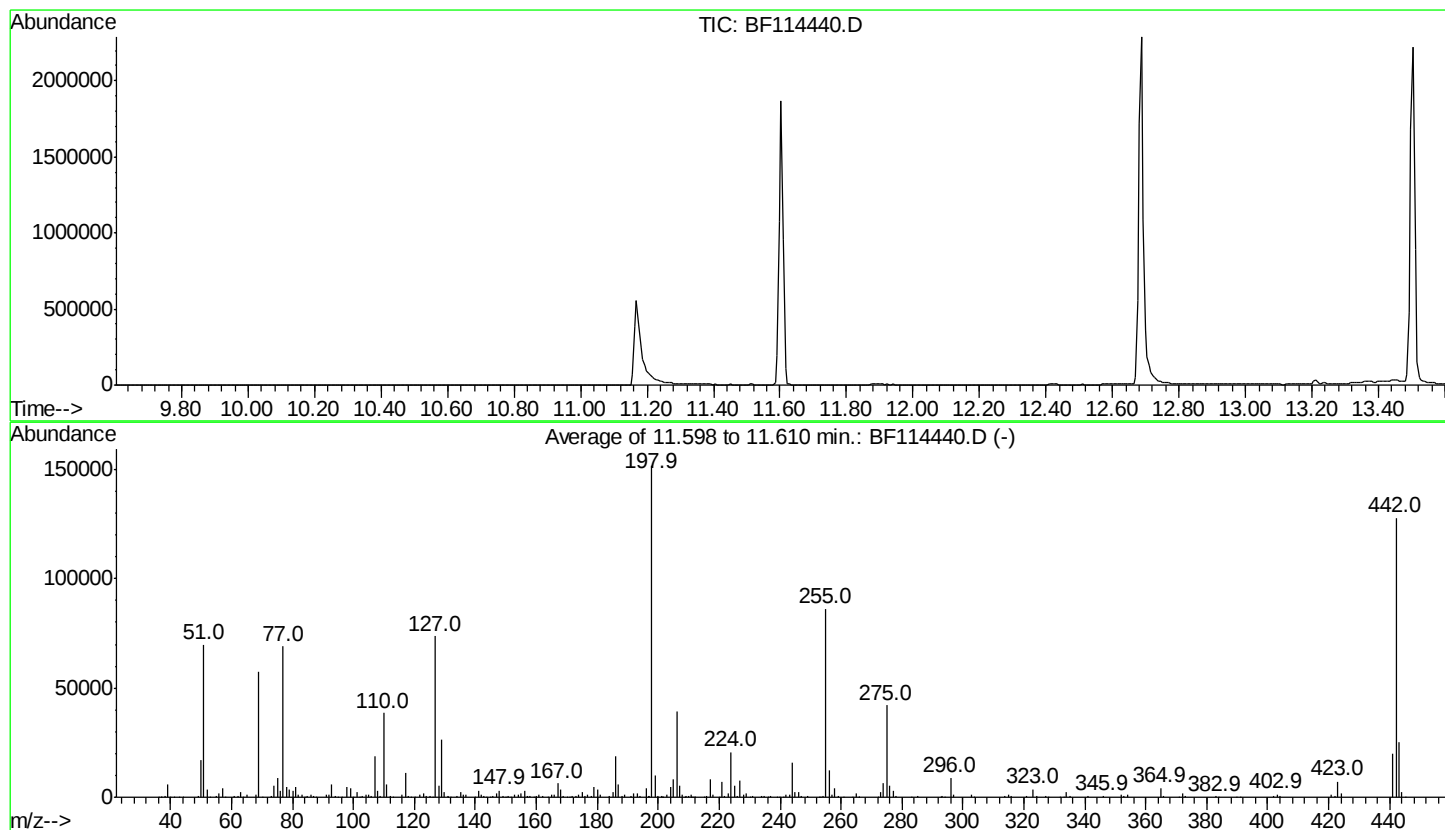

AutoFind: Scans 1617, 1618, 1619; Background Corrected with Scan 1612

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.0	69832	PASS
68	69	0.00	2	1.8	1052	PASS
69	198	0.00	100	37.7	57205	PASS
70	69	0.00	2	0.4	227	PASS
127	198	10	80	48.6	73706	PASS
197	198	0.00	2	0.5	688	PASS
198	198	100	100	100.0	151752	PASS
199	198	5	9	6.4	9737	PASS
275	198	10	60	27.7	42106	PASS
365	198	1	100	2.8	4226	PASS
441	198	0.01	100	13.3	20163	PASS
442	198	50	100	84.2	127744	PASS
443	442	15	24	19.7	25130	PASS