
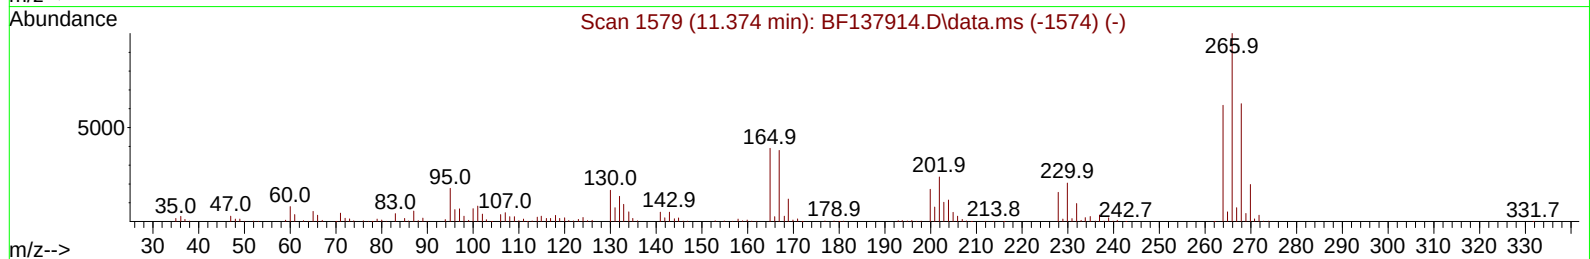
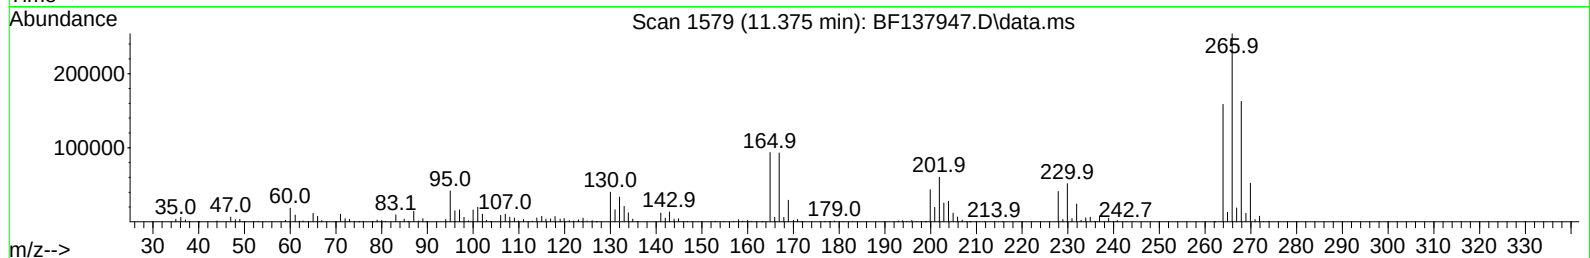


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052024\
Data File : BF137947.D
Acq On : 20 May 2024 08:29
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 20 11:26:28 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF051424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 15 04:12:16 2024
Response via : Initial Calibration

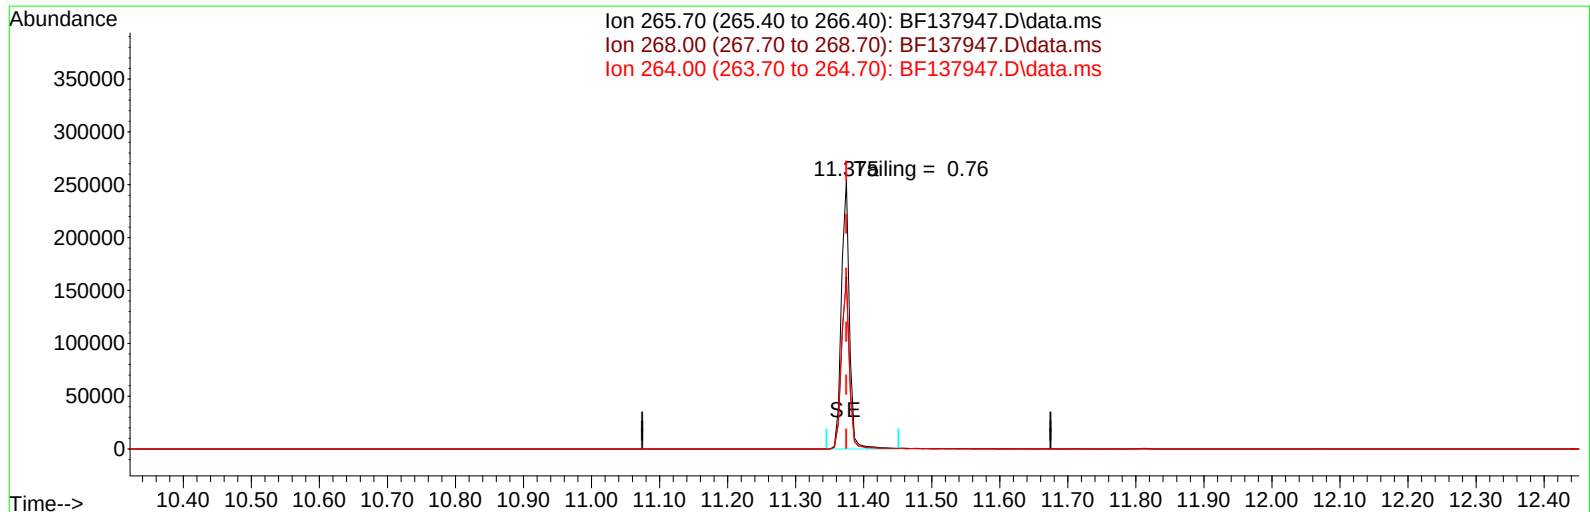

TIC: BF137947.D\data.ms

(70) Pentachlorophenol (C)




11.375min (+ 0.000) 34722.20 ng

response 209009

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	64.03
264.00	61.80	62.49
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052024\
Data File : BF137947.D
Acq On : 20 May 2024 08:29
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 20 11:26:28 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF051424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 15 04:12:16 2024
Response via : Initial Calibration

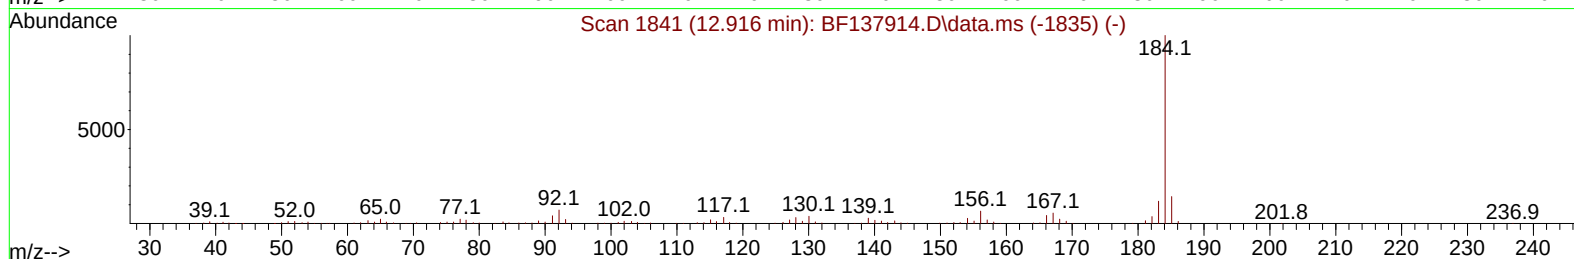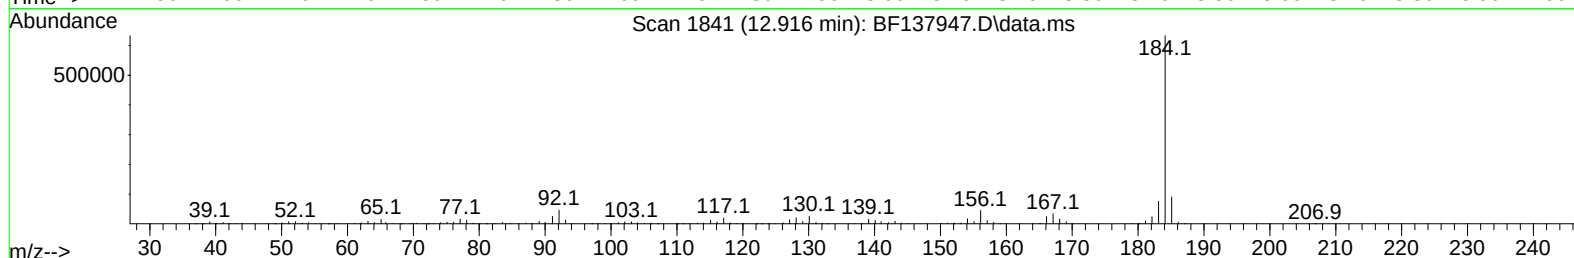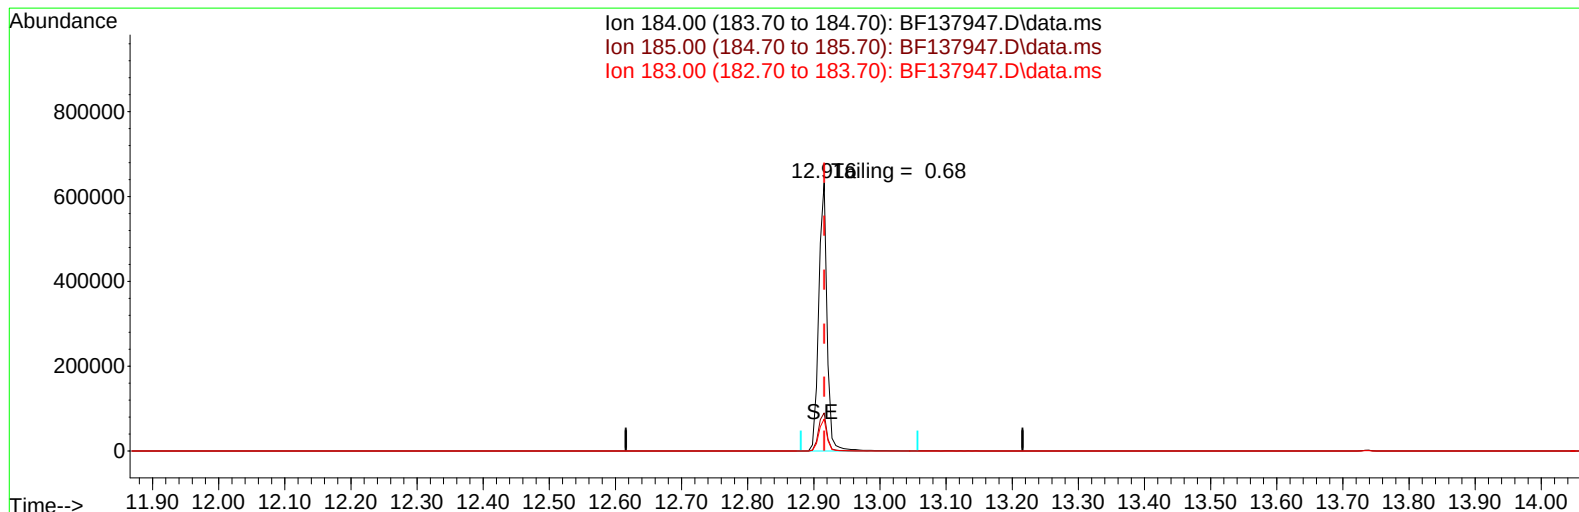

TIC: BF137947.D\data.ms

(77) Benzidine

12.916min (-0.000) 0.00 ng

response 557461

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.22
183.00	11.90	11.93
0.00	0.00	0.00