


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052024\
Data File : BF137947.D
Acq On : 20 May 2024 08:29
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF051424.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed May 15 04:12:16 2024

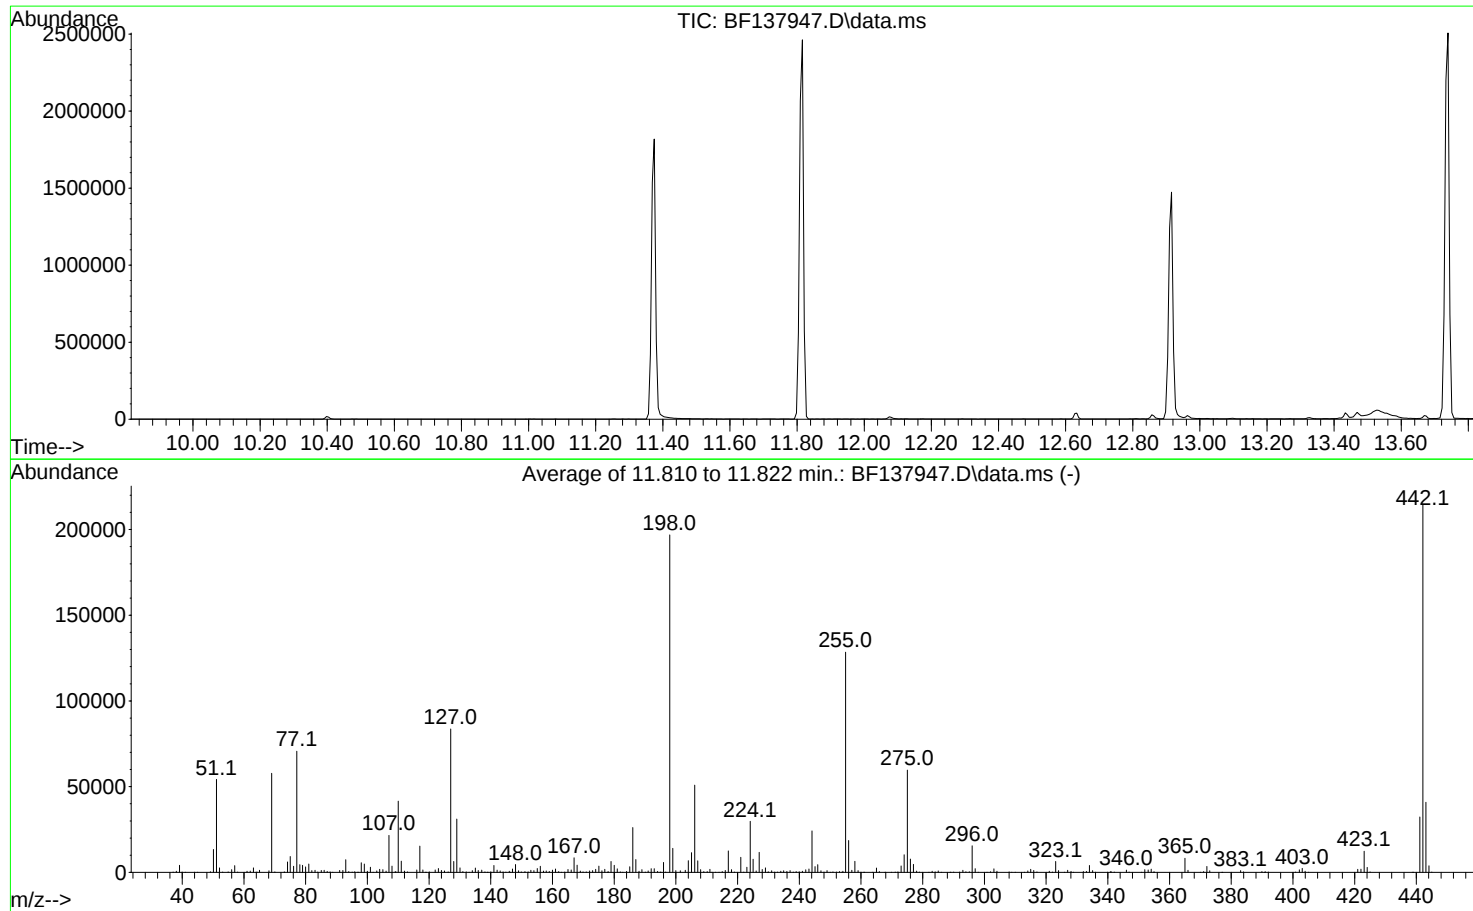

AutoFind: Scans 1653, 1654, 1655; Background Corrected with Scan 1648

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.5	54213	PASS
68	69	0.00	2	1.7	955	PASS
69	198	0.00	100	29.3	57738	PASS
70	69	0.00	2	0.6	320	PASS
127	198	10	80	42.5	83611	PASS
197	198	0.00	2	0.1	177	PASS
198	198	100	100	100.0	196880	PASS
199	198	5	9	7.1	14040	PASS
275	198	10	60	30.3	59600	PASS
365	198	1	100	4.2	8251	PASS
441	198	0.01	100	16.4	32325	PASS
442	442	50	100	100.0	214592	PASS
443	442	15	24	19.1	40888	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/20/2024	BNA_F	<u>BF137947.D</u>
Compound Name	Response	Retention Time
DDT	445850	13.739
DDD	10170	13.433
DDE	639	13.098
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10809	456659	2.37

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052024\
Data File : BF137947.D
Acq On : 20 May 2024 08:29
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 20 11:26:28 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF051424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 15 04:12:16 2024
Response via : Initial Calibration

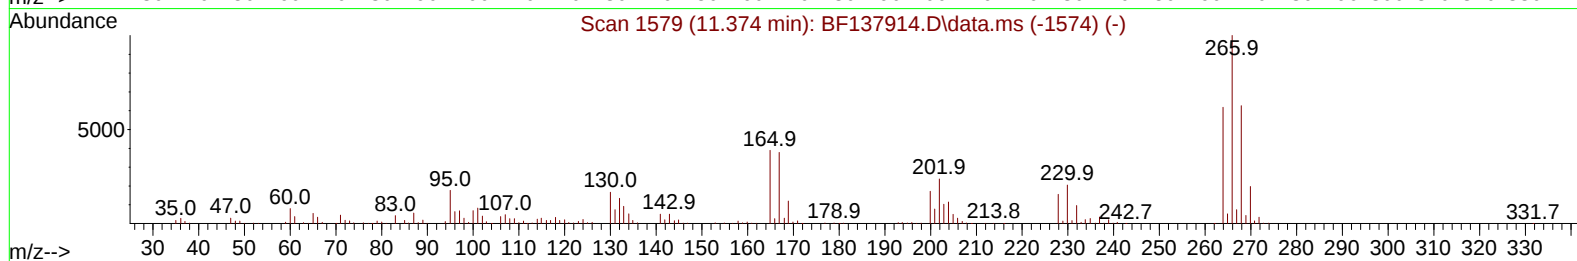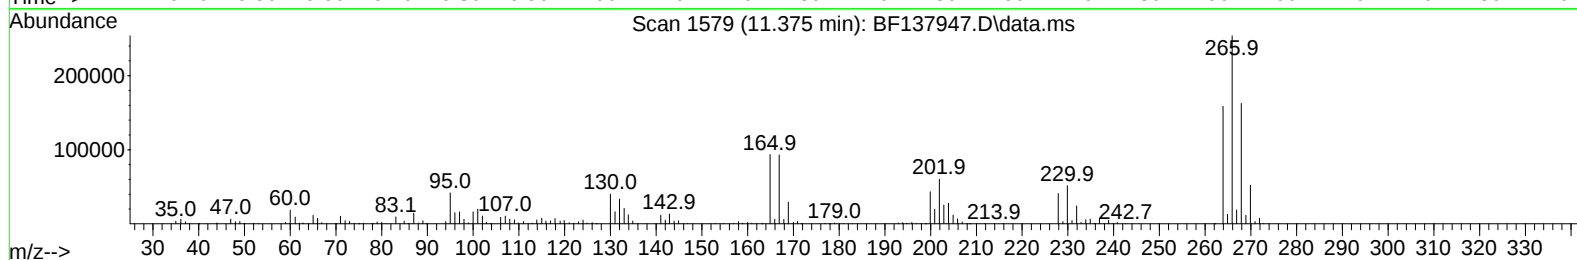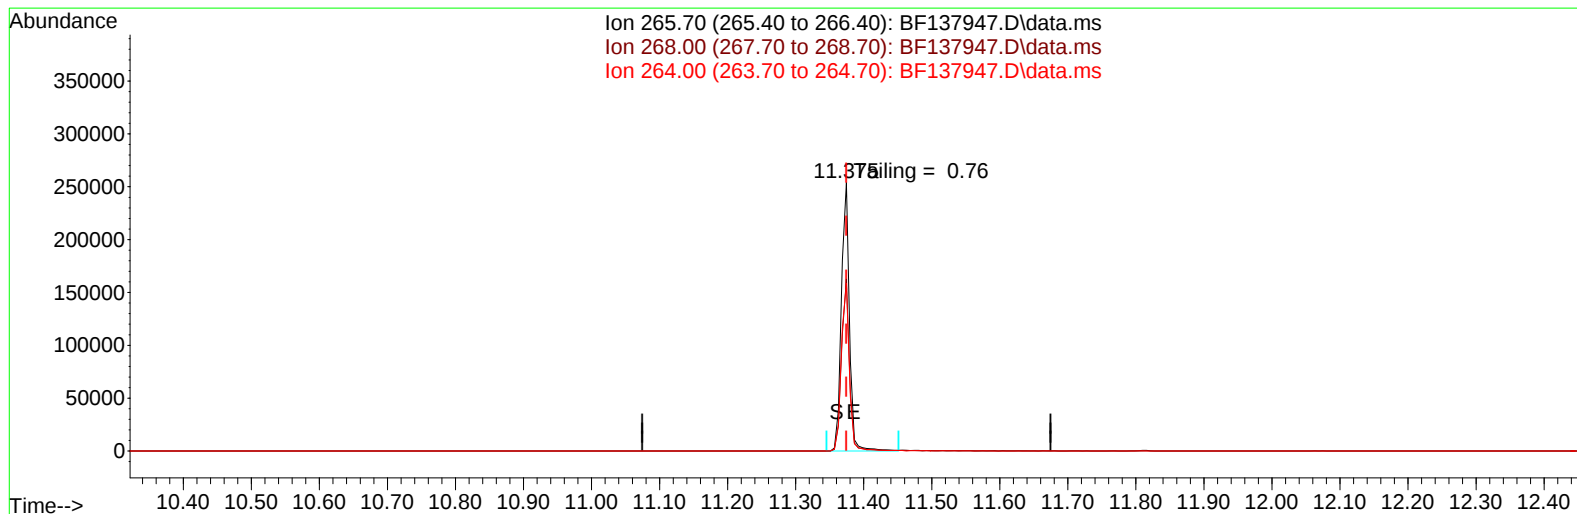

TIC: BF137947.D\data.ms

(70) Pentachlorophenol (C)

11.375min (+ 0.000) 34722.20 ng




response 209009

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	64.03
264.00	61.80	62.49
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052024\
Data File : BF137947.D
Acq On : 20 May 2024 08:29
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 20 11:26:28 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF051424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 15 04:12:16 2024
Response via : Initial Calibration

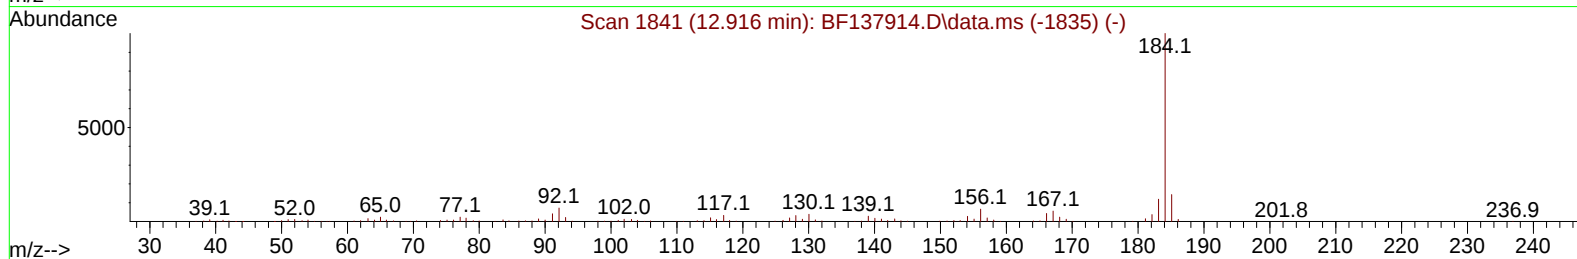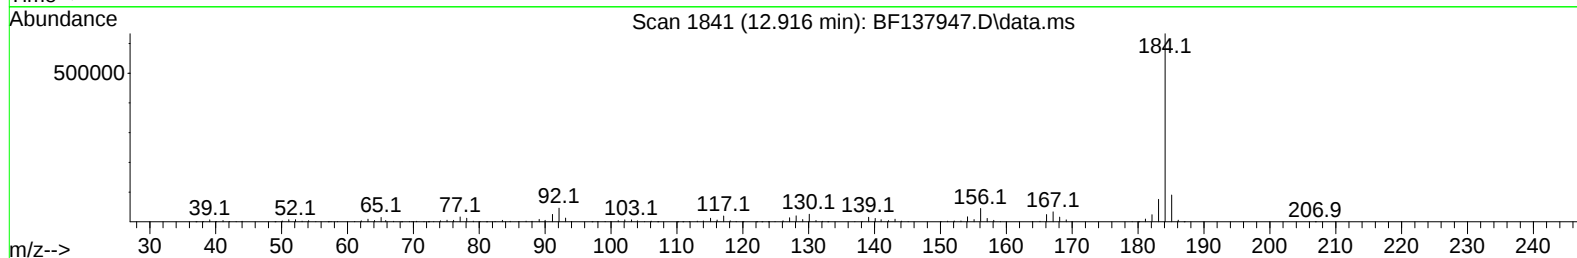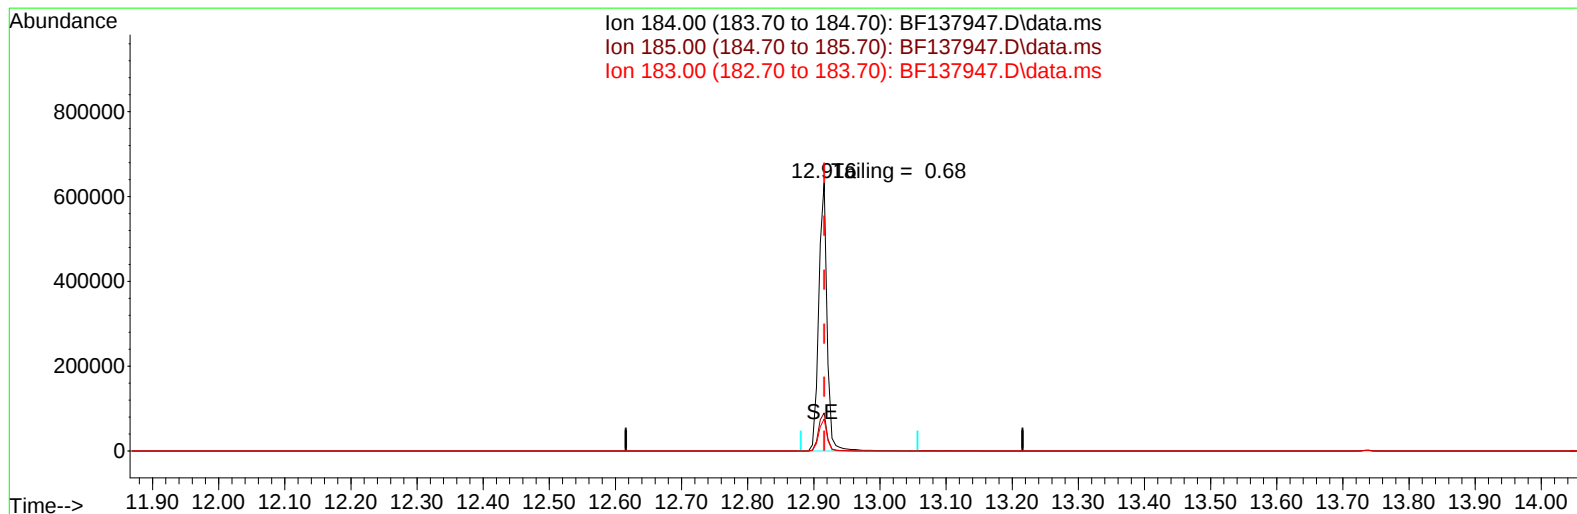

TIC: BF137947.D\data.ms

(77) Benzidine

12.916min (-0.000) 0.00 ng

response 557461

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.22
183.00	11.90	11.93
0.00	0.00	0.00