


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF052119\
 Data File : BF114448.D
 Acq On : 21 May 2019 11:44
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon May 20 04:47:40 2019

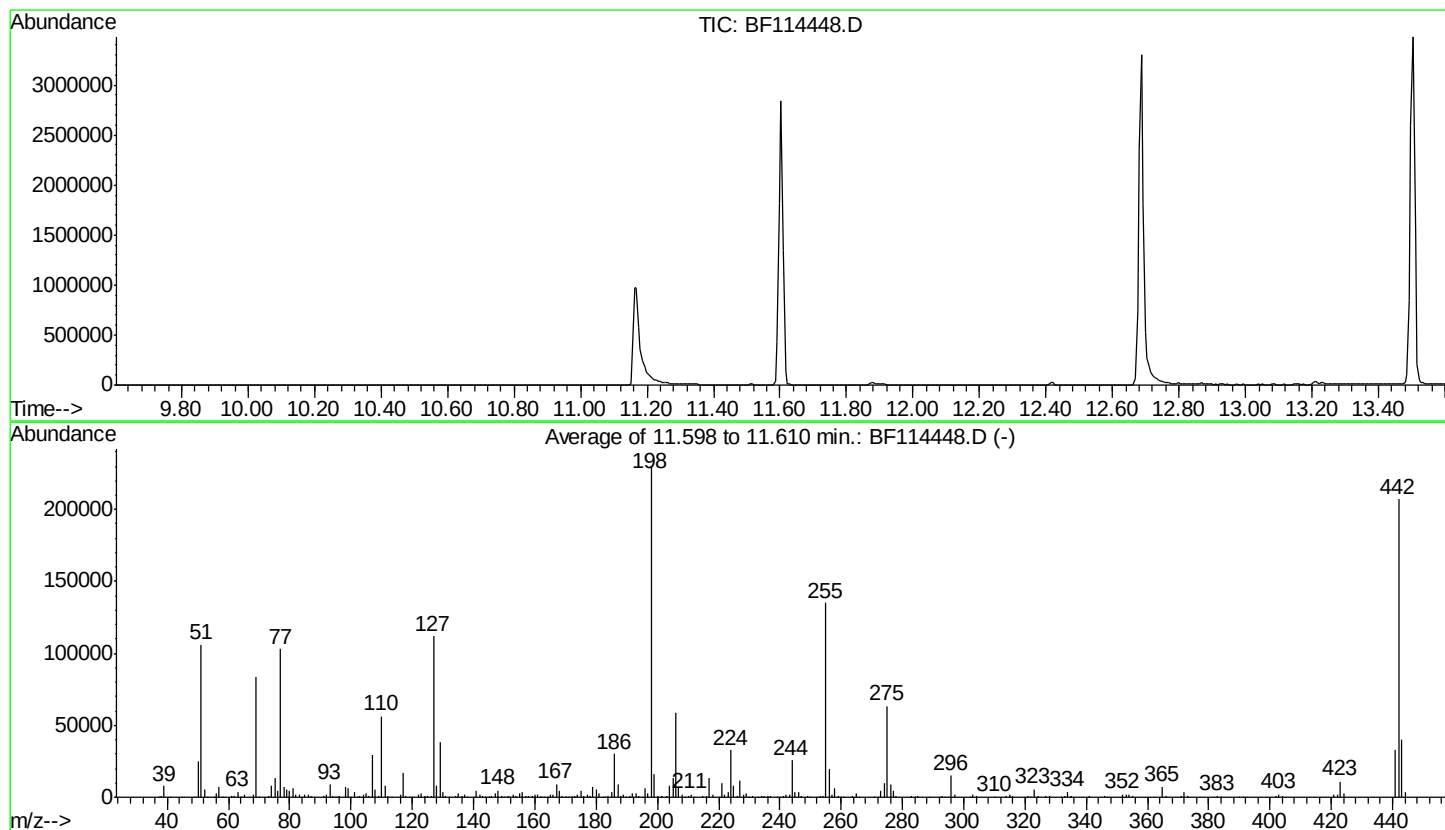

AutoFind: Scans 1617, 1618, 1619; Background Corrected with Scan 1611

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.0	106074	PASS
68	69	0.00	2	1.8	1480	PASS
69	198	0.00	100	36.3	83741	PASS
70	69	0.00	2	0.4	302	PASS
127	198	10	80	48.6	111906	PASS
197	198	0.00	2	1.1	2594	PASS
198	198	100	100	100.0	230485	PASS
199	198	5	9	6.8	15771	PASS
275	198	10	60	27.5	63485	PASS
365	198	1	100	3.2	7287	PASS
441	198	0.01	100	14.1	32512	PASS
442	198	50	100	89.8	206946	PASS
443	442	15	24	19.4	40138	PASS