


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052219\
Data File : BF114483.D
Acq On : 22 May 2019 9:21
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051019.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon May 20 04:47:40 2019

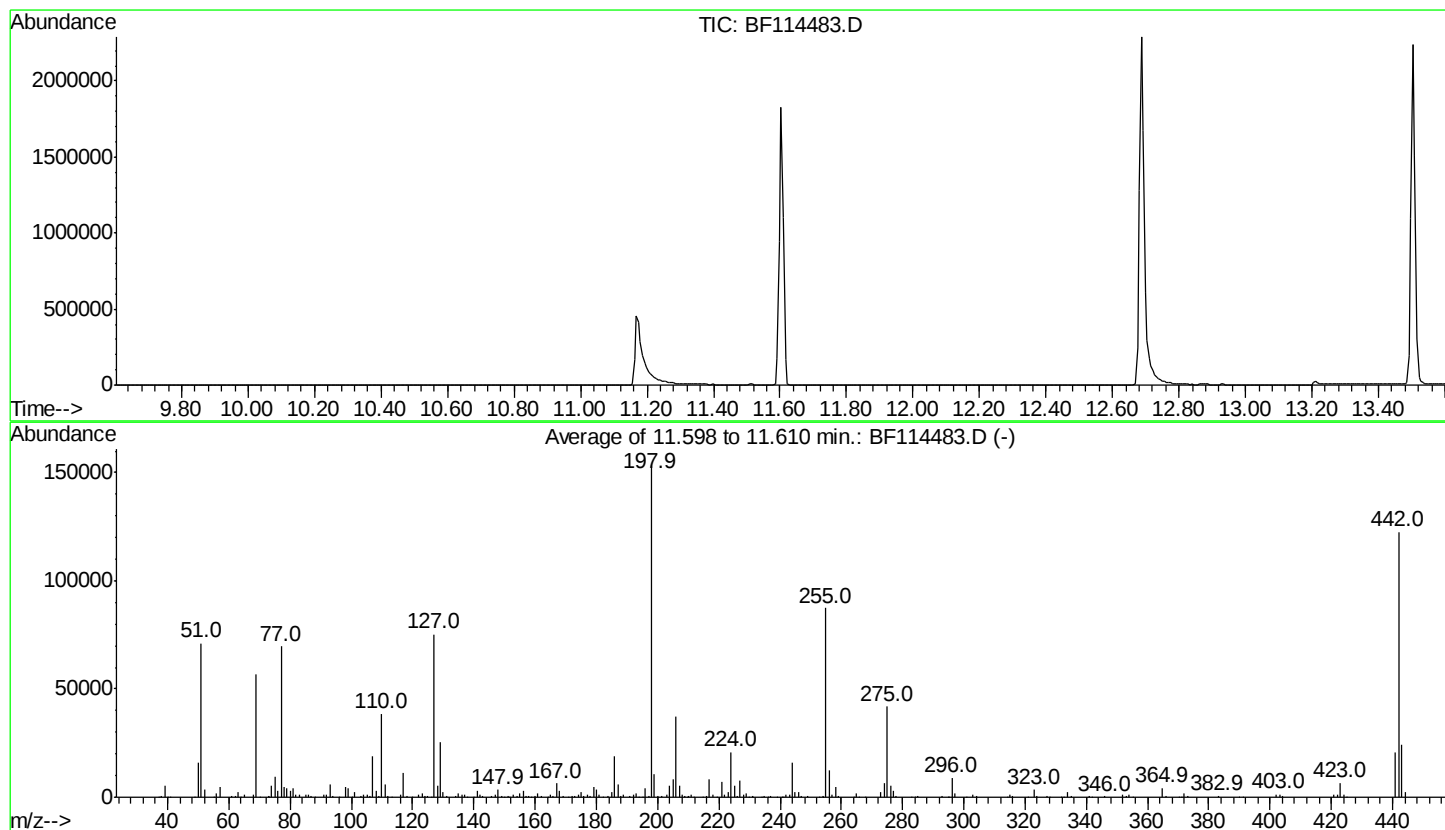

AutoFind: Scans 1617, 1618, 1619; Background Corrected with Scan 1612

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.4	71136	PASS
68	69	0.00	2	1.7	961	PASS
69	198	0.00	100	37.0	56741	PASS
70	69	0.00	2	0.4	253	PASS
127	198	10	80	49.1	75232	PASS
197	198	0.00	2	0.5	767	PASS
198	198	100	100	100.0	153213	PASS
199	198	5	9	6.8	10406	PASS
275	198	10	60	27.4	41954	PASS
365	198	1	100	2.9	4393	PASS
441	198	0.01	100	13.4	20560	PASS
442	198	50	100	80.0	122530	PASS
443	442	15	24	19.9	24330	PASS