


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF052219\
 Data File : BF114488.D
 Acq On : 22 May 2019 17:36
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 23 03:49:15 2019

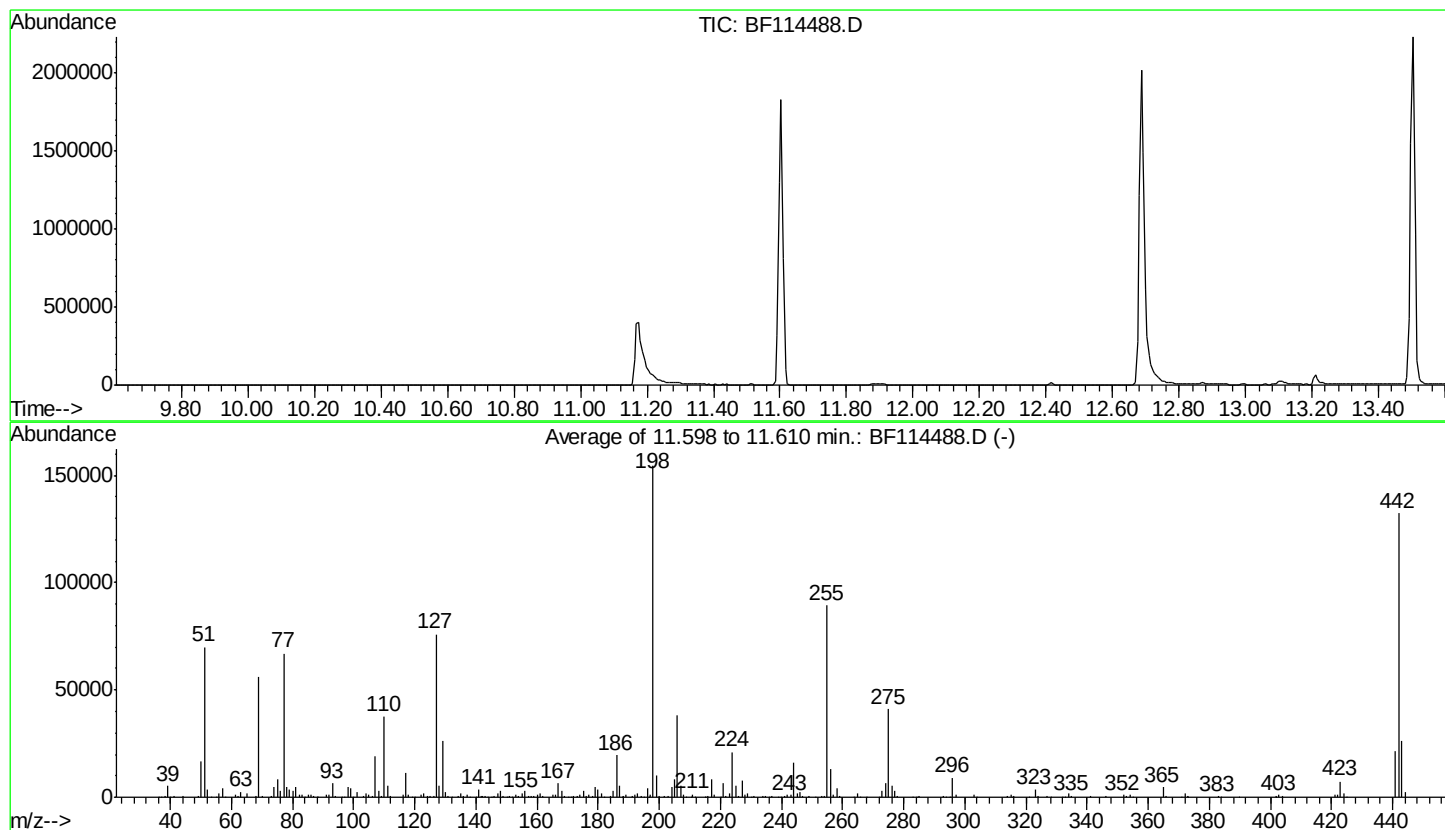

AutoFind: Scans 1617, 1618, 1619; Background Corrected with Scan 1612

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.2	69874	PASS
68	69	0.00	2	1.6	889	PASS
69	198	0.00	100	36.4	56224	PASS
70	69	0.00	2	0.6	358	PASS
127	198	10	80	49.2	76016	PASS
197	198	0.00	2	0.7	1012	PASS
198	198	100	100	100.0	154544	PASS
199	198	5	9	6.5	10063	PASS
275	198	10	60	26.5	41026	PASS
365	198	1	100	3.0	4679	PASS
441	198	0.01	100	14.0	21569	PASS
442	198	50	100	85.6	132285	PASS
443	442	15	24	19.8	26229	PASS