


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF052219\
 Data File : BF114513.D
 Acq On : 23 May 2019 5:11
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 23 03:49:15 2019

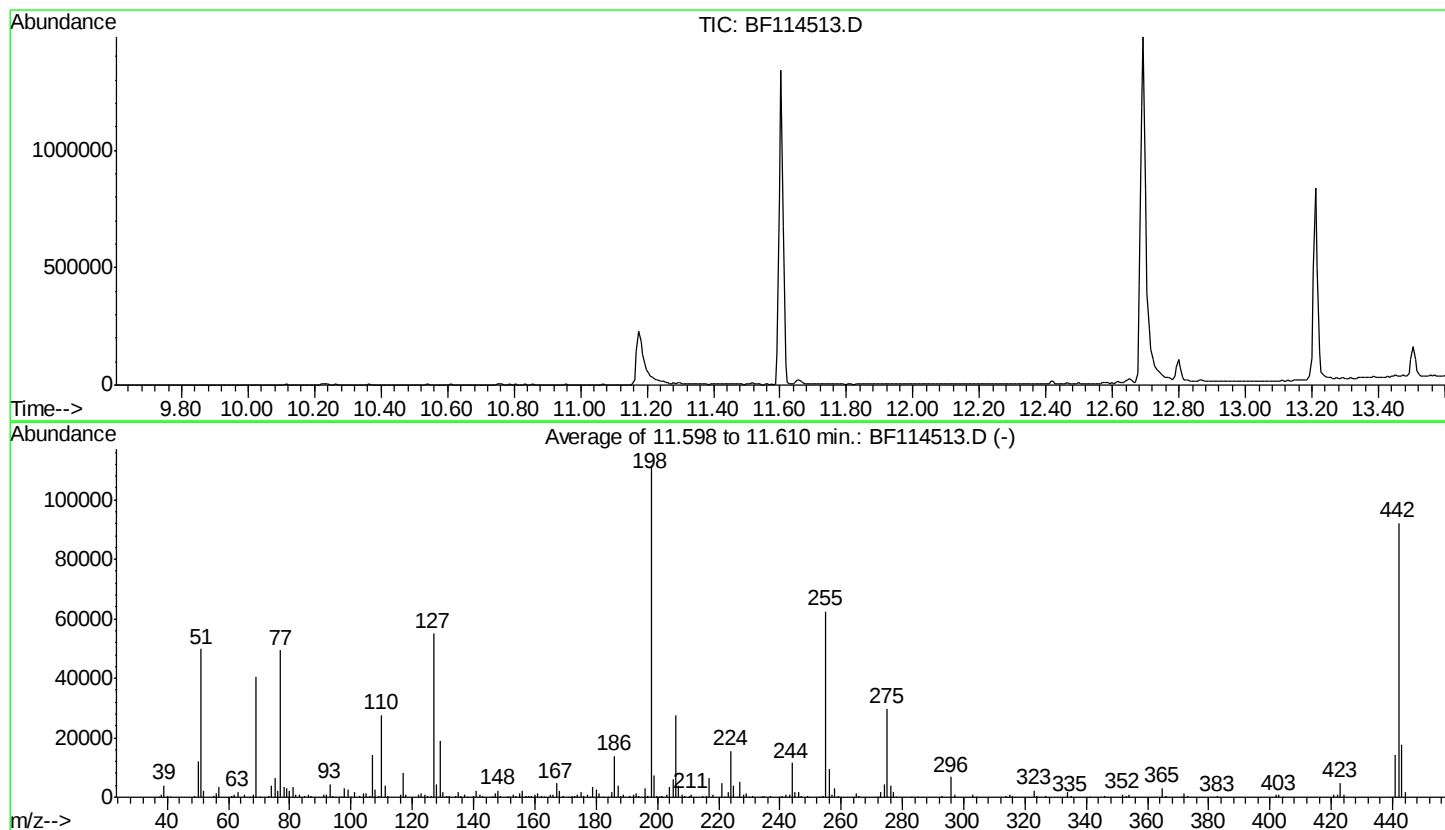

AutoFind: Scans 1617, 1618, 1619; Background Corrected with Scan 1612

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.6	49736	PASS
68	69	0.00	2	1.8	732	PASS
69	198	0.00	100	36.2	40352	PASS
70	69	0.00	2	0.5	217	PASS
127	198	10	80	49.3	54992	PASS
197	198	0.00	2	0.4	459	PASS
198	198	100	100	100.0	111496	PASS
199	198	5	9	6.7	7485	PASS
275	198	10	60	26.8	29832	PASS
365	198	1	100	2.9	3182	PASS
441	198	0.01	100	12.6	14035	PASS
442	198	50	100	82.8	92304	PASS
443	442	15	24	19.0	17582	PASS