
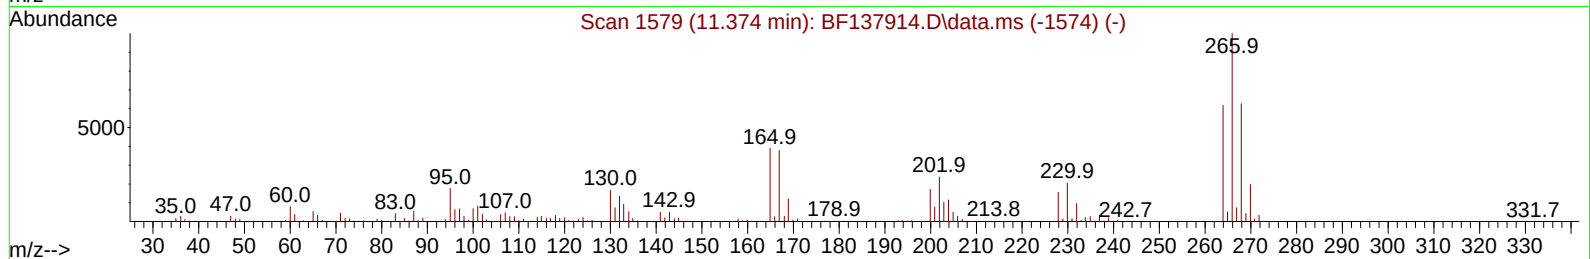
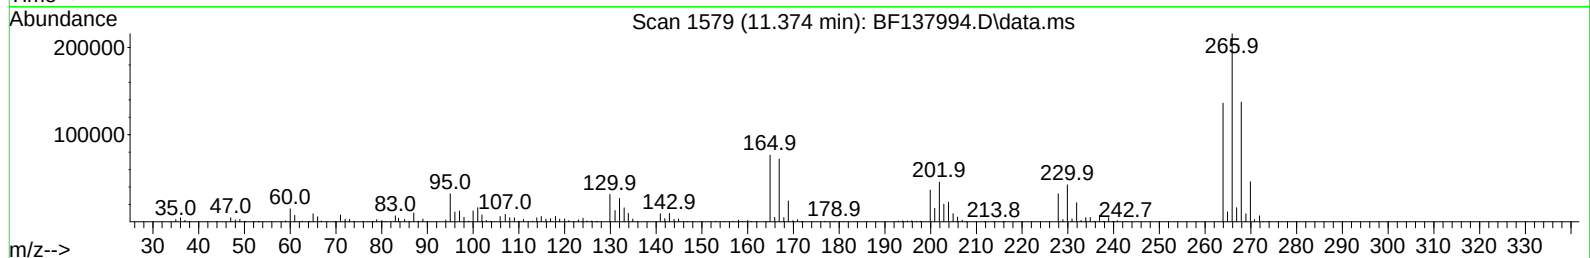


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052224\
Data File : BF137994.D
Acq On : 22 May 2024 09:17
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 22 09:37:50 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF051424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 15 04:12:16 2024
Response via : Initial Calibration

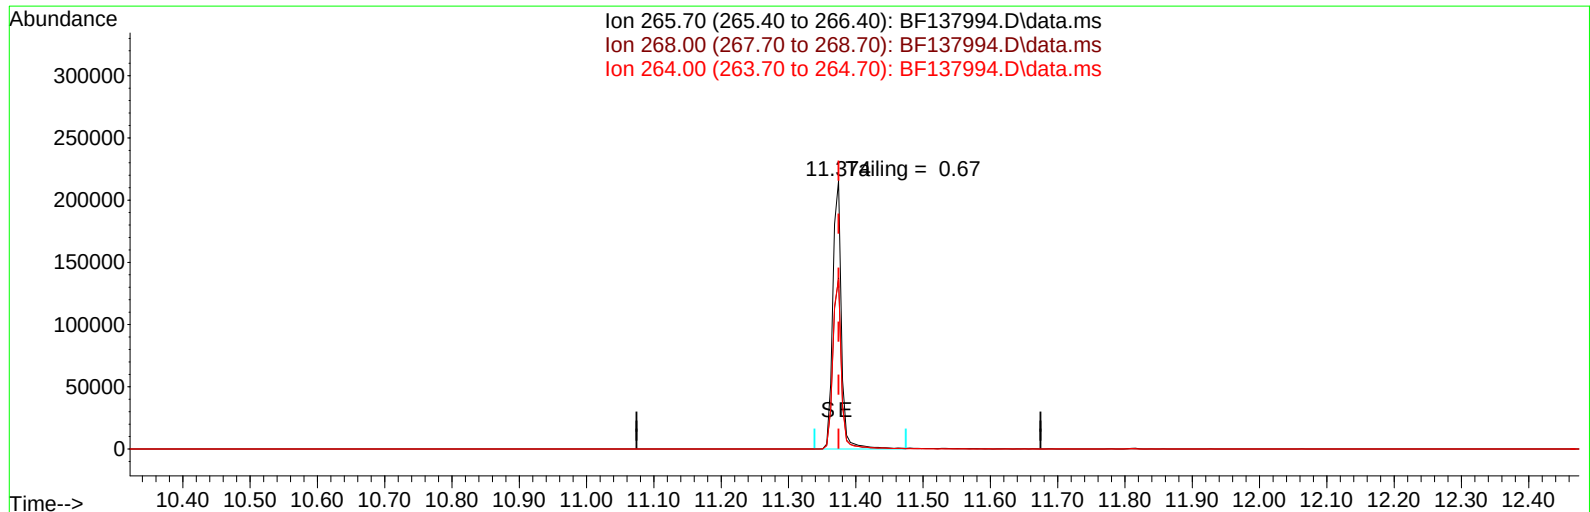

TIC: BF137994.D\data.ms

(70) Pentachlorophenol (C)




11.374min (0.000) 29246.02 ng

response 192861

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	63.71
264.00	61.80	63.12
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052224\  
Data File : BF137994.D  
Acq On    : 22 May 2024  09:17  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: May 22 09:37:50 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF051424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 15 04:12:16 2024
Response via : Initial Calibration

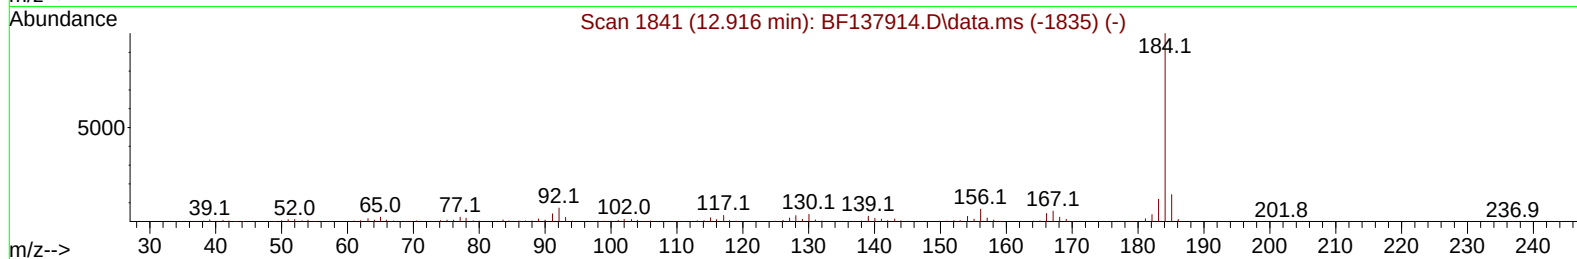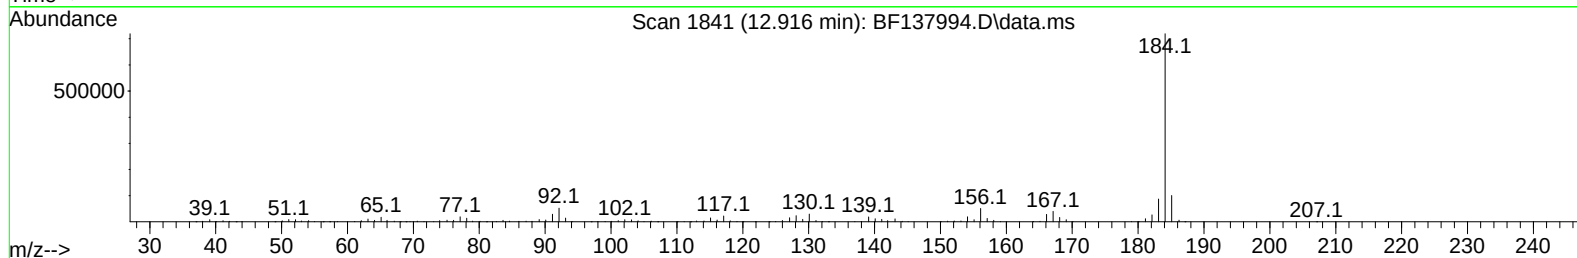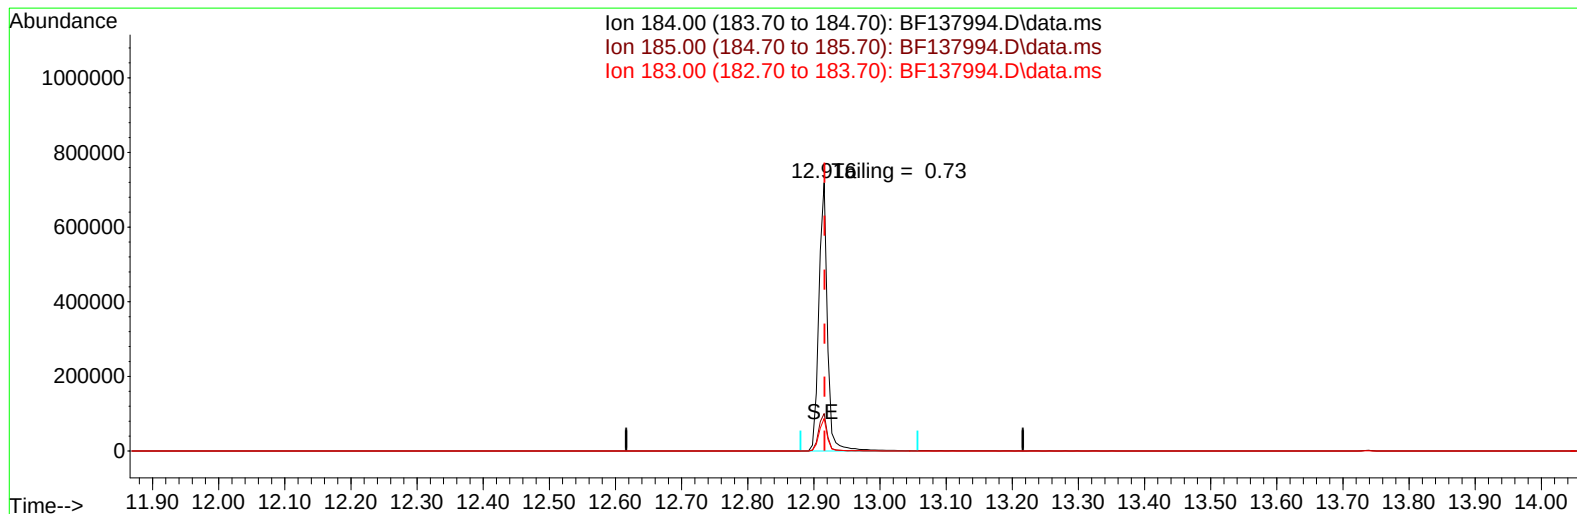

TIC: BF137994.D\data.ms

(77) Benzidine

12.916min (-0.000) 0.00 ng

response **653094**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	13.97
183.00	11.90	12.14
0.00	0.00	0.00