

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052224\
 Data File : BF138007.D
 Acq On : 22 May 2024 16:21
 Operator : CG\JU
 Sample : P2563-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OILY-WATER

Quant Time: May 22 17:03:51 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF051424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 15 04:12:16 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.034	152	129085	20.000	ng	-0.01
21) Naphthalene-d8	8.316	136	491378	20.000	ng	-0.01
39) Acenaphthene-d10	10.081	164	264791	20.000	ng	0.00
64) Phenanthrene-d10	11.575	188	457271	20.000	ng	0.00
76) Chrysene-d12	14.222	240	264047	20.000	ng	0.00
86) Perylene-d12	15.786	264	111814	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.651	112	381218	50.165	ng	-0.01
7) Phenol-d6	6.640	99	299113	31.953	ng	-0.02
23) Nitrobenzene-d5	7.593	82	551811	66.088	ng	-0.02
42) 2,4,6-Tribromophenol	10.875	330	330264	123.700	ng	0.00
45) 2-Fluorobiphenyl	9.392	172	1229019	71.497	ng	0.00
79) Terphenyl-d14	13.163	244	1297239	72.406	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052224\
Data File : BF138007.D
Acq On : 22 May 2024 16:21
Operator : CG\JU
Sample : P2563-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OILY-WATER

Quant Time: May 22 17:03:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF051424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 15 04:12:16 2024
Response via : Initial Calibration




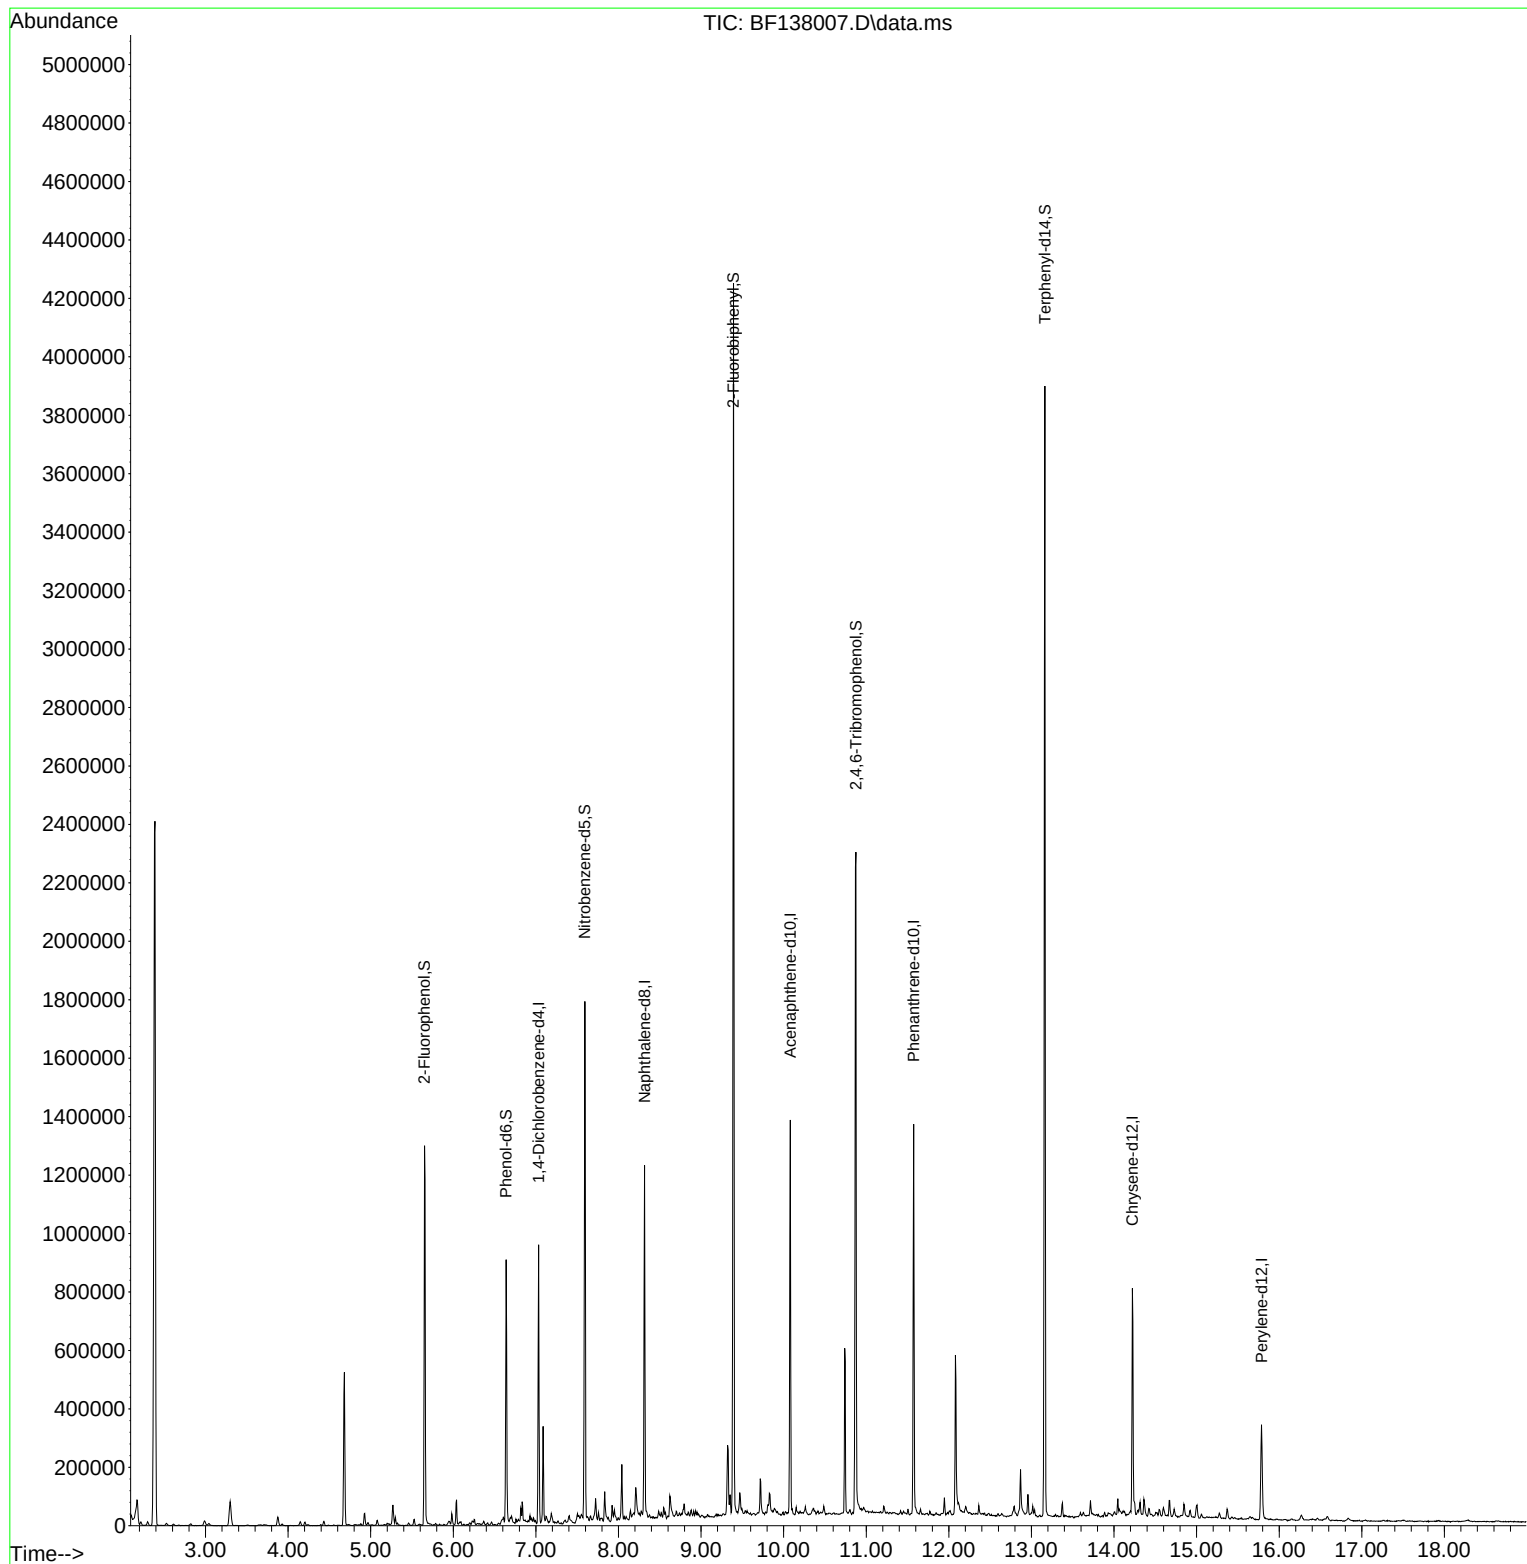


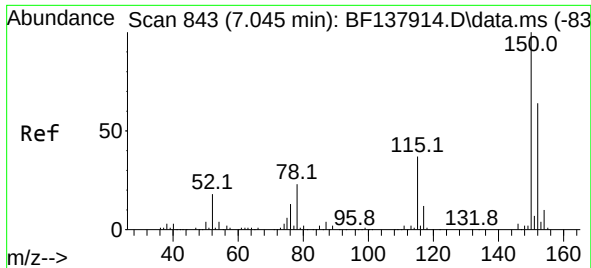

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.034 min Scan# 84
Delta R.T. -0.011 min
Lab File: BF138007.D
Acq: 22 May 2024 16:21




Instrument :
BNA_F
ClientSampleId :
OILY-WATER


Tgt Ion:152 Resp: 129085
Ion Ratio Lower Upper
152 100
150 154.2 125.7 188.5
115 59.8 47.0 70.6

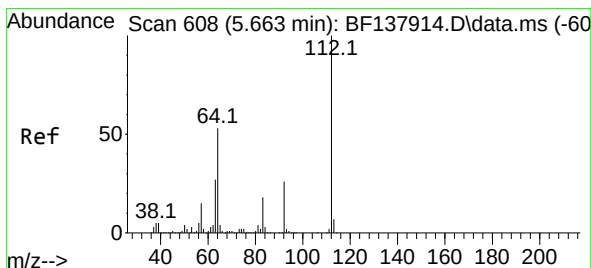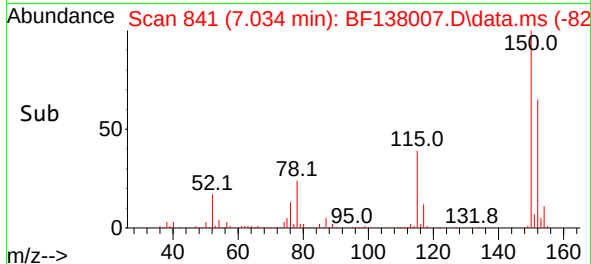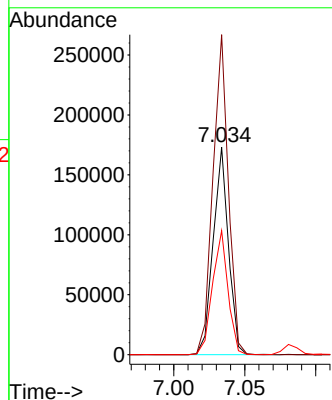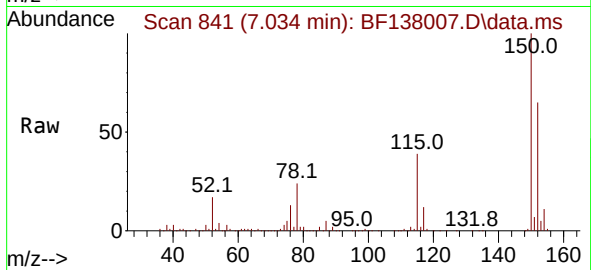

#5
2-Fluorophenol
Concen: 50.165 ng
RT: 5.651 min Scan# 606
Delta R.T. -0.012 min
Lab File: BF138007.D
Acq: 22 May 2024 16:21

Tgt Ion:112 Resp: 381218
Ion Ratio Lower Upper
112 100
64 56.0 42.4 63.6
63 27.6 21.4 32.2


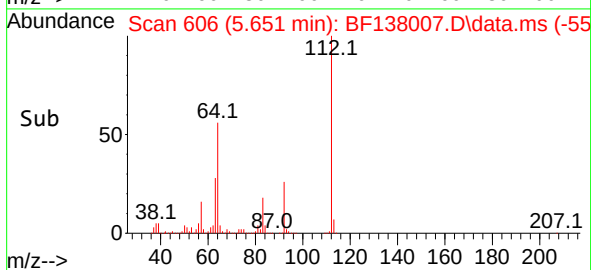
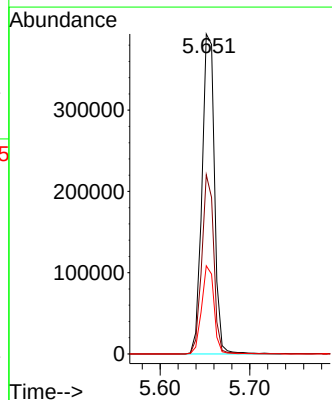
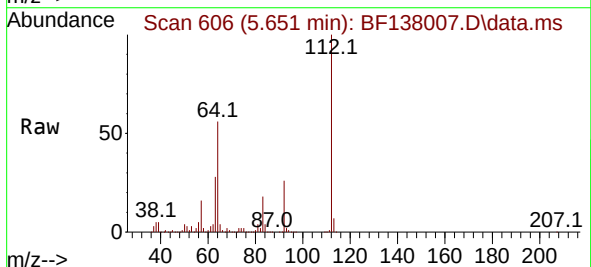


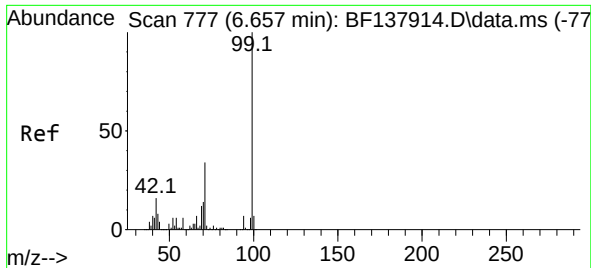

#7
Phenol-d6
Concen: 31.953 ng
RT: 6.640 min Scan# 71
Delta R.T. -0.017 min
Lab File: BF138007.D
Acq: 22 May 2024 16:21




Instrument :
BNA_F
ClientSampleId :
OILY-WATER


Tgt Ion: 99 Resp: 299113
Ion Ratio Lower Upper
99 100
42 15.5 12.6 18.8
71 33.1 27.1 40.7

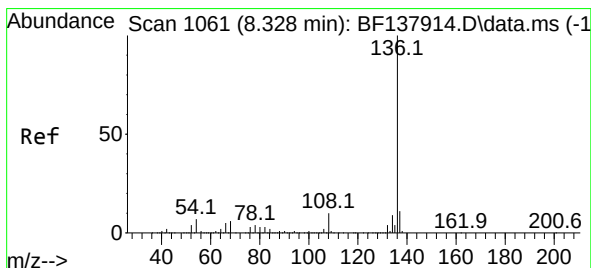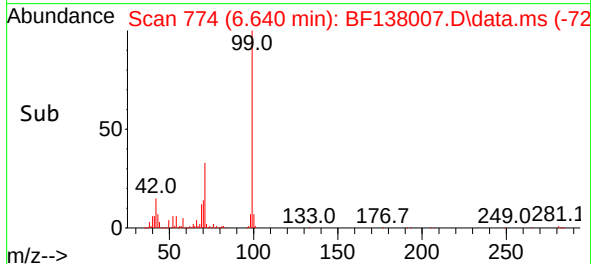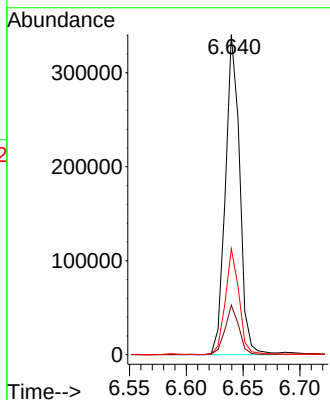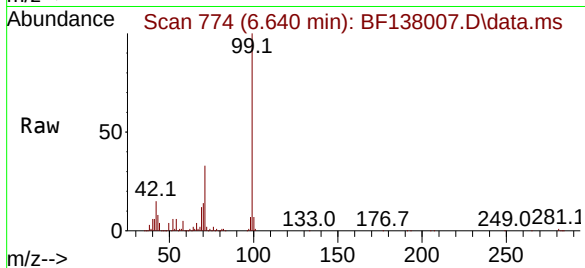

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.316 min Scan# 1059
Delta R.T. -0.012 min
Lab File: BF138007.D
Acq: 22 May 2024 16:21

Tgt Ion: 136 Resp: 491378
Ion Ratio Lower Upper
136 100
137 10.6 8.7 13.1
54 6.6 5.4 8.2
68 5.4 4.6 7.0


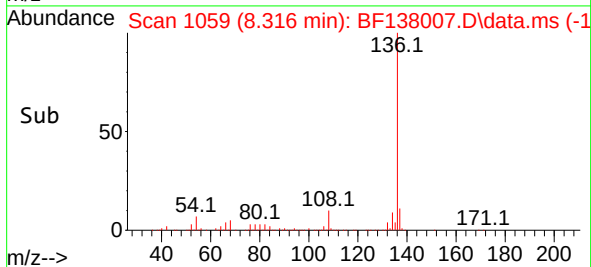
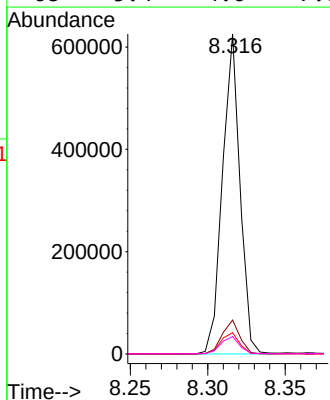
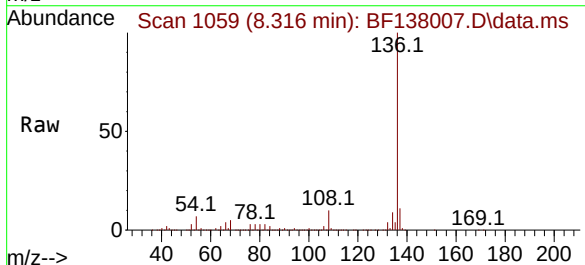


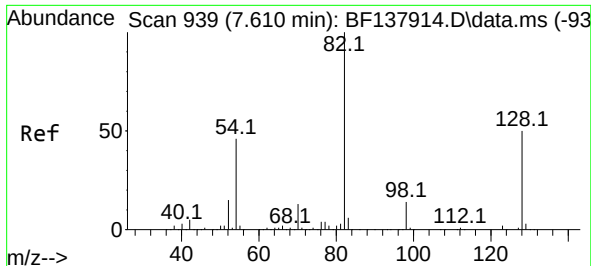

#23
Nitrobenzene-d5
Concen: 66.088 ng
RT: 7.593 min Scan# 91
Delta R.T. -0.017 min
Lab File: BF138007.D
Acq: 22 May 2024 16:21




Instrument :
BNA_F
ClientSampleId :
OILY-WATER


Tgt Ion: 82 Resp: 551811
Ion Ratio Lower Upper
82 100
128 47.8 40.3 60.5
54 47.7 36.8 55.2

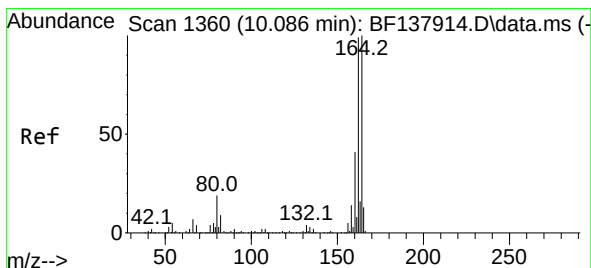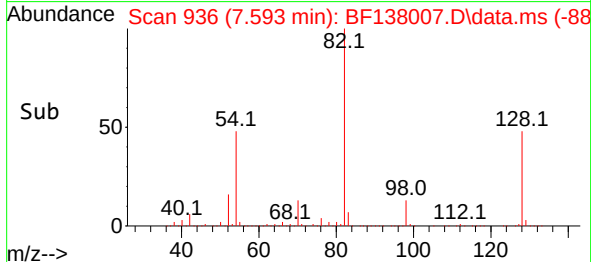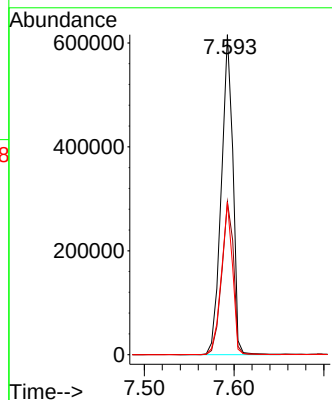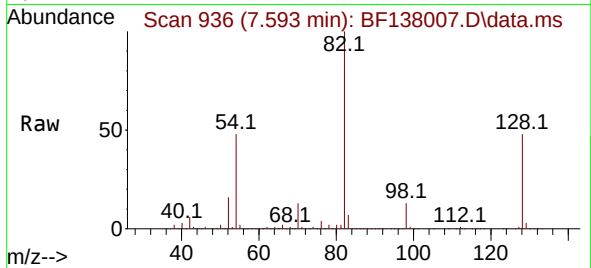

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 10.081 min Scan# 1359
Delta R.T. -0.005 min
Lab File: BF138007.D
Acq: 22 May 2024 16:21

Tgt Ion:164 Resp: 264791
Ion Ratio Lower Upper
164 100
162 98.8 79.4 119.2
160 43.0 33.1 49.7


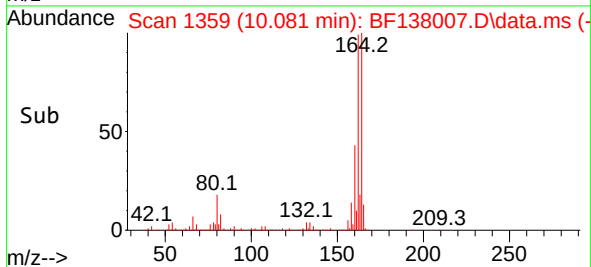
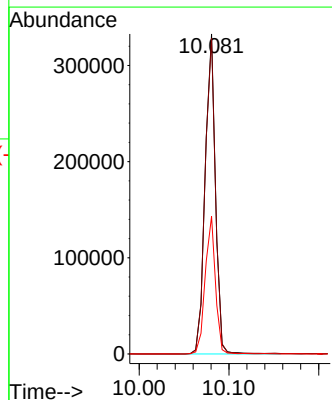
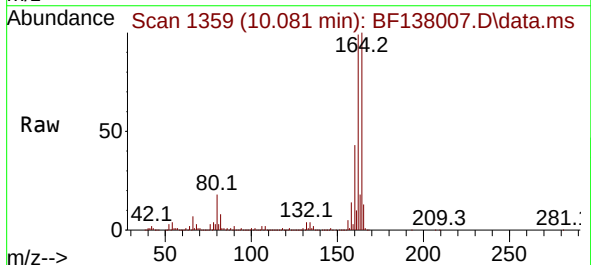


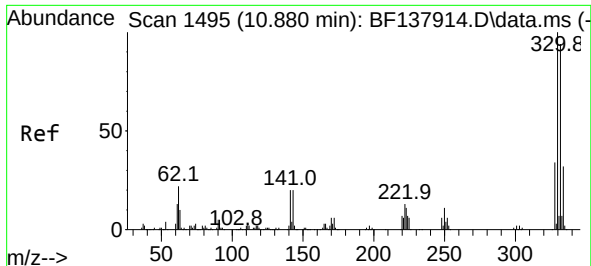

#42
2,4,6-Tribromophenol
Concen: 123.700 ng
RT: 10.875 min Scan# 1494
Delta R.T. -0.006 min
Lab File: BF138007.D
Acq: 22 May 2024 16:21




Instrument :
BNA_F
ClientSampleId :
OILY-WATER


Tgt Ion:330 Resp: 330264
Ion Ratio Lower Upper
330 100
332 97.5 75.8 113.8
141 28.8 23.8 35.6

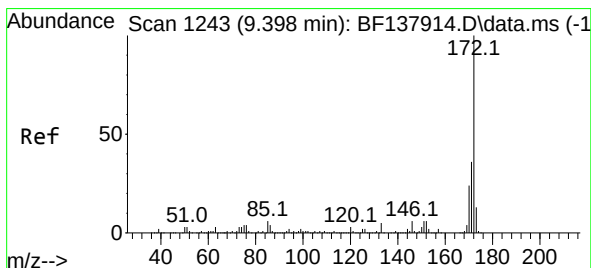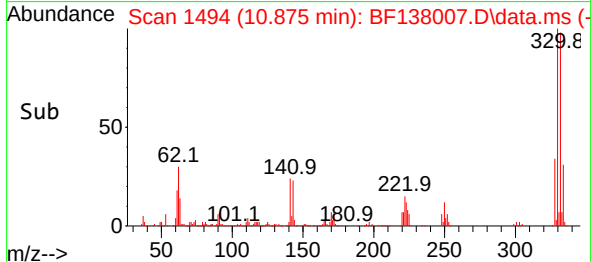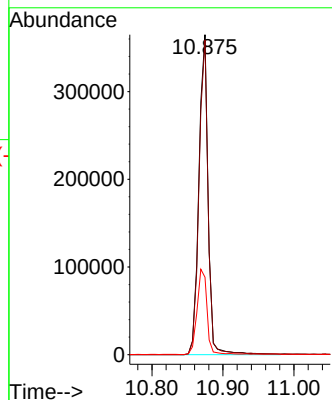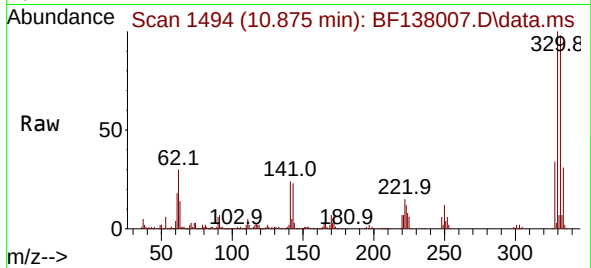

#45
2-Fluorobiphenyl
Concen: 71.497 ng
RT: 9.392 min Scan# 1242
Delta R.T. -0.006 min
Lab File: BF138007.D
Acq: 22 May 2024 16:21

Tgt Ion:172 Resp: 1229019
Ion Ratio Lower Upper
172 100
171 35.8 28.9 43.3
170 23.2 18.9 28.3


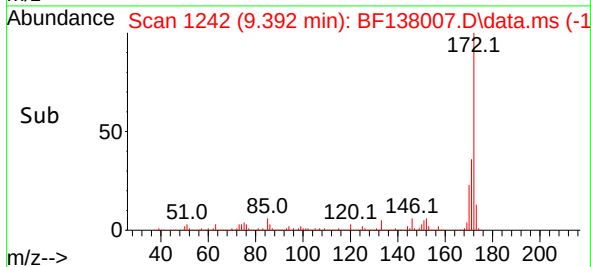
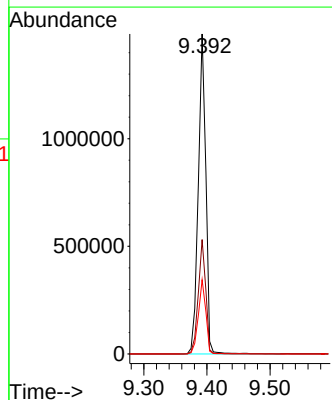
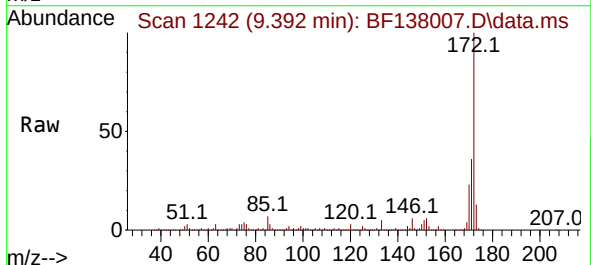


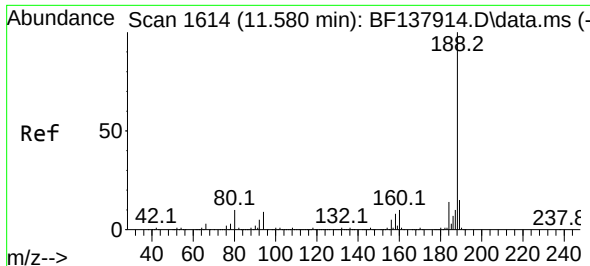

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.575 min Scan# 1
Delta R.T. -0.006 min
Lab File: BF138007.D
Acq: 22 May 2024 16:21




Instrument :
BNA_F
ClientSampleId :
OILY-WATER


Tgt Ion:188 Resp: 457271
Ion Ratio Lower Upper
188 100
94 9.3 7.0 10.4
80 9.5 7.7 11.5

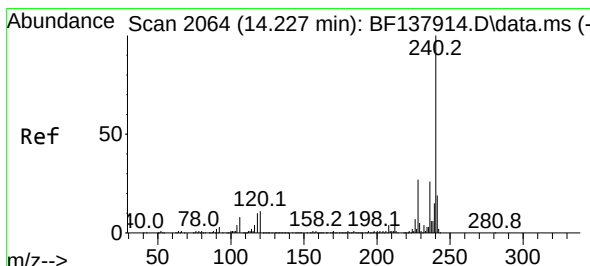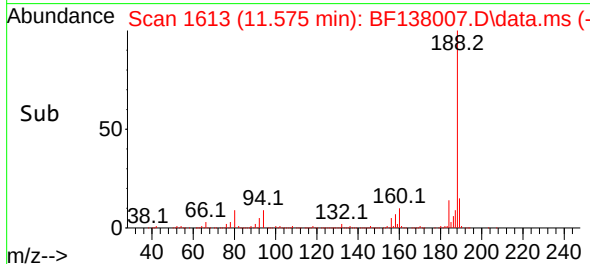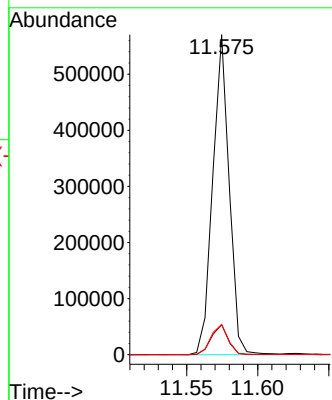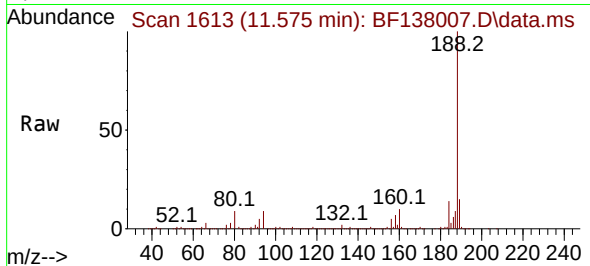

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.222 min Scan# 2063
Delta R.T. -0.006 min
Lab File: BF138007.D
Acq: 22 May 2024 16:21

Tgt Ion:240 Resp: 264047
Ion Ratio Lower Upper
240 100
120 12.3 8.9 13.3
236 24.8 21.0 31.4

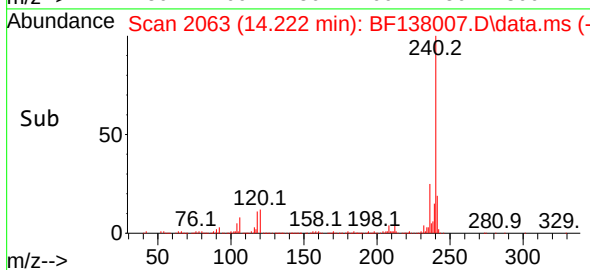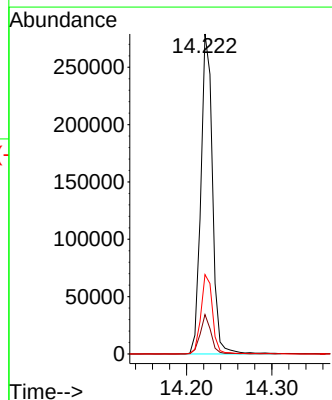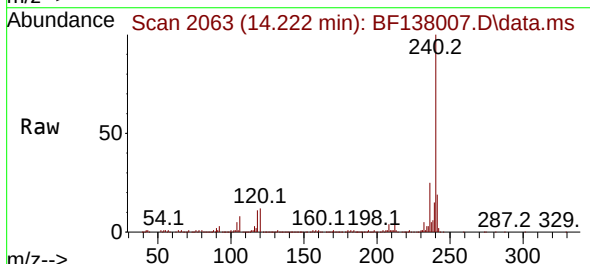




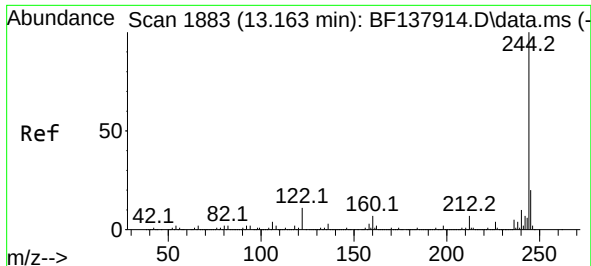


#79
 Terphenyl-d14
 Concen: 72.406 ng
 RT: 13.163 min Scan# 1883
 Delta R.T. 0.000 min
 Lab File: BF138007.D
 Acq: 22 May 2024 16:21

Instrument :
 BNA_F
 ClientSampleId :
 OILY-WATER

Tgt Ion:244 Resp: 1297239

Ion	Ratio	Lower	Upper
244	100		
212	6.6	5.6	8.4
122	9.8	8.8	13.2

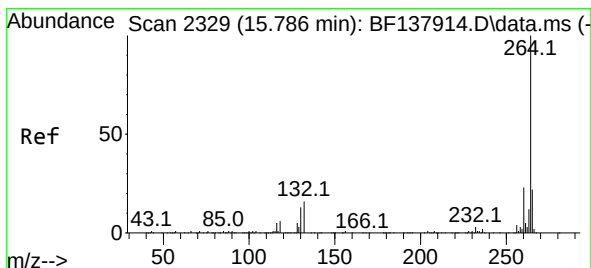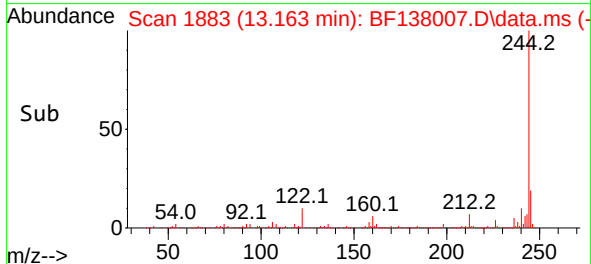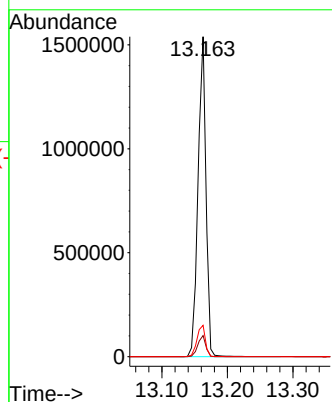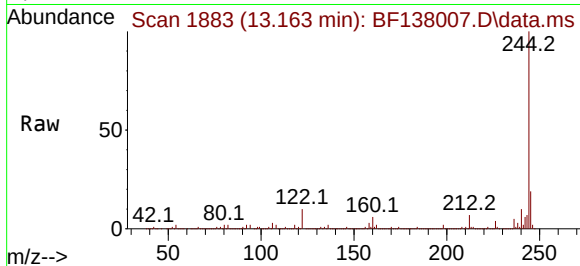

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.786 min Scan# 2329
 Delta R.T. 0.000 min
 Lab File: BF138007.D
 Acq: 22 May 2024 16:21

Tgt Ion:264 Resp: 111814

Ion	Ratio	Lower	Upper
264	100		
260	25.0	18.3	27.5
265	21.5	17.6	26.4

