


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052224\
Data File : BF137994.D
Acq On : 22 May 2024 09:17
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF051424.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed May 15 04:12:16 2024

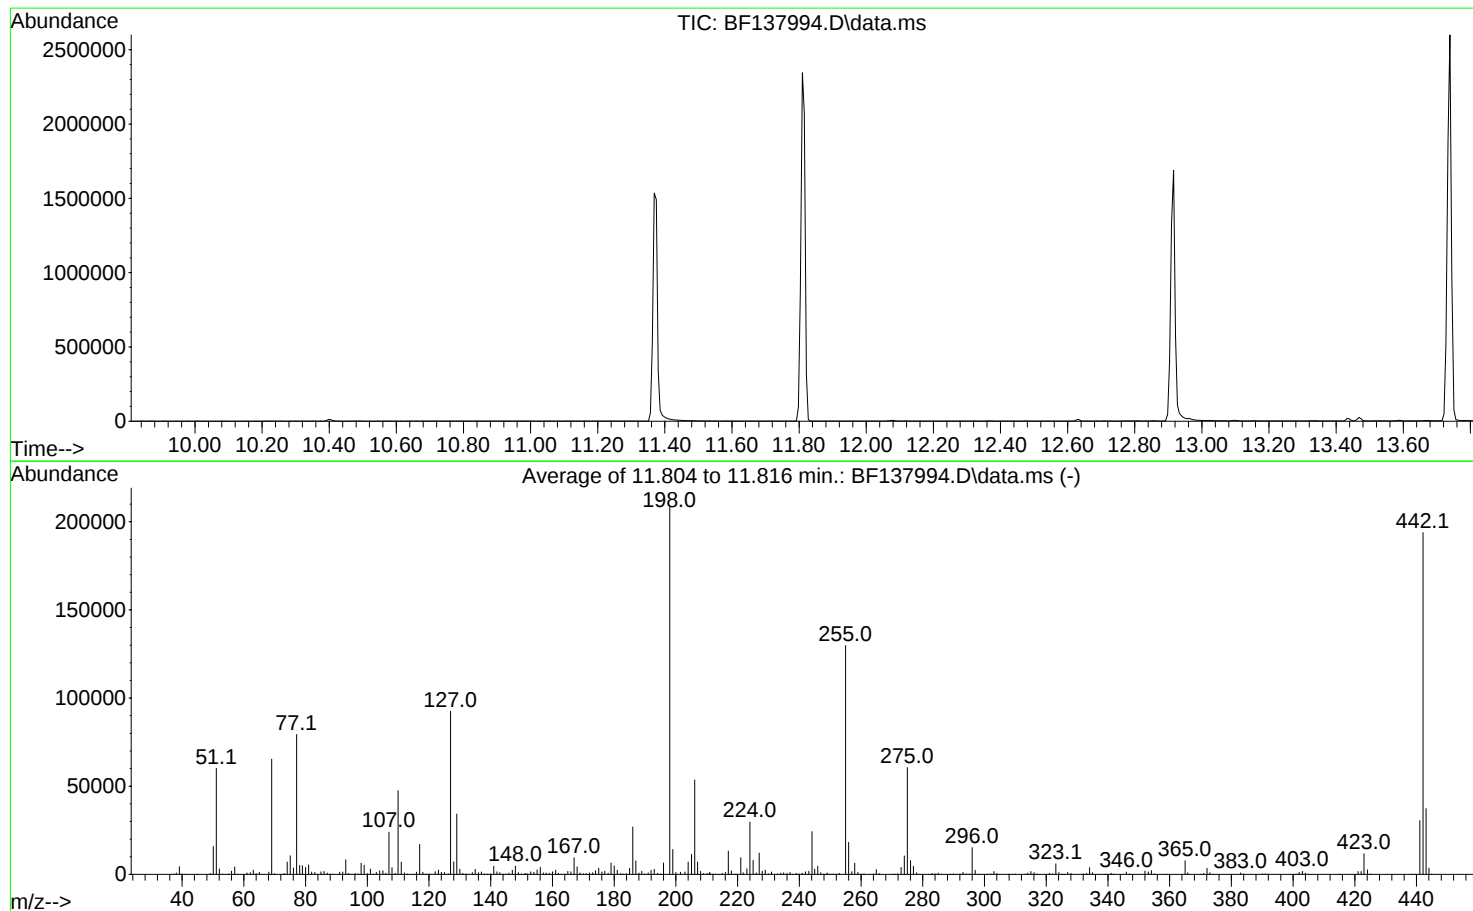

AutoFind: Scans 1652, 1653, 1654; Background Corrected with Scan 1647

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.8	60053	PASS
68	69	0.00	2	1.9	1267	PASS
69	198	0.00	100	31.3	65392	PASS
70	69	0.00	2	0.5	328	PASS
127	198	10	80	44.3	92472	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	208659	PASS
199	198	5	9	6.8	14086	PASS
275	198	10	60	29.0	60579	PASS
365	198	1	100	3.7	7720	PASS
441	198	0.01	100	14.6	30527	PASS
442	442	50	100	100.0	193832	PASS
443	442	15	24	19.3	37315	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/22/2024	BNA_F	<u>BF137994.D</u>
Compound Name	Response	Retention Time
DDT	449137	13.739
DDD	7779	13.468
DDE	968	13.098
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8747	457884	1.91

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052224\
Data File : BF137994.D
Acq On : 22 May 2024 09:17
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 22 09:37:50 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF051424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 15 04:12:16 2024
Response via : Initial Calibration

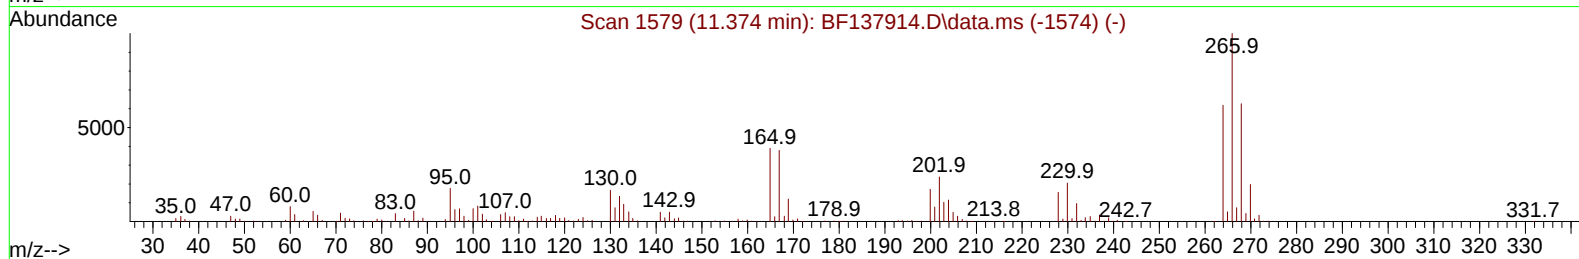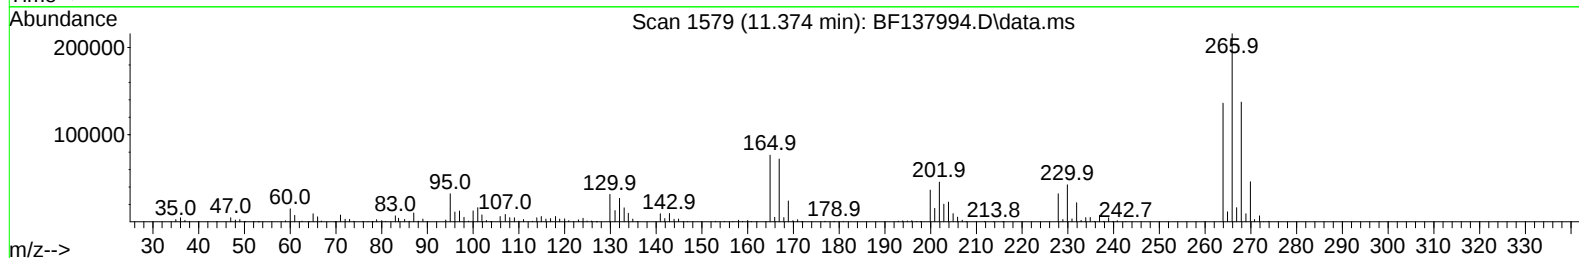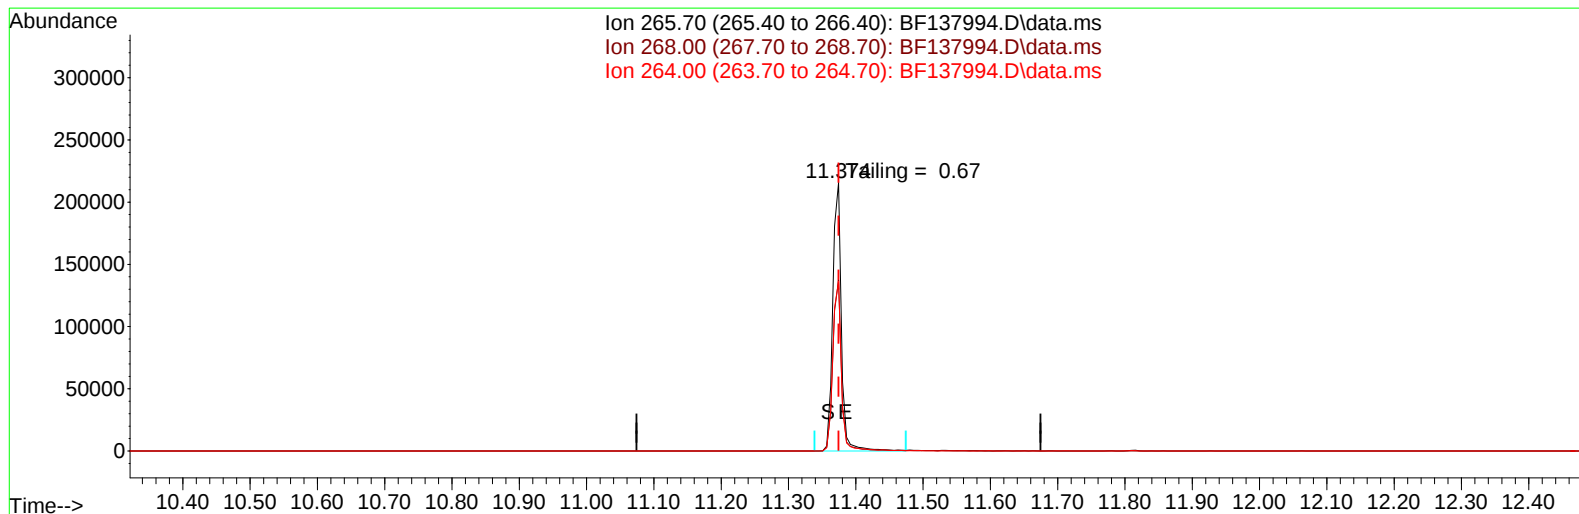

TIC: BF137994.D\data.ms

(70) Pentachlorophenol (C)

11.374min (0.000) 29246.02 ng




response 192861

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	63.71
264.00	61.80	63.12
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052224\
Data File : BF137994.D
Acq On : 22 May 2024 09:17
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 22 09:37:50 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF051424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 15 04:12:16 2024
Response via : Initial Calibration

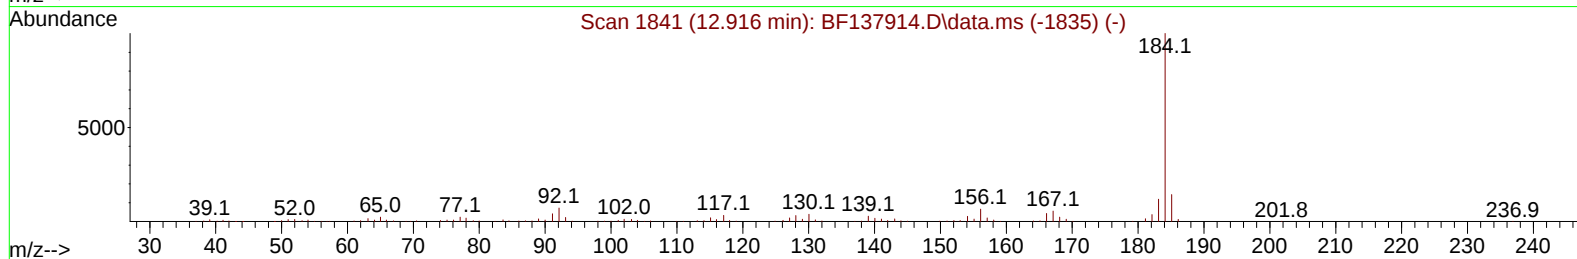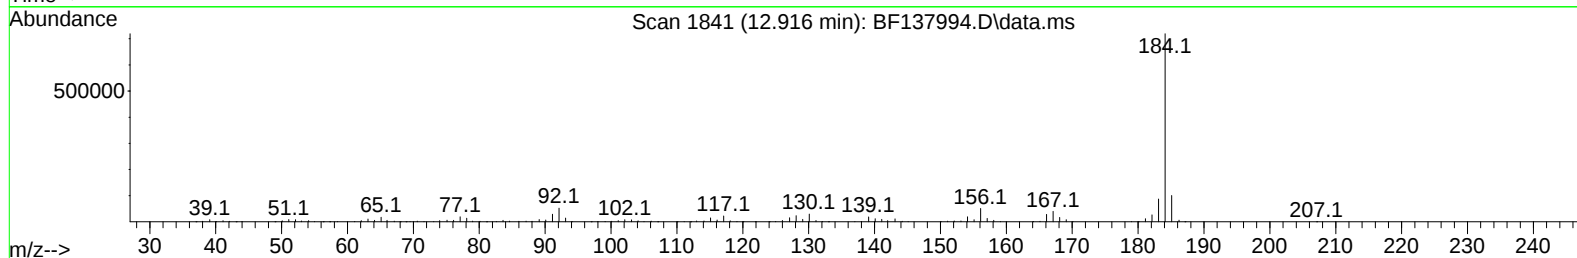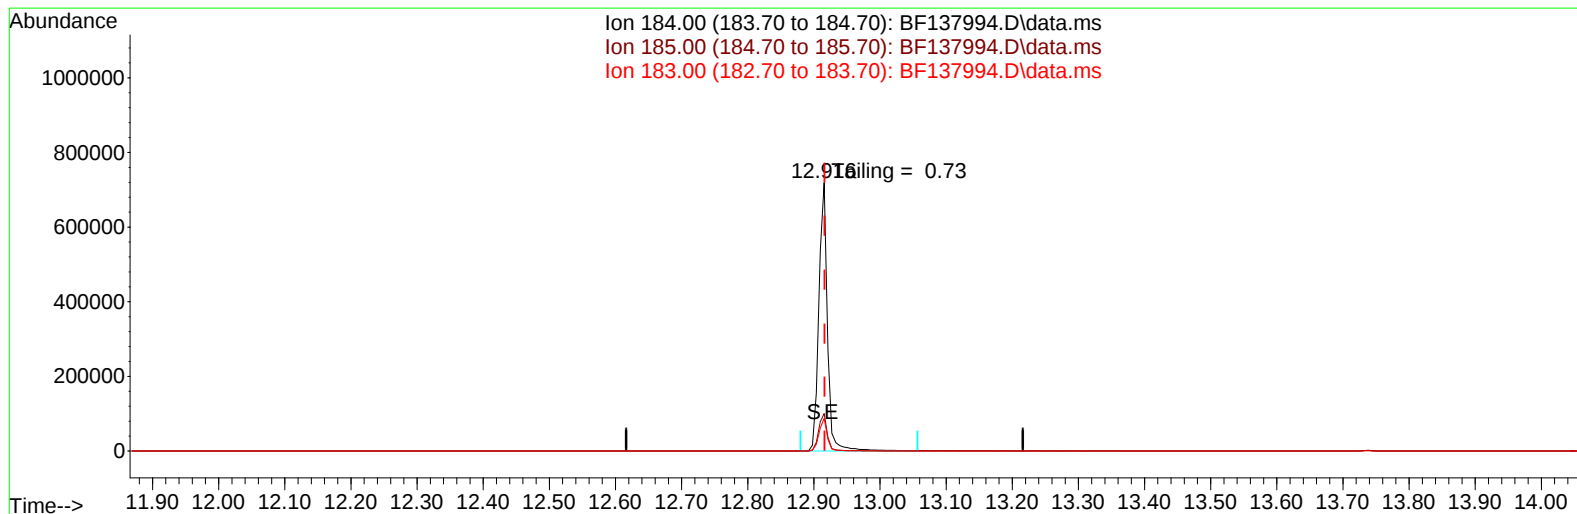

TIC: BF137994.D\data.ms

(77) Benzidine

12.916min (-0.000) 0.00 ng

response 653094

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	13.97
183.00	11.90	12.14
0.00	0.00	0.00