


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF052319\
 Data File : BF114520.D
 Acq On : 23 May 2019 10:22
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 24 07:23:33 2019

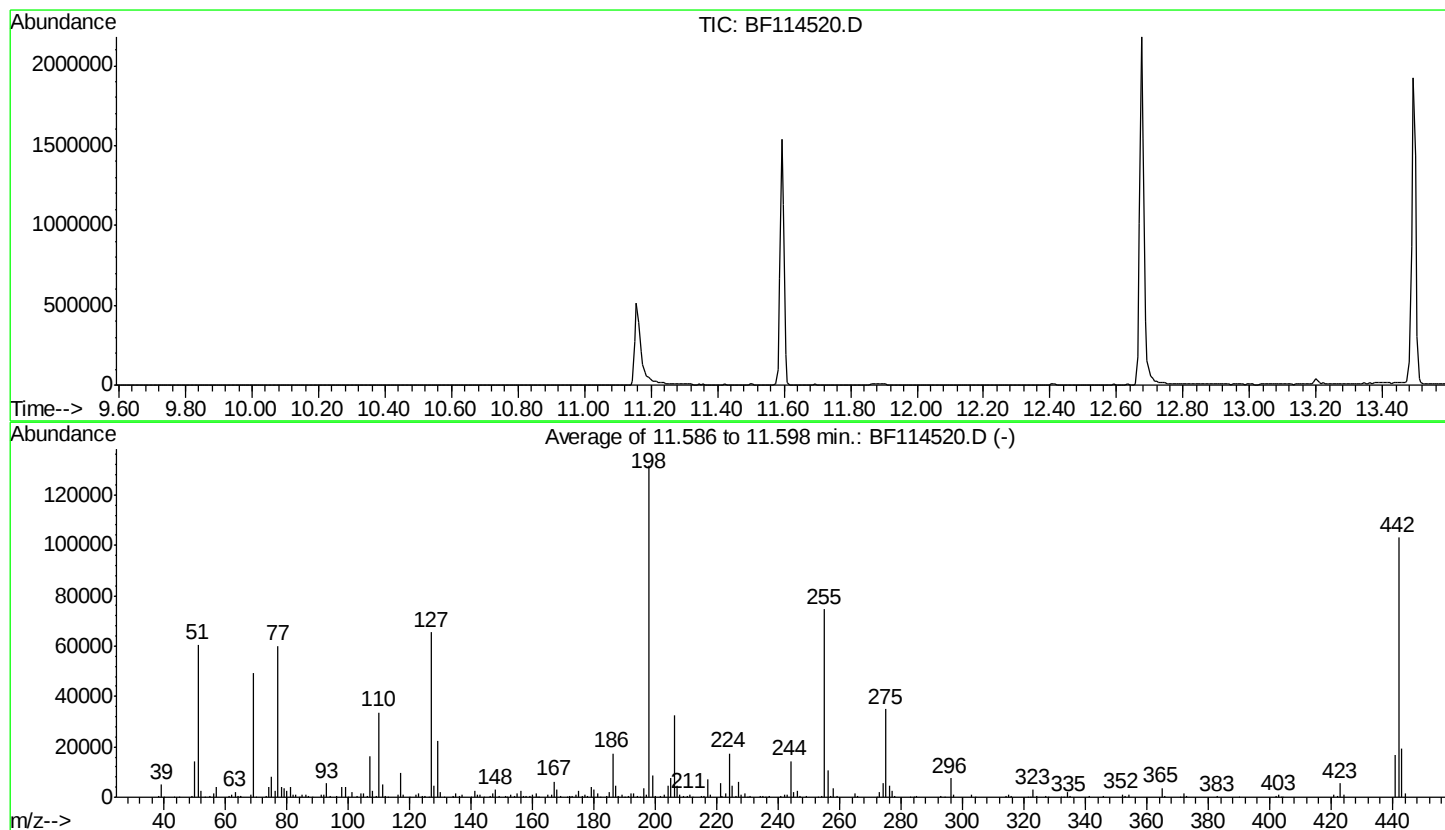

AutoFind: Scans 1615, 1616, 1617; Background Corrected with Scan 1610

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.1	60693	PASS
68	69	0.00	2	1.6	809	PASS
69	198	0.00	100	37.6	49448	PASS
70	69	0.00	2	0.3	167	PASS
127	198	10	80	49.7	65418	PASS
197	198	0.00	2	0.7	967	PASS
198	198	100	100	100.0	131602	PASS
199	198	5	9	6.4	8486	PASS
275	198	10	60	26.5	34816	PASS
365	198	1	100	2.8	3702	PASS
441	198	0.01	100	12.9	16911	PASS
442	198	50	100	78.2	102933	PASS
443	442	15	24	18.9	19438	PASS