


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF052319\
 Data File : BF114532.D
 Acq On : 23 May 2019 18:51
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 24 07:23:33 2019

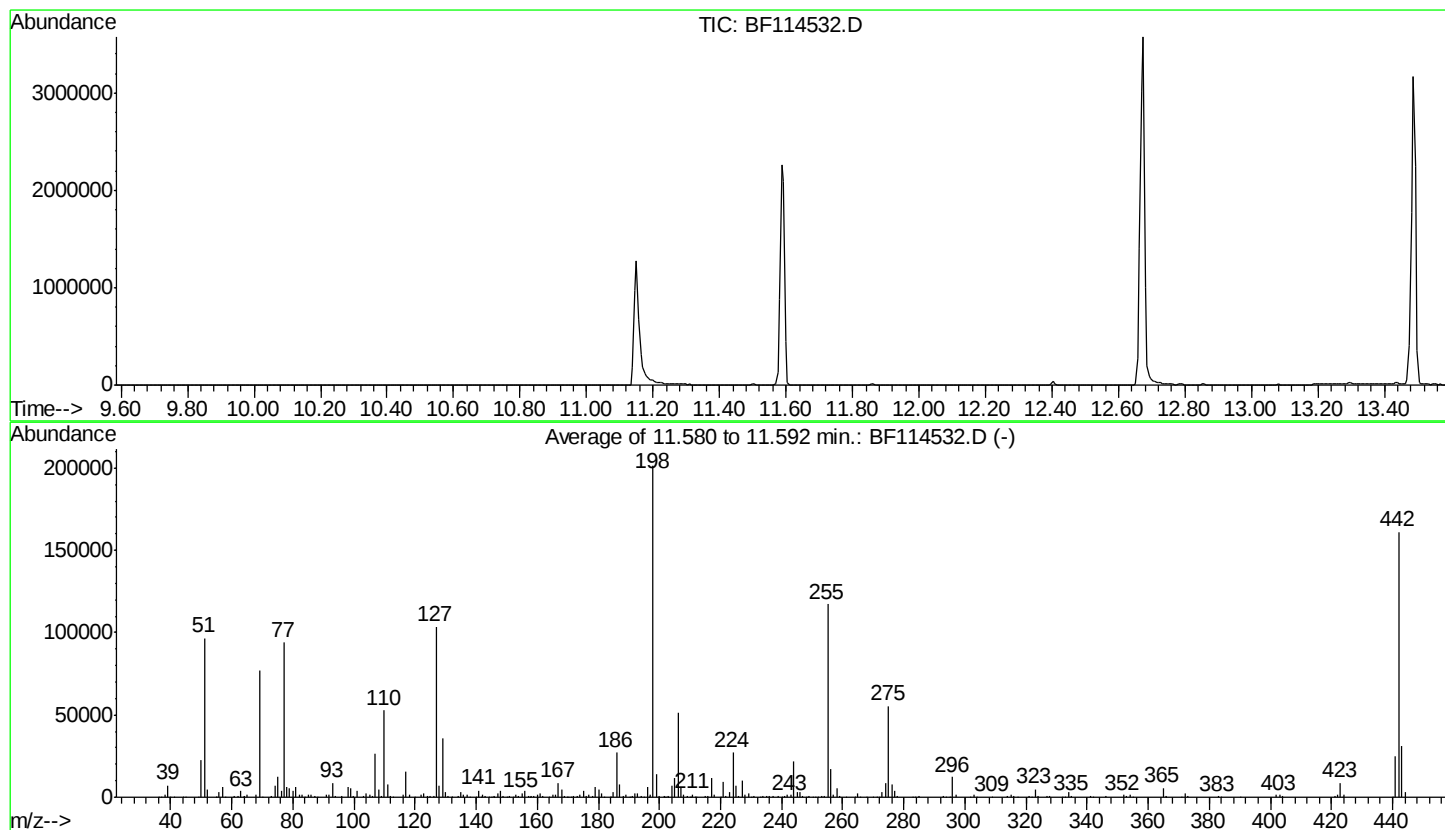

AutoFind: Scans 1614, 1615, 1616; Background Corrected with Scan 1609

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.0	96757	PASS
68	69	0.00	2	1.9	1448	PASS
69	198	0.00	100	38.1	76848	PASS
70	69	0.00	2	0.5	386	PASS
127	198	10	80	51.4	103616	PASS
197	198	0.00	2	0.7	1392	PASS
198	198	100	100	100.0	201461	PASS
199	198	5	9	6.9	13857	PASS
275	198	10	60	27.5	55437	PASS
365	198	1	100	2.8	5639	PASS
441	198	0.01	100	12.5	25212	PASS
442	198	50	100	80.0	161133	PASS
443	442	15	24	19.4	31224	PASS